


Data Path : Z:\HPCHEM1\BNA_F\Data\BF062316\
 Data File : BF088314.D
 Acq On : 24 Jun 2016 4:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 14:55:14 2016

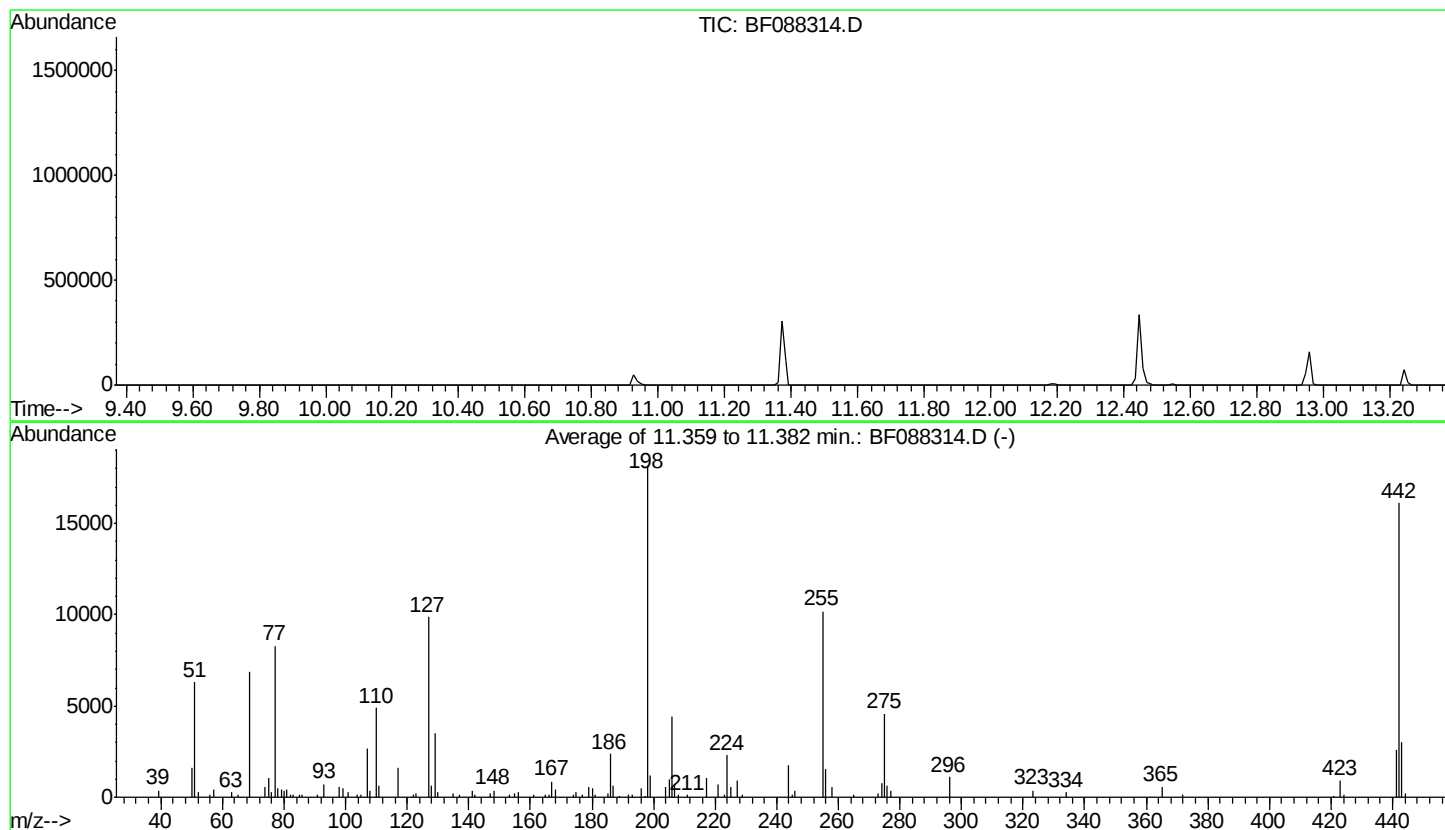

AutoFind: Scans 855, 856, 857; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	6290	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.8	6867	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	9867	PASS
197	198	0.00	2	0.6	100	PASS
198	198	100	100	100.0	18173	PASS
199	198	5	9	6.4	1160	PASS
275	198	10	60	25.2	4584	PASS
365	198	1	100	3.2	573	PASS
441	442	0.01	24	16.2	2606	PASS
442	198	50	100	88.7	16126	PASS
443	442	15	24	18.8	3038	PASS