

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062317\
 Data File : BF096159.D
 Acq On : 23 Jun 2017 14:56
 Operator : SJ/MA
 Sample : PB100046BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB100046BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.540	7	9	46	rVB	712149	1467673	65.96%	8.648%
2	4.446	499	503	522	rBV	61521	193917	8.71%	1.143%
3	5.151	619	623	654	rBV	637370	1509880	67.85%	8.896%
4	6.834	905	909	919	rBV	778280	1321994	59.41%	7.789%
5	6.916	919	923	939	rVB	1049029	1853944	83.32%	10.924%
6	7.263	978	982	1004	rVB	214099	327247	14.71%	1.928%
7	7.492	1016	1021	1049	rBV	899480	1301381	58.48%	7.668%
8	8.181	1134	1138	1176	rBV	562084	953848	42.87%	5.620%
9	9.292	1323	1327	1350	rBV	287726	451525	20.29%	2.660%
10	11.069	1623	1629	1649	rBV	1395711	2023671	90.94%	11.924%
11	12.110	1802	1806	1825	rBV2	364674	527619	23.71%	3.109%
12	13.410	2022	2027	2053	rBV	730724	1150441	51.70%	6.779%
13	14.510	2209	2214	2237	rBV	347802	554993	24.94%	3.270%
14	16.904	2614	2621	2624	rBV	1691876	2225207	100.00%	13.111%
15	18.245	2845	2849	2866	rBV	384980	587052	26.38%	3.459%
16	19.921	3130	3134	3147	rBV	303339	498398	22.40%	2.937%
17	20.350	3201	3207	3212	rBV4	16372	23076	1.04%	0.136%


Sum of corrected areas: 16971866

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062317\
Data File : BF096159.D
Acq On : 23 Jun 2017 14:56
Operator : SJ/MA
Sample : PB100046BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100046BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

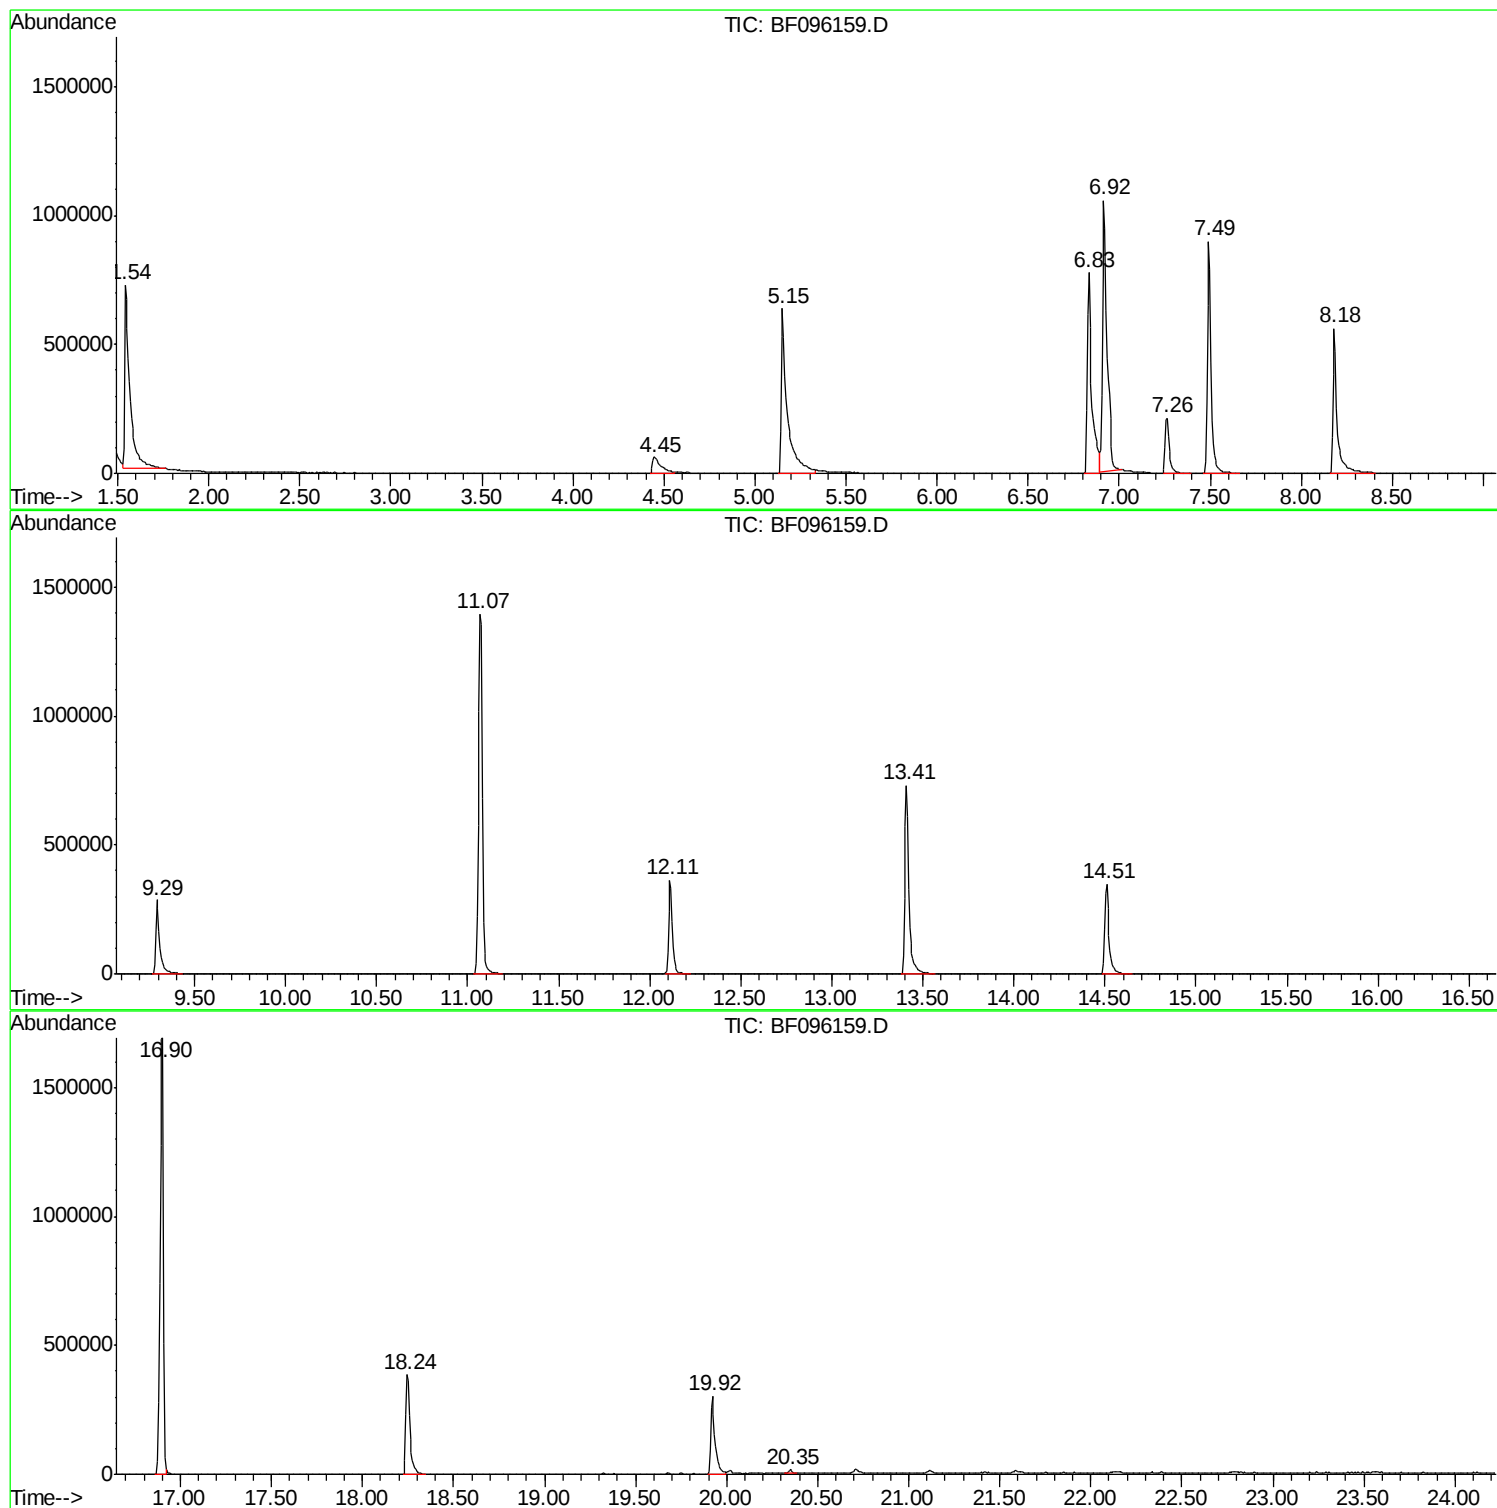

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062317\
Data File : BF096159.D
Acq On : 23 Jun 2017 14:56
Operator : SJ/MA
Sample : PB100046BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100046BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.45	11.85 ng	193917	1,4-Dichlorobenzene-d4	7.26

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			3-Hexanol	102	C6H14O	000623-37-0	28
4			Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	25
5			5-Hexen-2-one	98	C6H10O	000109-49-9	9

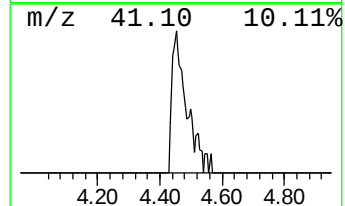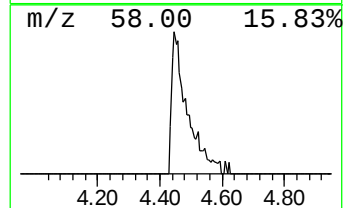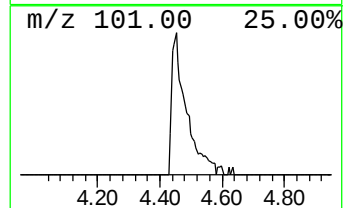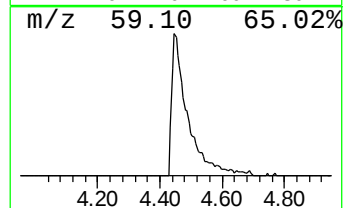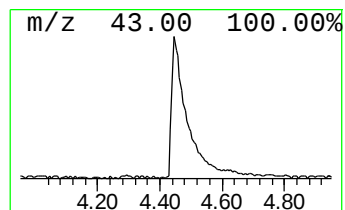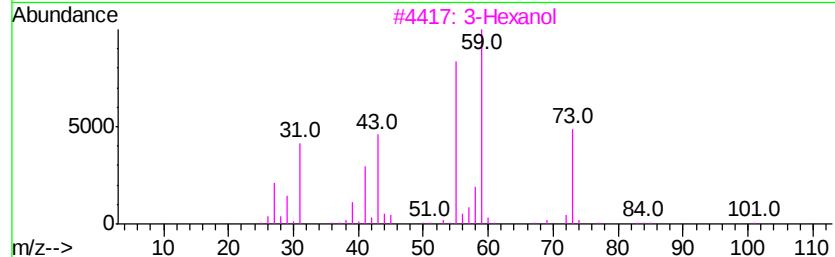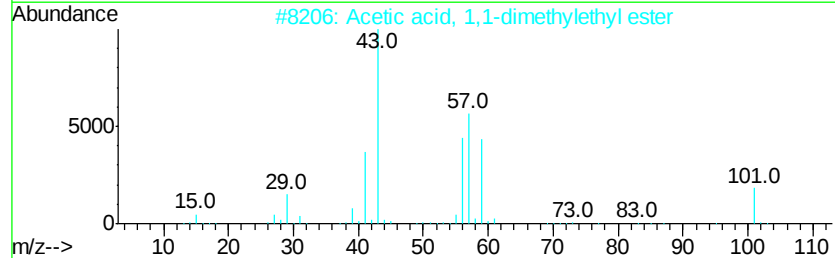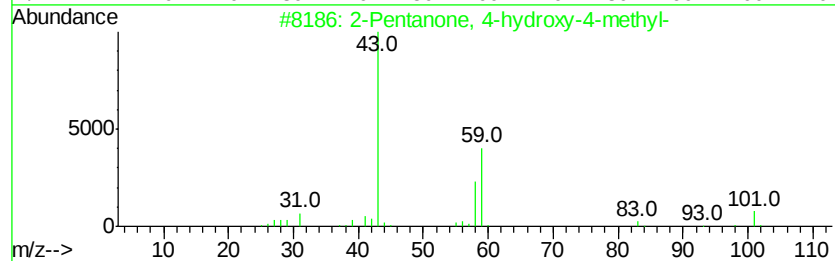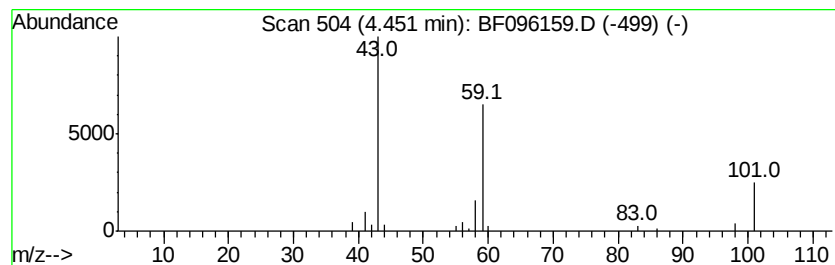

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062317\
Data File : BF096159.D
Acq On : 23 Jun 2017 14:56
Operator : SJ/MA
Sample : PB100046BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100046BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown6.92 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.92	113.31 ng	1853940	1,4-Dichlorobenzene-d4	7.26

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	38
2	(E)-3-Chloro-2-methyl-2-pentenal			132	C6H9ClO	031357-76-3	17
3	1H-Indazole, 7-methyl-			132	C8H8N2	1000316-00-7	10
4	4-Chloro-6-fluoro-pyrimidine			132	C4H2ClFN2	051422-01-6	9
5	5-Fluoro-2-chloropyrimidine			132	C4H2ClFN2	062802-42-0	9

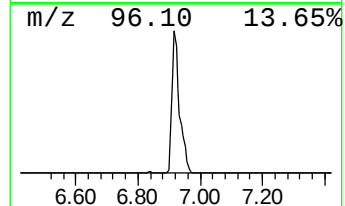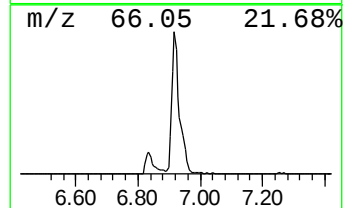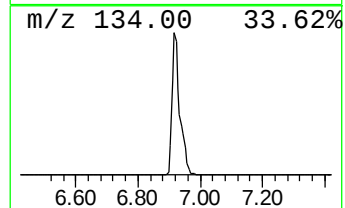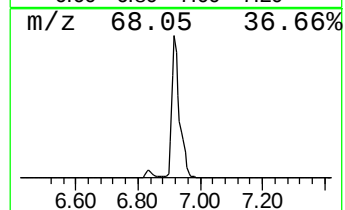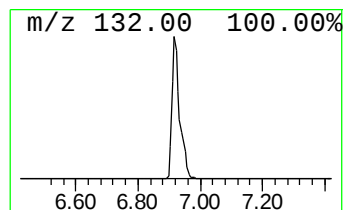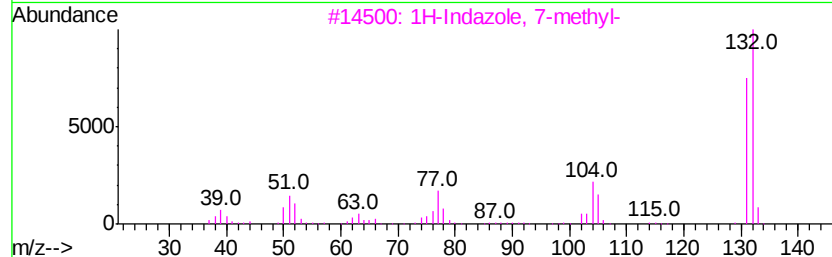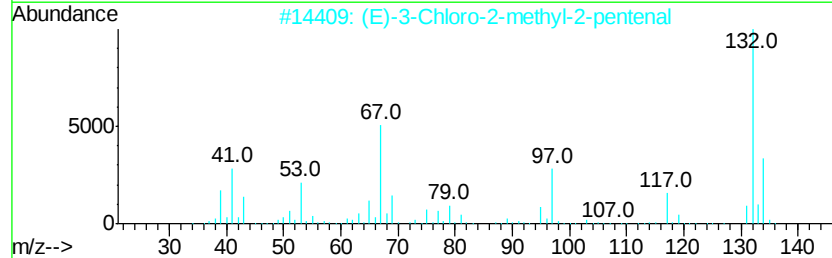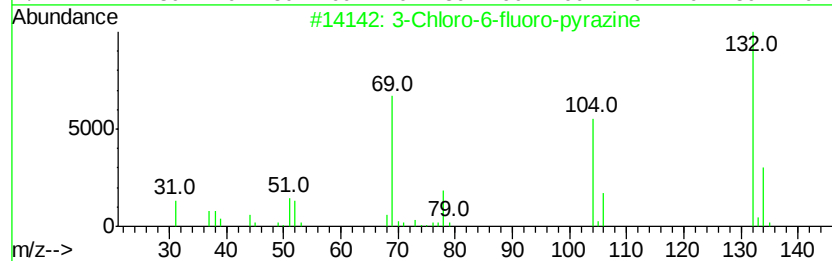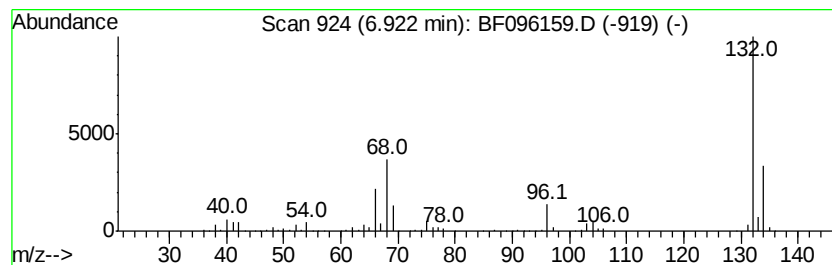

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062317\
Data File : BF096159.D
Acq On : 23 Jun 2017 14:56
Operator : SJ/MA
Sample : PB100046BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100046BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.45	11.9	ng	193917	1	7.26	327247	20.0
unknown6.92	6.92	113.3	ng	1853940	1	7.26	327247	20.0