


Data Path : Z:\HPCHEM1\BNA F\Data\BF062317\
 Data File : BF096156.D
 Acq On : 23 Jun 2017 13:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

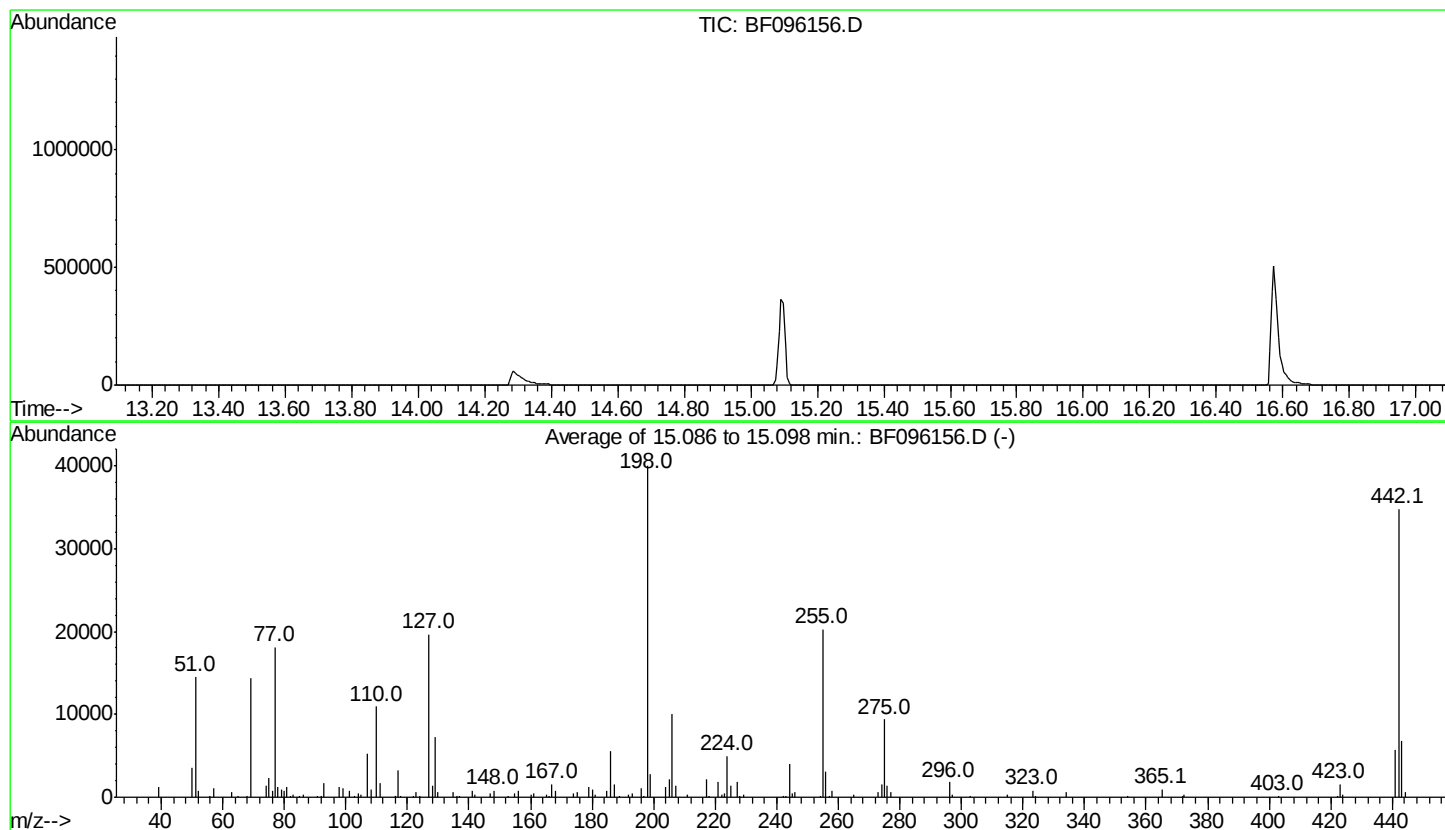

AutoFind: Scans 2312, 2313, 2314; Background Corrected with Scan 2306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	14600	PASS
68	69	0.00	2	0.7	105	PASS
69	198	0.00	100	36.1	14430	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	19635	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40010	PASS
199	198	5	9	6.9	2752	PASS
275	198	10	60	23.4	9382	PASS
365	198	1	100	2.4	947	PASS
441	442	0.01	24	16.5	5727	PASS
442	198	50	100	86.9	34781	PASS
443	442	15	24	19.5	6771	PASS