
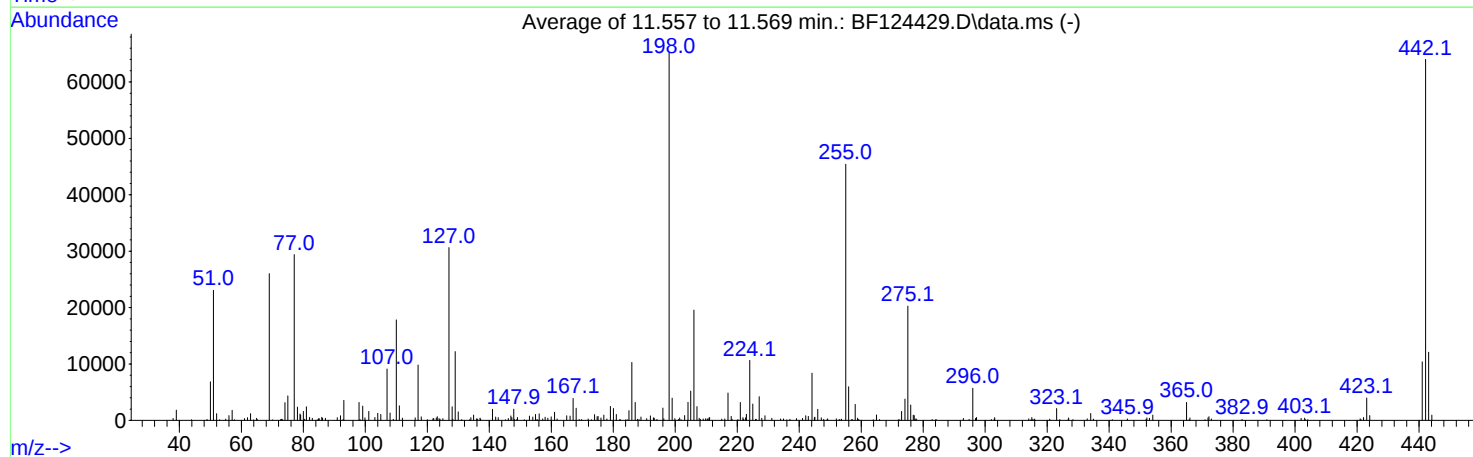


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062321\
 Data File : BF124429.D
 Acq On : 23 Jun 2021 12:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 23 18:48:27 2021

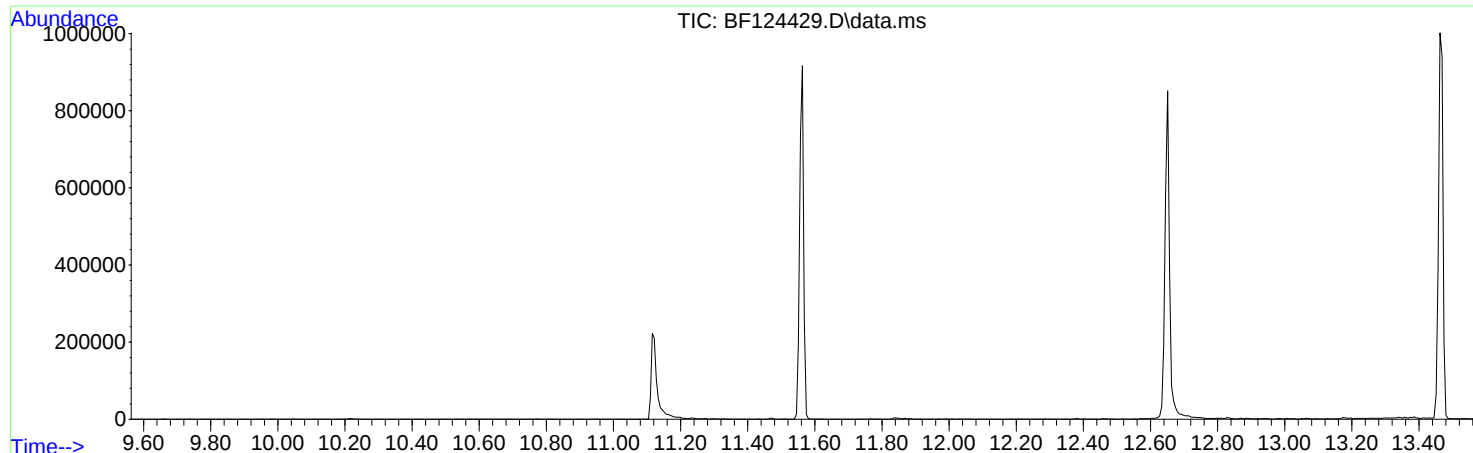




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	23078	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.9	26021	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	47.0	30651	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65235	PASS
199	198	5	9	6.0	3938	PASS
275	198	10	60	31.0	20254	PASS
365	198	1	100	4.9	3195	PASS
441	198	0.01	100	15.9	10385	PASS
442	442	50	100	100.0	64003	PASS
443	442	15	24	18.9	12082	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062321\
 Data File : BF124429.D
 Acq On : 23 Jun 2021 12:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 23 13:06:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 13:02:13 2021
 Response via : Initial Calibration

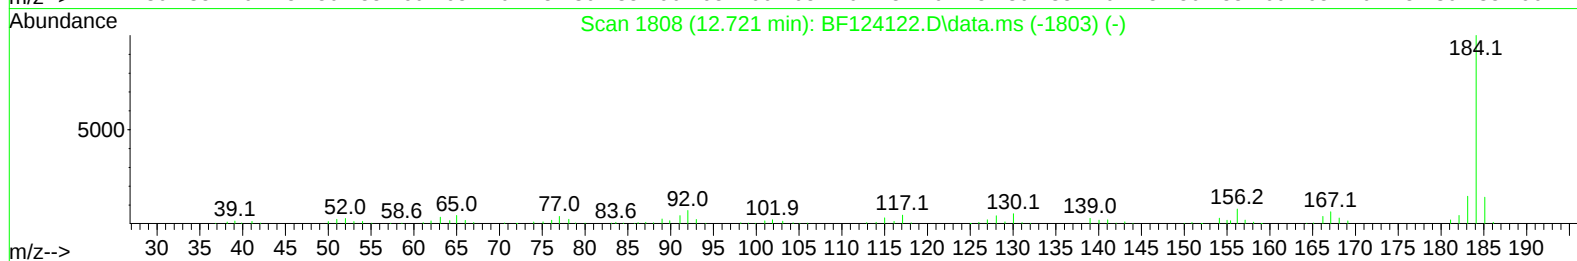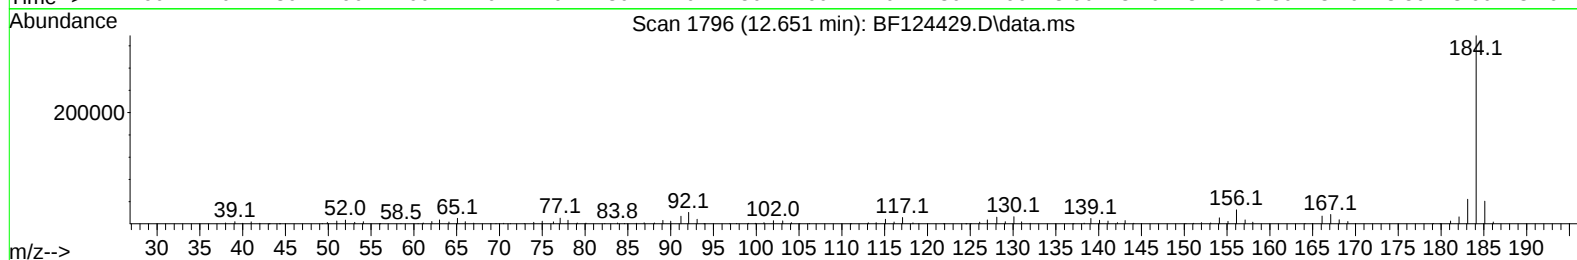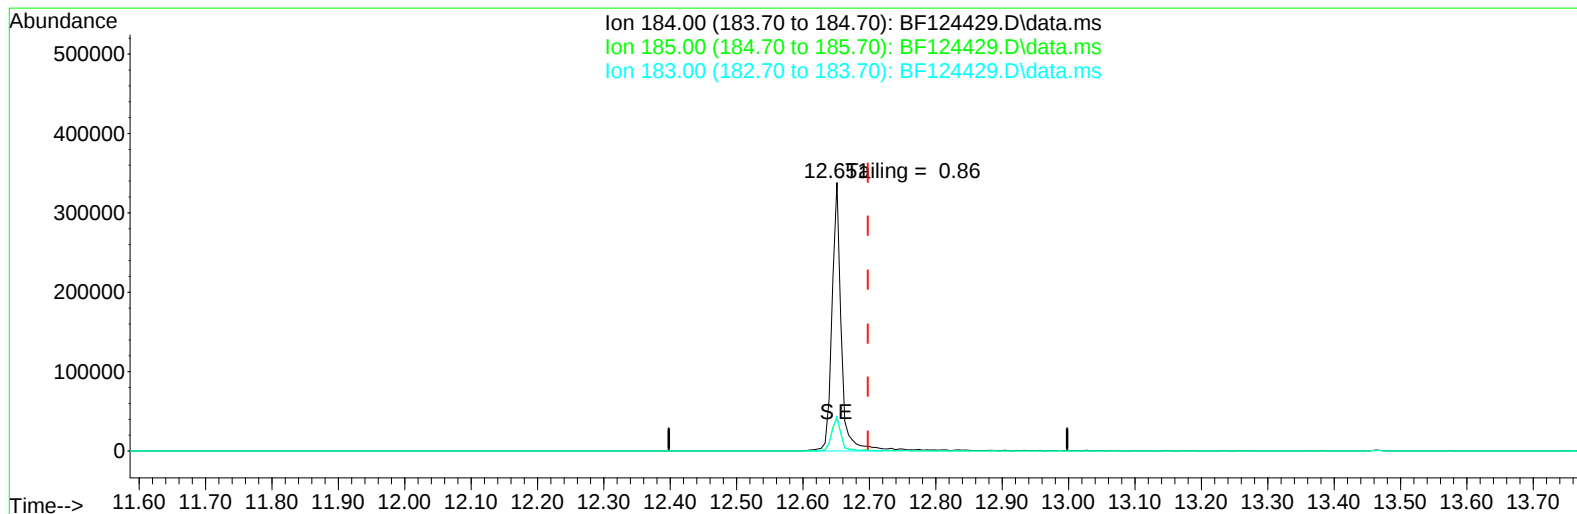

TIC: BF124429.D\data.ms

(77) Benzidine

12.651min (-0.047) 0.00 ng




response 330897

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	12.12
183.00	9.80	13.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062321\
Data File : BF124429.D
Acq On : 23 Jun 2021 12:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 13:06:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 13:02:13 2021
Response via : Initial Calibration

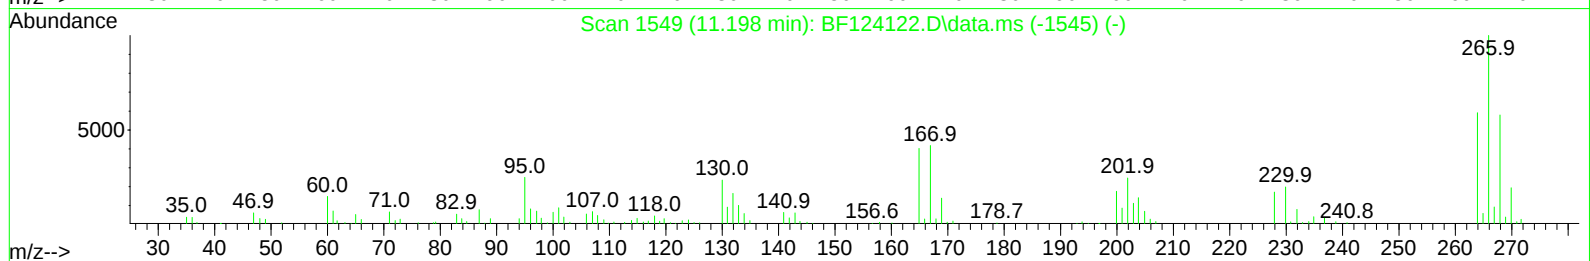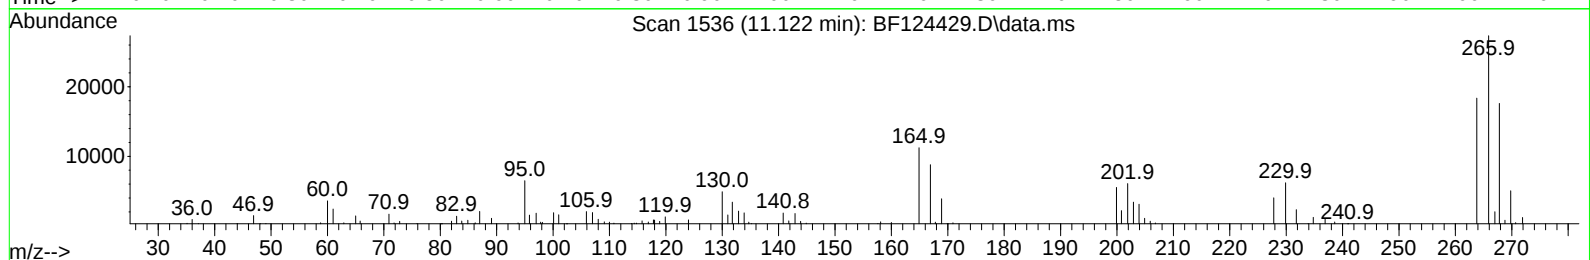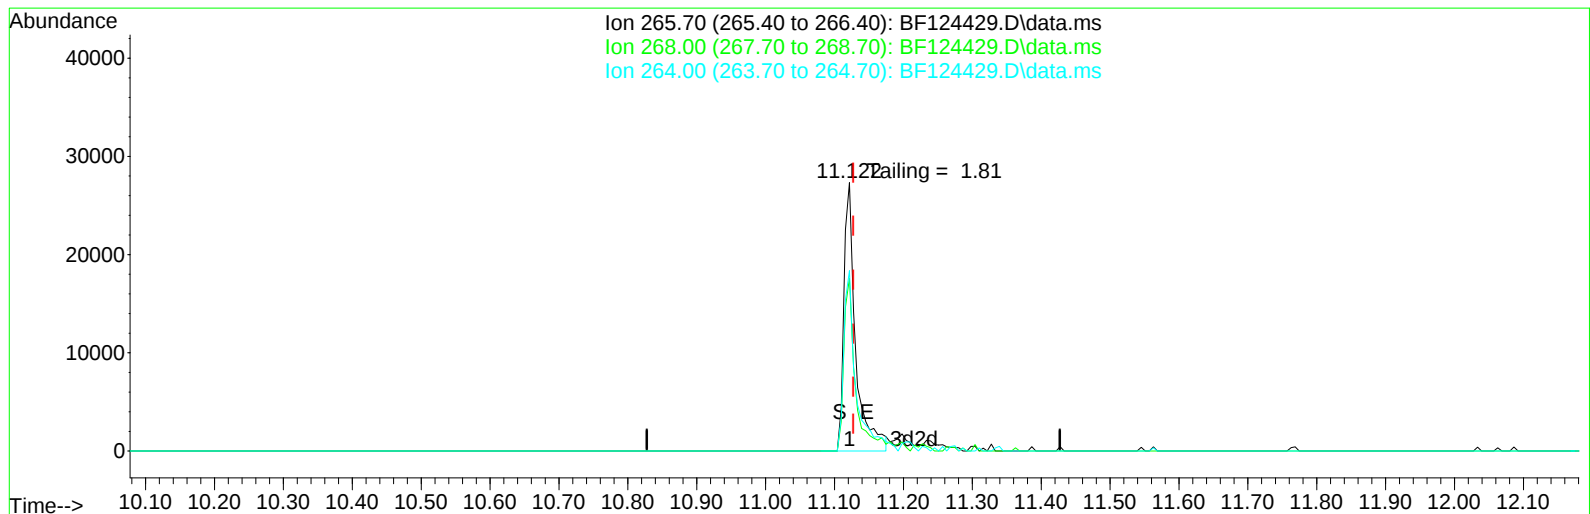

TIC: BF124429.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 12697.35 ng

response 32724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.37
264.00	65.70	67.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/23/2021	BNA_F	<u>BF124429.D</u>
Compound Name	Response	Retention Time
DDT	173366	13.46
DDD	566	13.17
DDE	396	12.82
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
962	174328	0.55