
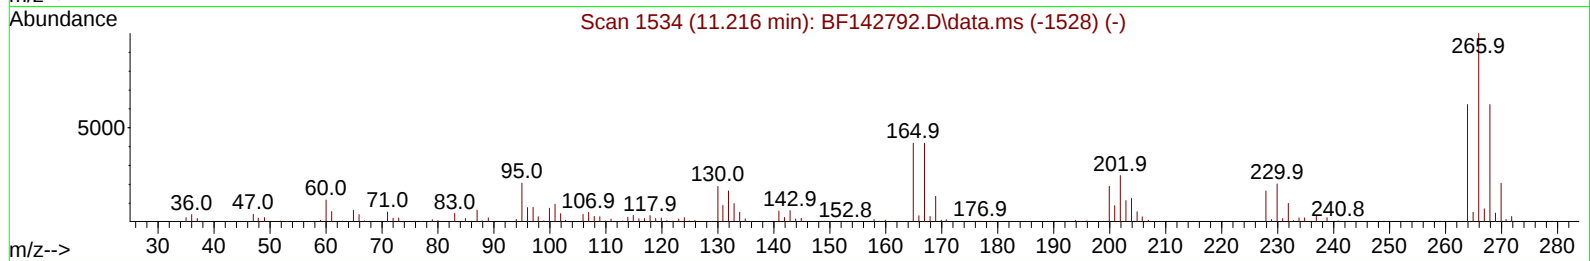
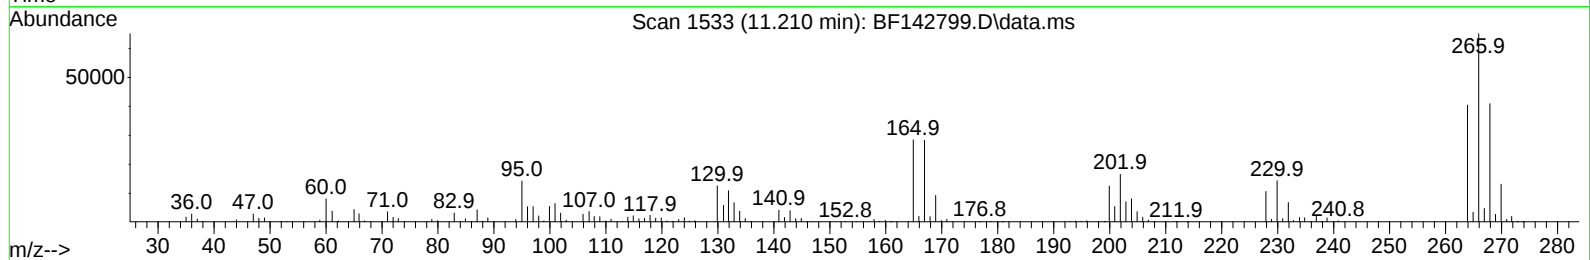


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062325\
Data File : BF142799.D
Acq On : 23 Jun 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 11:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 20 05:06:14 2025
Response via : Initial Calibration

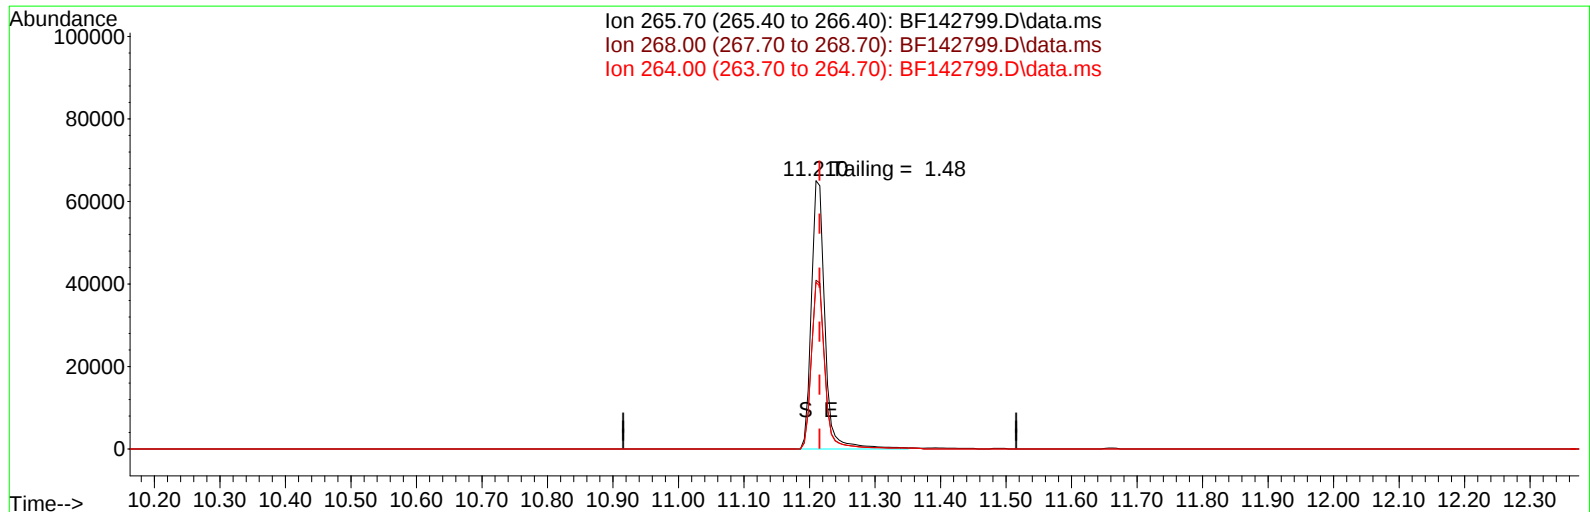

TIC: BF142799.D\data.ms




(70) Pentachlorophenol (C)

11.210min (-0.006) 40007.16 ng

response 93532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.91
264.00	62.40	62.11
0.00	0.00	0.00

Quant Time: Jun 23 11:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 20 05:06:14 2025
Response via : Initial Calibration

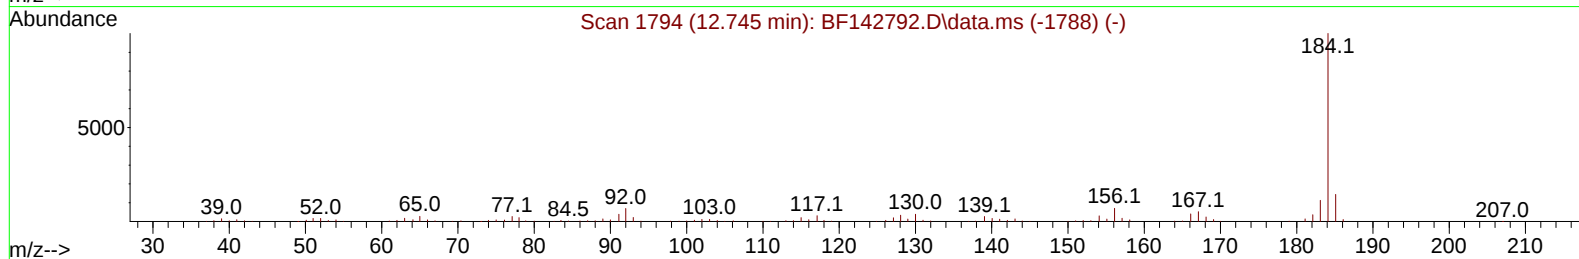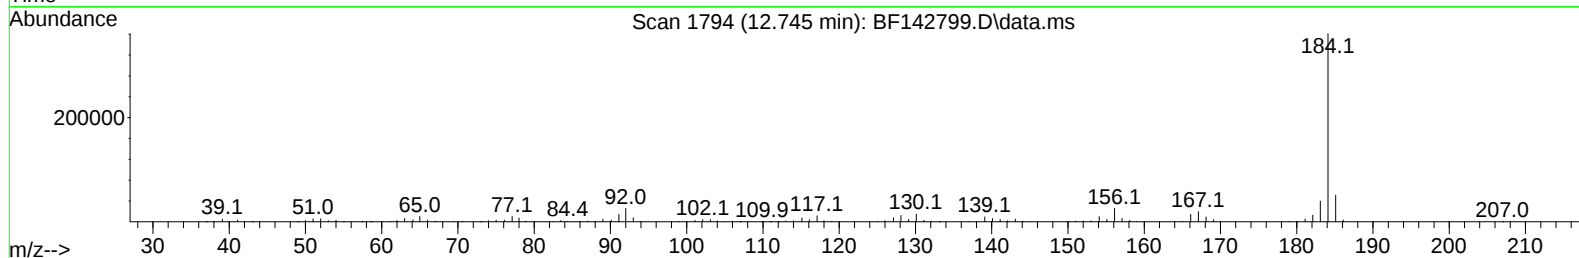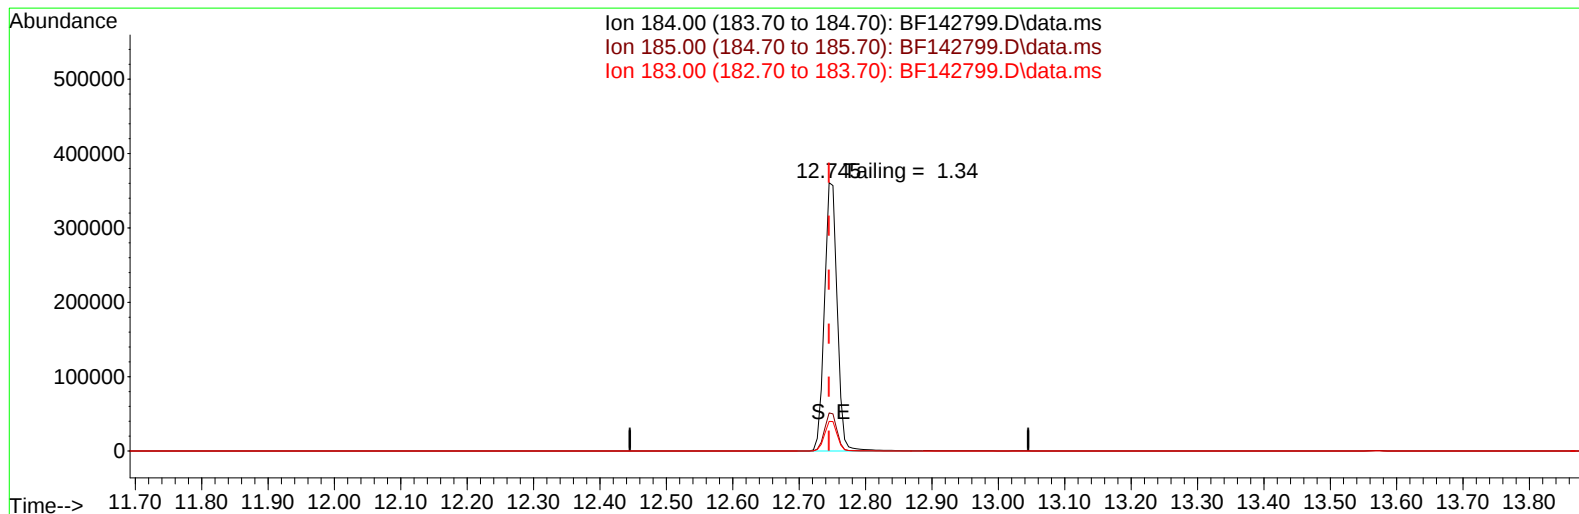

TIC: BF142799.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response **483690**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.19
183.00	11.20	11.06
0.00	0.00	0.00