

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062325\
 Data File : BF142803.D
 Acq On : 23 Jun 2025 13:12
 Operator : RC/JU
 Sample : PB168544TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168544TB

Quant Time: Jun 24 06:40:02 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	96843	20.000	ng	0.00
21) Naphthalene-d8	8.163	136	367745	20.000	ng	0.00
39) Acenaphthene-d10	9.922	164	198814	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	348592	20.000	ng	0.00
76) Chrysene-d12	14.051	240	205315	20.000	ng	0.00
86) Perylene-d12	15.545	264	163065	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	810767	139.387	ng	0.02
7) Phenol-d6	6.510	99	975007	142.077	ng	0.00
23) Nitrobenzene-d5	7.440	82	602430	89.855	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	307456	150.277	ng	0.00
45) 2-Fluorobiphenyl	9.239	172	1274819	84.234	ng	0.00
79) Terphenyl-d14	12.998	244	1312638	88.336	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062325\
Data File : BF142803.D
Acq On : 23 Jun 2025 13:12
Operator : RC/JU
Sample : PB168544TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168544TB

Quant Time: Jun 24 06:40:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration




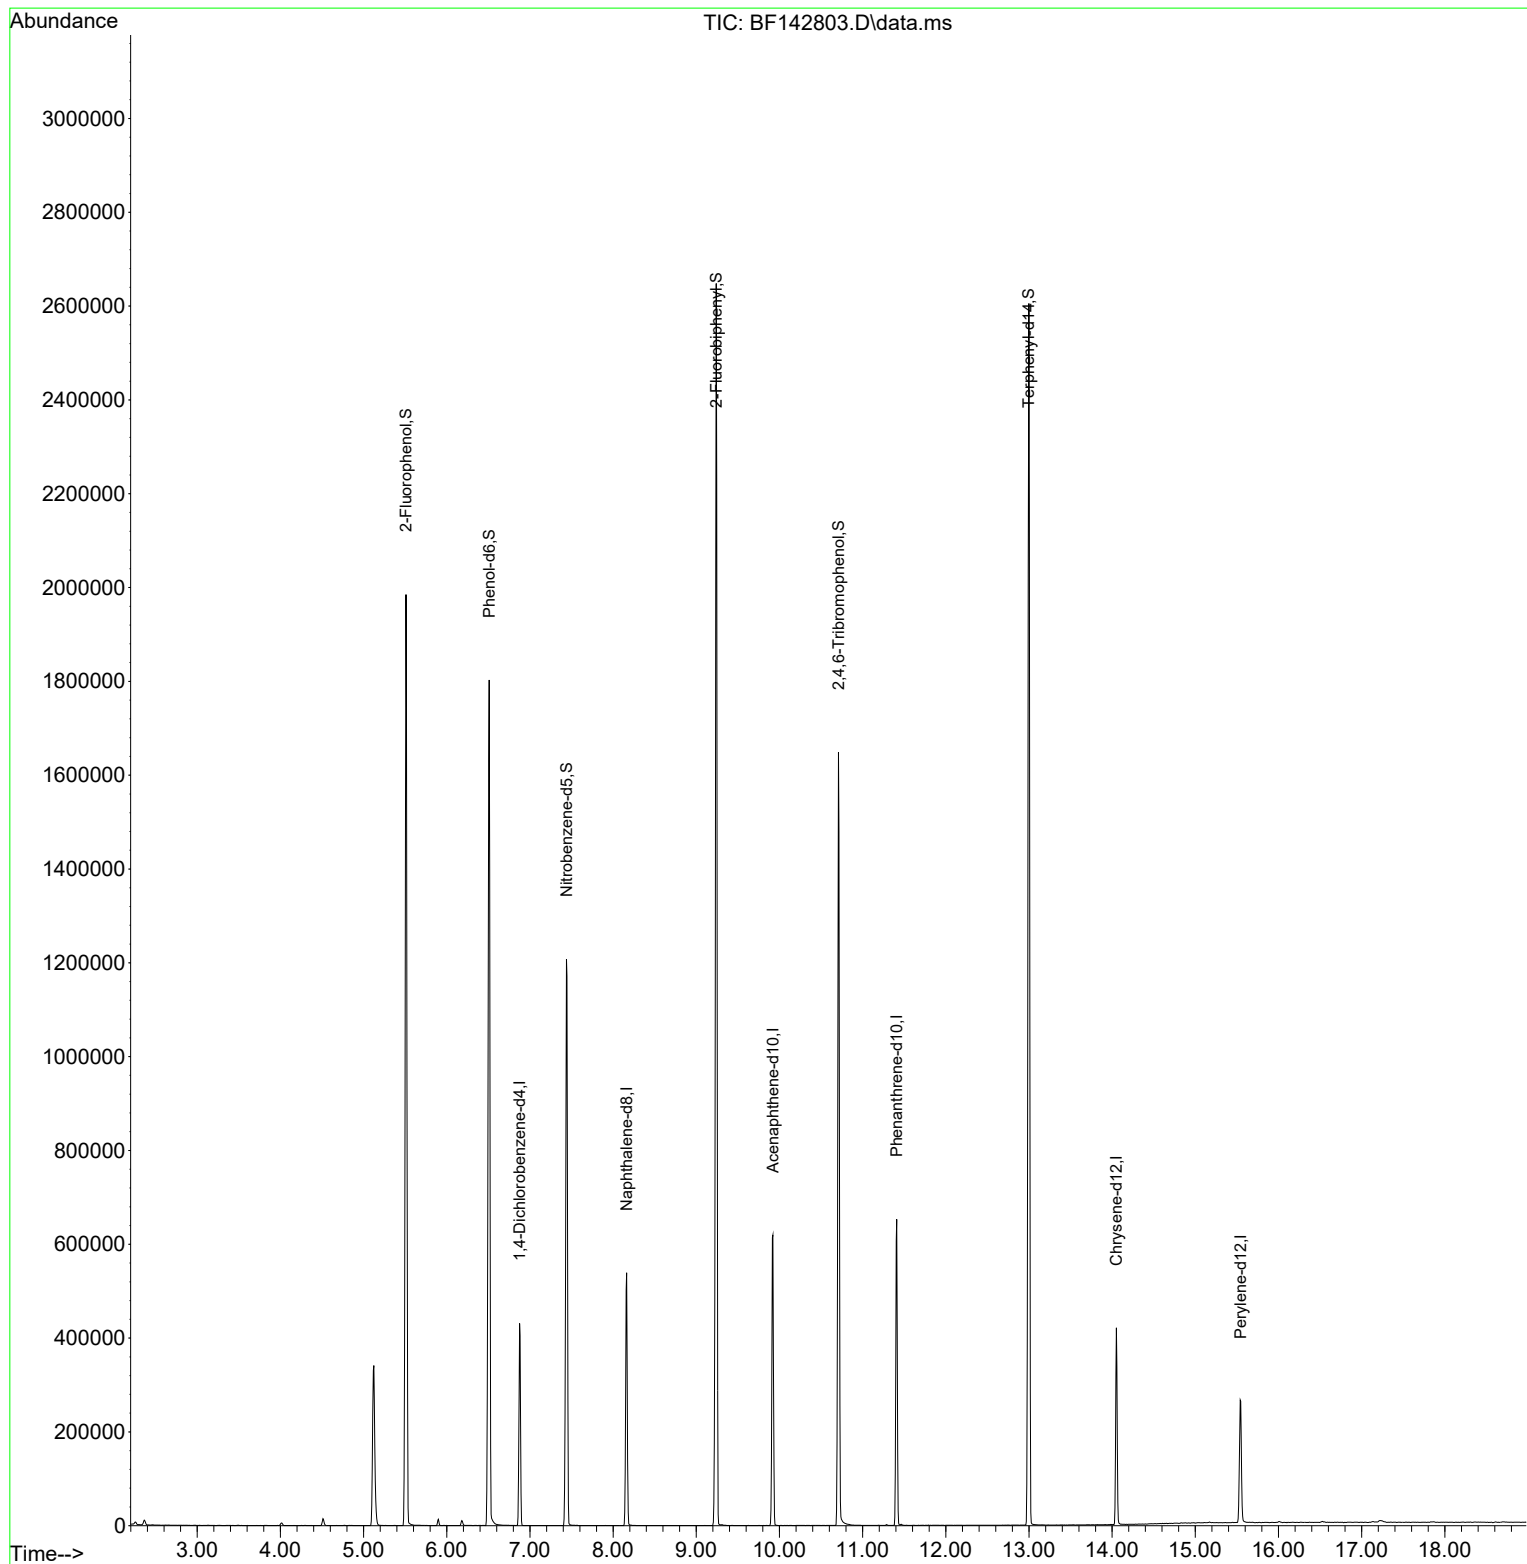




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 797
Delta R.T. -0.006 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12




Instrument :
BNA_F
ClientSampleId :
PB168544TB


Tgt Ion:152 Resp: 96843
Ion Ratio Lower Upper
152 100
150 156.4 127.2 190.8
115 59.9 46.6 69.8

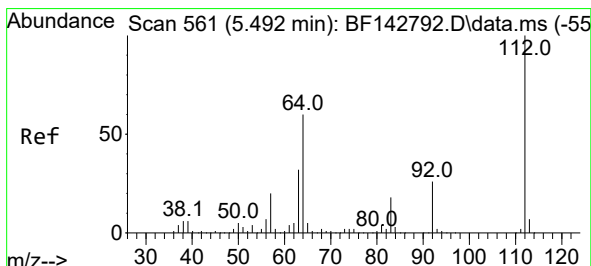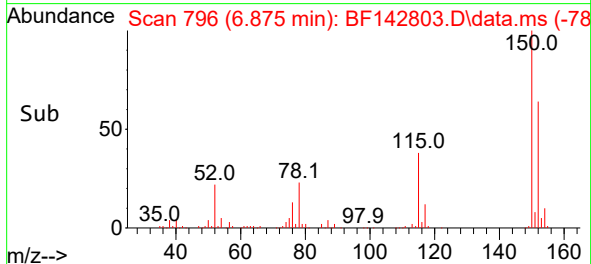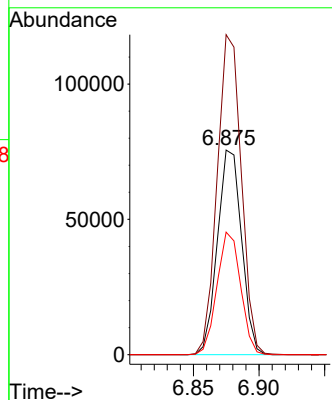

#5
2-Fluorophenol
Concen: 139.387 ng
RT: 5.510 min Scan# 564
Delta R.T. 0.018 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12

Tgt Ion:112 Resp: 810767
Ion Ratio Lower Upper
112 100
64 58.9 48.2 72.2
63 31.4 25.7 38.5


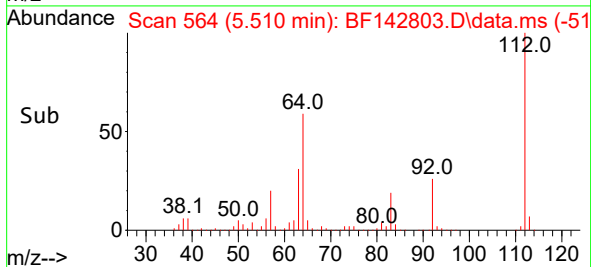
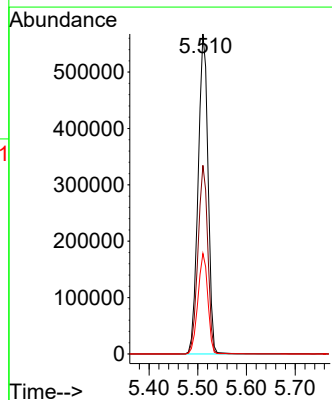
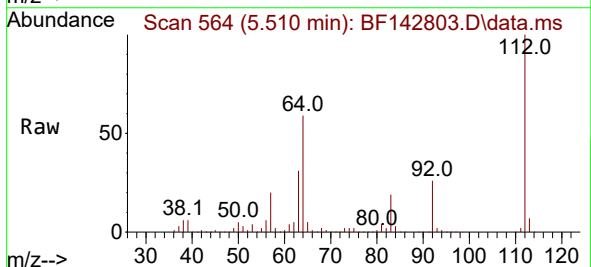


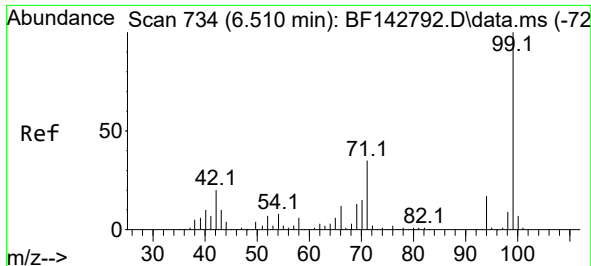

#7
Phenol-d6
Concen: 142.077 ng
RT: 6.510 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12




Instrument :
BNA_F
ClientSampleId :
PB168544TB


Tgt Ion: 99 Resp: 975007
Ion Ratio Lower Upper
99 100
42 19.8 15.9 23.9
71 35.1 27.8 41.8

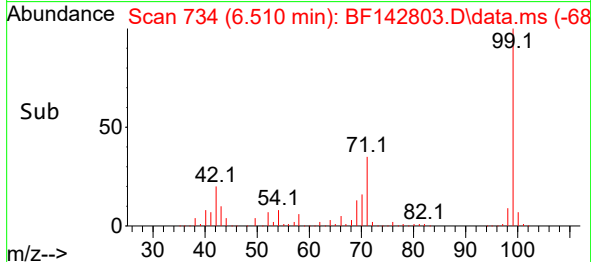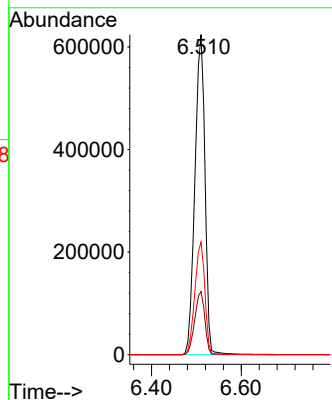

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.163 min Scan# 1015
Delta R.T. -0.006 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12

Tgt Ion: 136 Resp: 367745
Ion Ratio Lower Upper
136 100
137 10.7 8.4 12.6
54 7.6 6.3 9.5
68 4.8 3.7 5.5

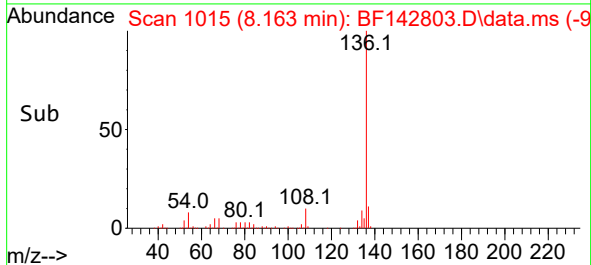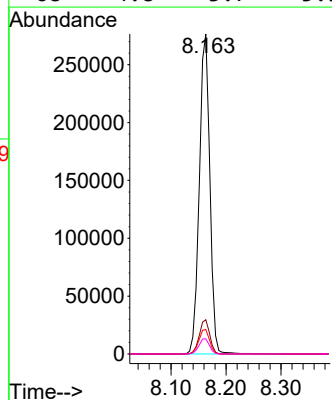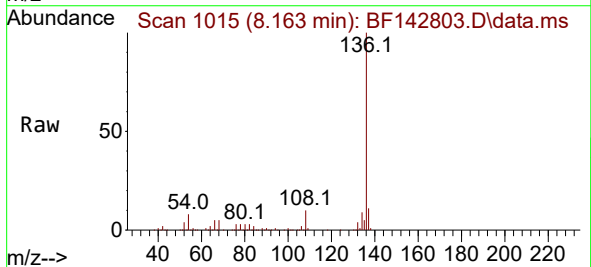

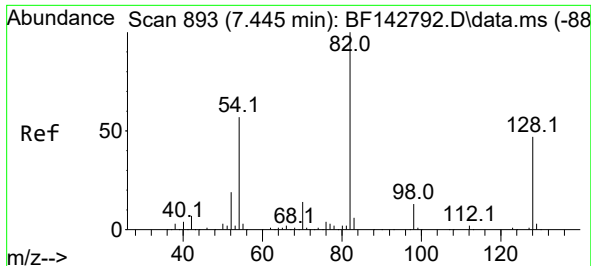

#23

Nitrobenzene-d5

Concen: 89.855 ng

RT: 7.440 min Scan# 893

Delta R.T. -0.005 min

Lab File: BF142803.D

Acq: 23 Jun 2025 13:12

Instrument :

BNA_F

ClientSampleId :

PB168544TB





Tgt Ion: 82 Resp: 602430

Ion Ratio Lower Upper

82 100

128 46.8 37.7 56.5

54 57.1 45.7 68.5

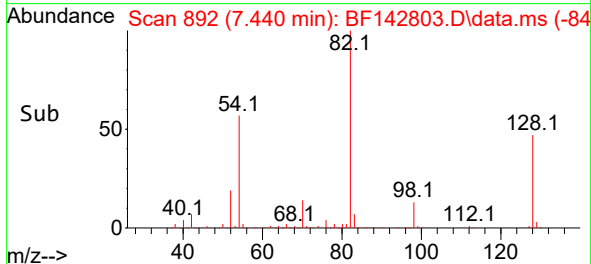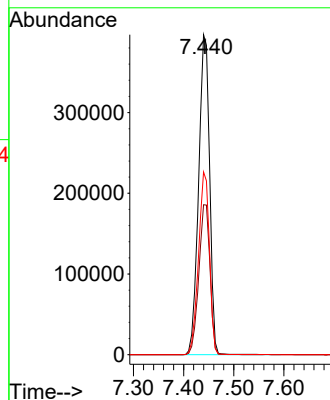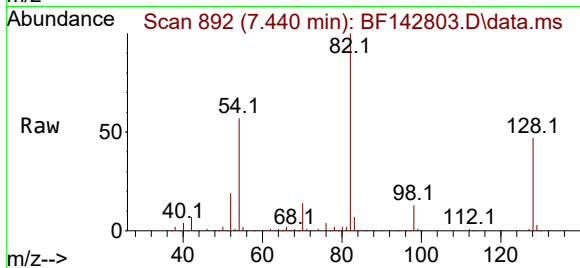

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.922 min Scan# 1314

Delta R.T. 0.000 min

Lab File: BF142803.D

Acq: 23 Jun 2025 13:12




Tgt Ion:164 Resp: 198814


Ion Ratio Lower Upper

164 100

162 100.5 81.8 122.8

160 44.3 36.0 54.0


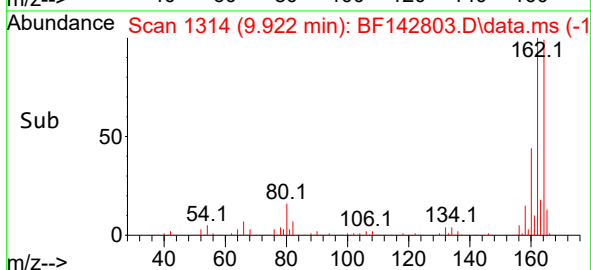
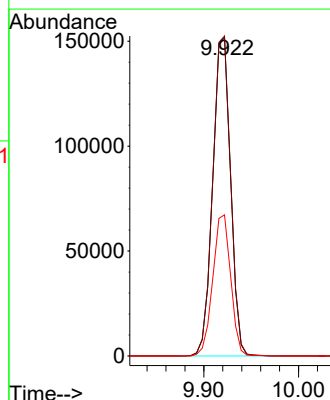
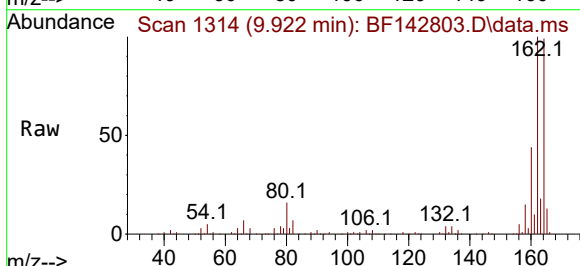


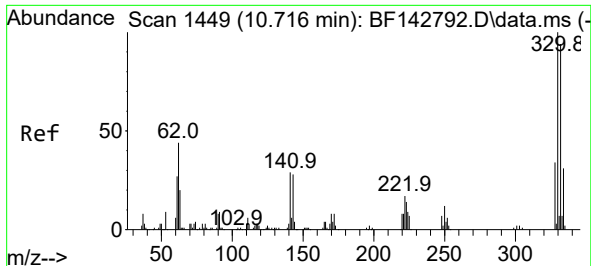

#42
2,4,6-Tribromophenol
Concen: 150.277 ng
RT: 10.710 min Scan# 1449
Delta R.T. -0.006 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12




Instrument :
BNA_F
ClientSampleId :
PB168544TB


Tgt Ion:330 Resp: 307456
Ion Ratio Lower Upper
330 100
332 96.6 75.0 112.6
141 31.0 25.3 37.9

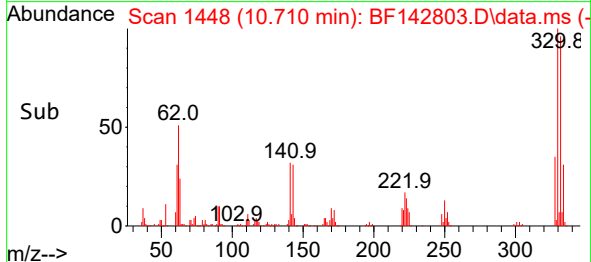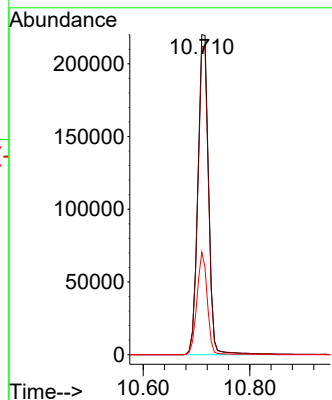

#45
2-Fluorobiphenyl
Concen: 84.234 ng
RT: 9.239 min Scan# 1198
Delta R.T. -0.006 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12

Tgt Ion:172 Resp: 1274819
Ion Ratio Lower Upper
172 100
171 35.5 28.2 42.4
170 23.4 18.5 27.7


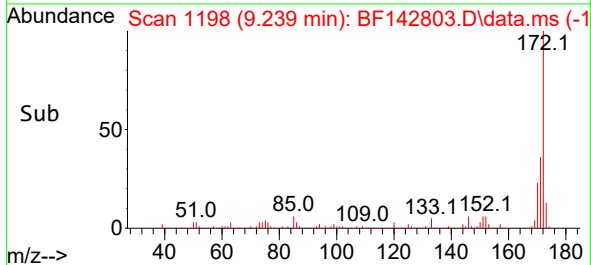
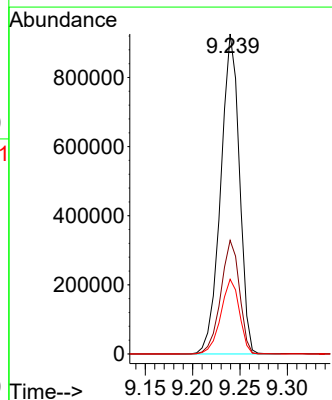
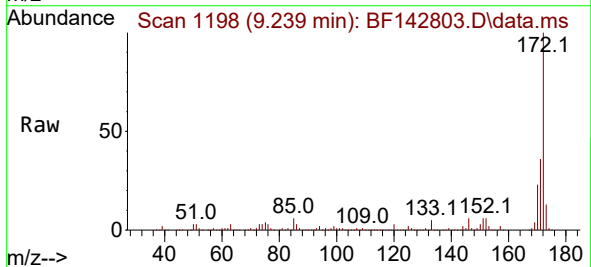




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.410 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12




Instrument :
BNA_F
ClientSampleId :
PB168544TB


Tgt Ion:188 Resp: 348592
Ion Ratio Lower Upper
188 100
94 8.2 6.7 10.1
80 8.4 6.9 10.3

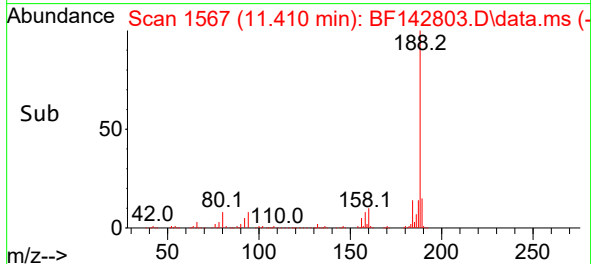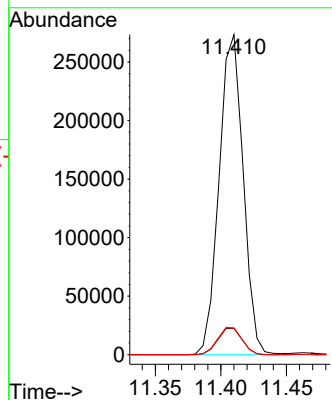

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.051 min Scan# 2016
Delta R.T. -0.006 min
Lab File: BF142803.D
Acq: 23 Jun 2025 13:12

Tgt Ion:240 Resp: 205315
Ion Ratio Lower Upper
240 100
120 10.2 8.2 12.2
236 25.5 19.8 29.8


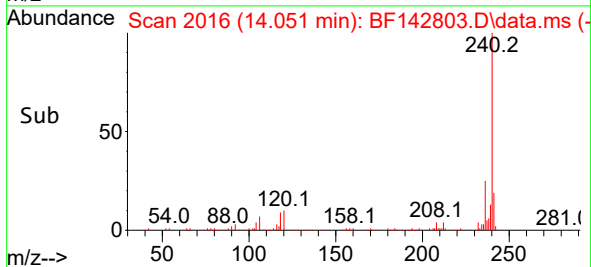
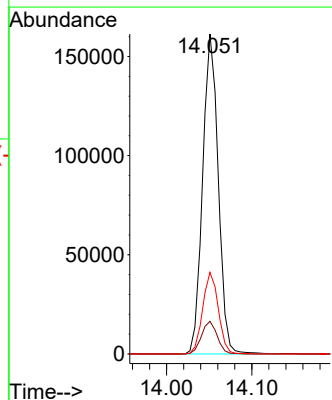
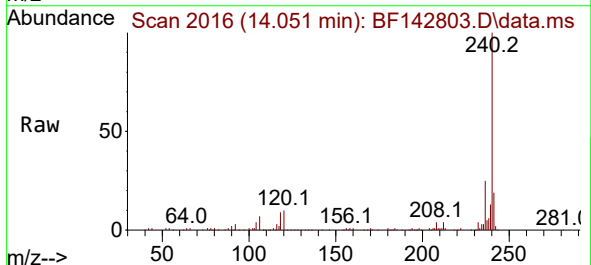


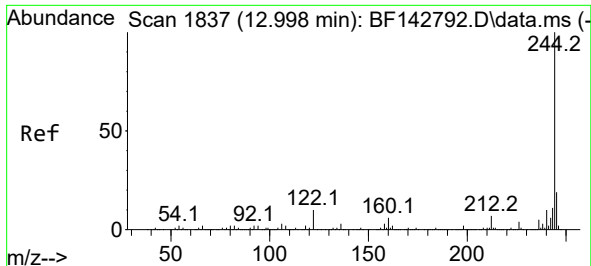

#79
 Terphenyl-d14
 Concen: 88.336 ng
 RT: 12.998 min Scan# 1837
 Delta R.T. 0.000 min
 Lab File: BF142803.D
 Acq: 23 Jun 2025 13:12

Instrument :
 BNA_F
 ClientSampleId :
 PB168544TB

Tgt Ion:244 Resp: 1312638
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.4 8.0
 122 10.5 8.2 12.2

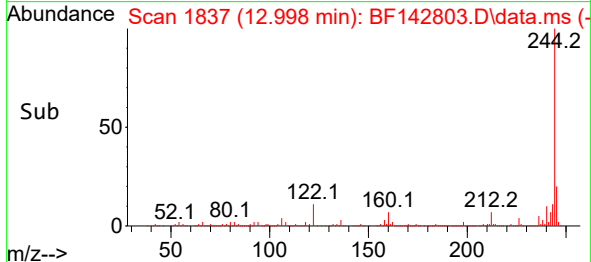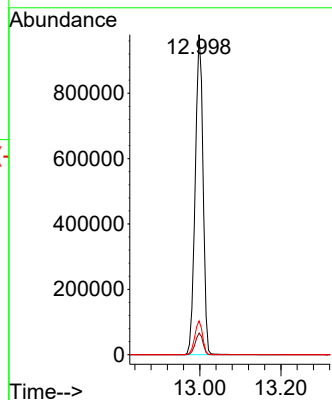

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.545 min Scan# 2270
 Delta R.T. 0.000 min
 Lab File: BF142803.D
 Acq: 23 Jun 2025 13:12

Tgt Ion:264 Resp: 163065
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.1 27.1
 265 21.4 16.6 25.0

