


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062325\
Data File : BF142799.D
Acq On : 23 Jun 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

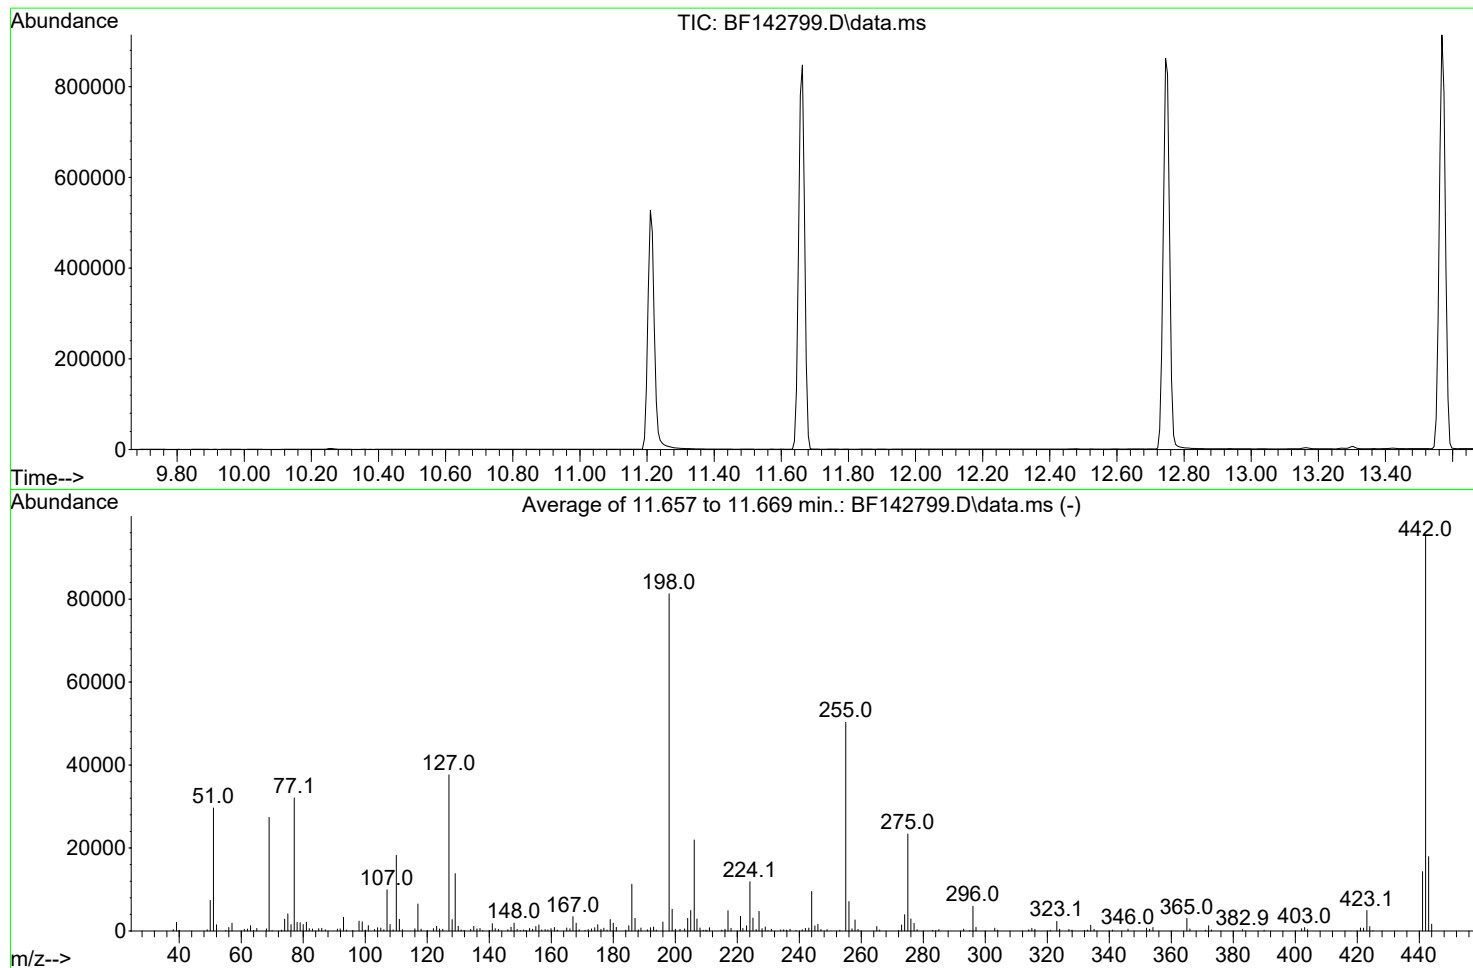

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	540	PASS
69	69	100	100	100.0	27376	PASS
70	69	0.00	2	0.4	112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81285	PASS
199	198	5	9	6.5	5251	PASS
365	198	1	100	3.7	3039	PASS
441	443	0.01	150	79.7	14301	PASS
442	442	100	100	100.0	95165	PASS
443	442	15	24	18.8	17934	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/23/2025	BNA_F	<u>BF142799.D</u>
Compound Name	Response	Retention Time
DDT	235328	13.568
DDD	3162	13.304
DDE	335	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3497	238825	1.46

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062325\
Data File : BF142799.D
Acq On : 23 Jun 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 11:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 20 05:06:14 2025
Response via : Initial Calibration

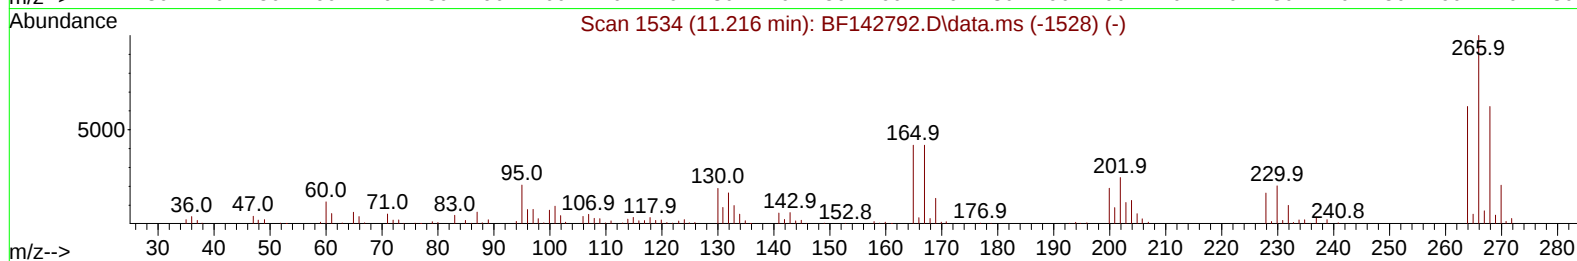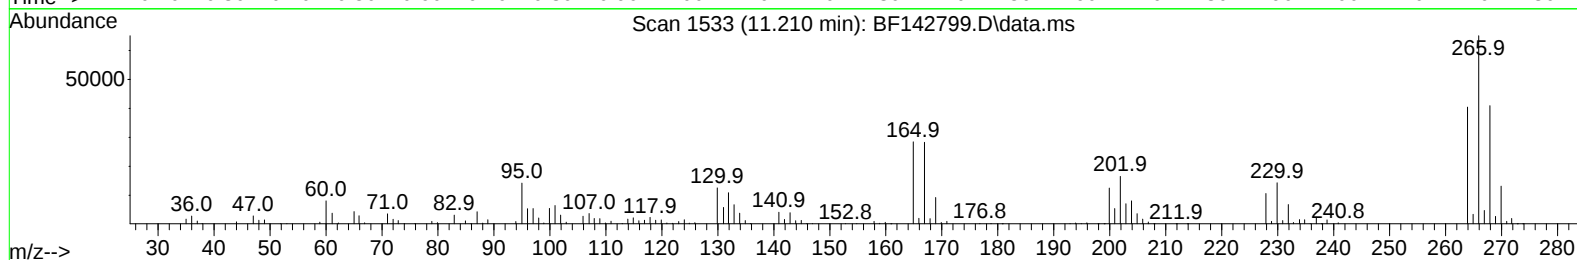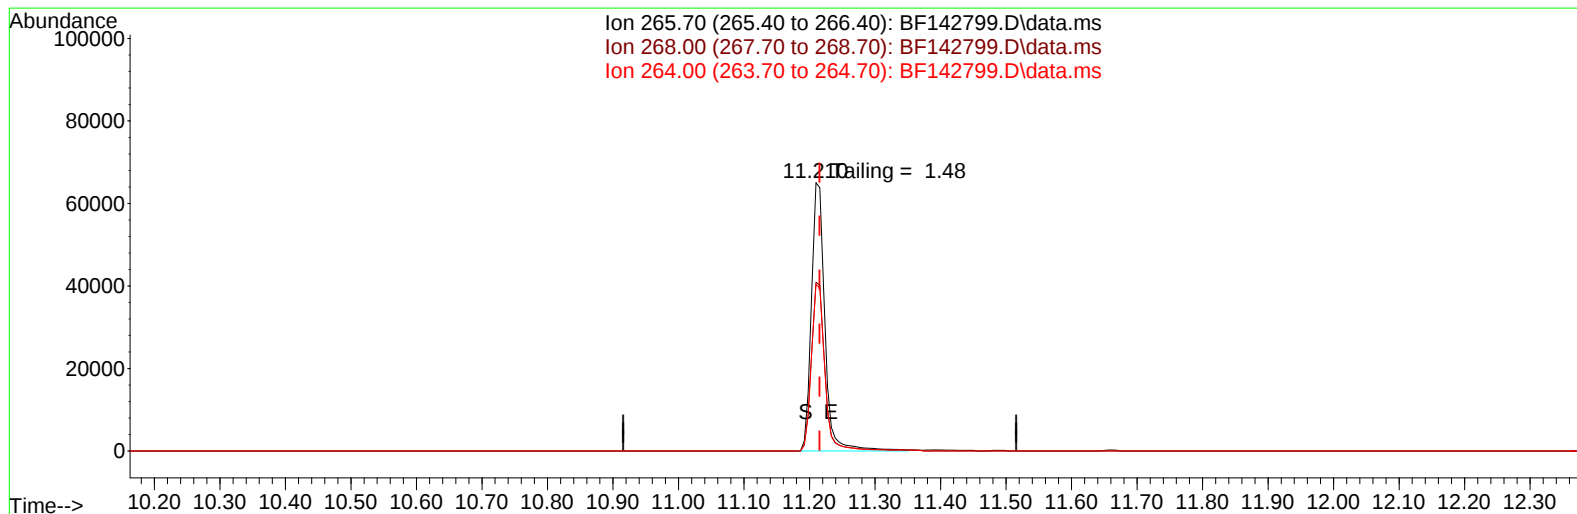

TIC: BF142799.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 40007.16 ng




response 93532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.91
264.00	62.40	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062325\
Data File : BF142799.D
Acq On : 23 Jun 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 11:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 20 05:06:14 2025
Response via : Initial Calibration

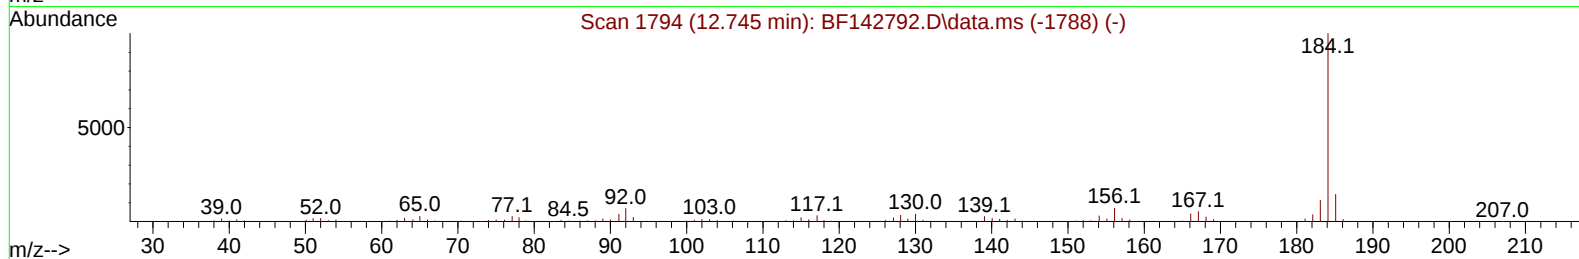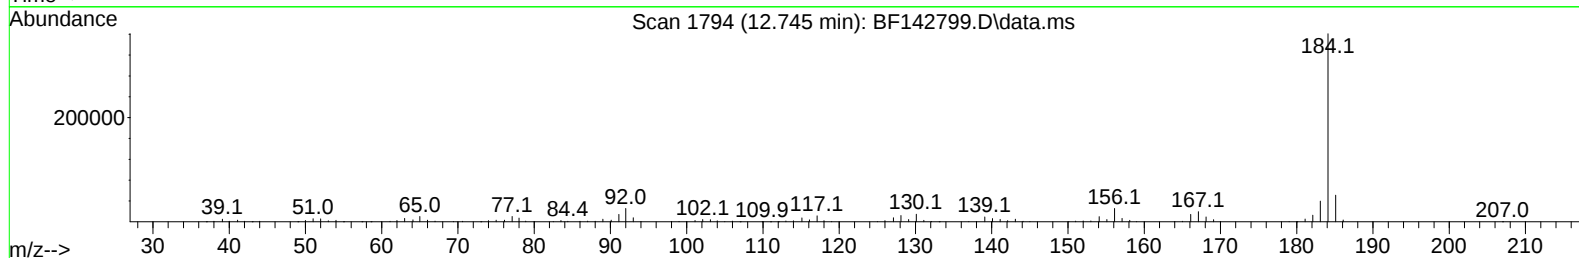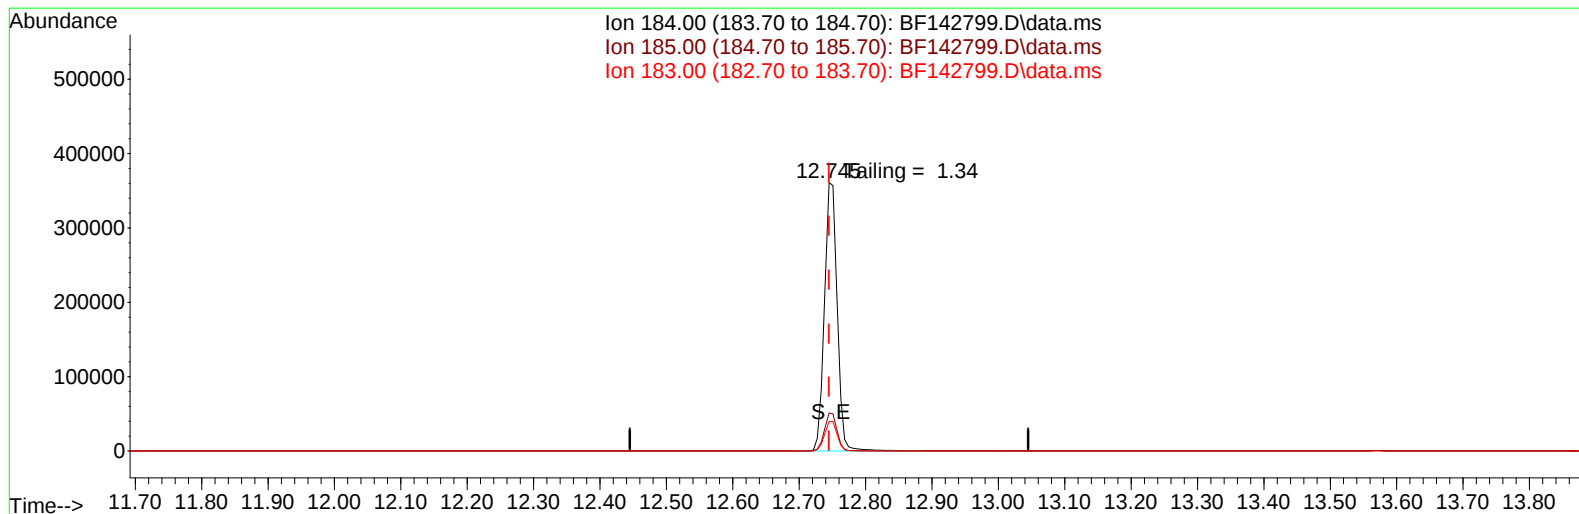

TIC: BF142799.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 483690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.19
183.00	11.20	11.06
0.00	0.00	0.00