
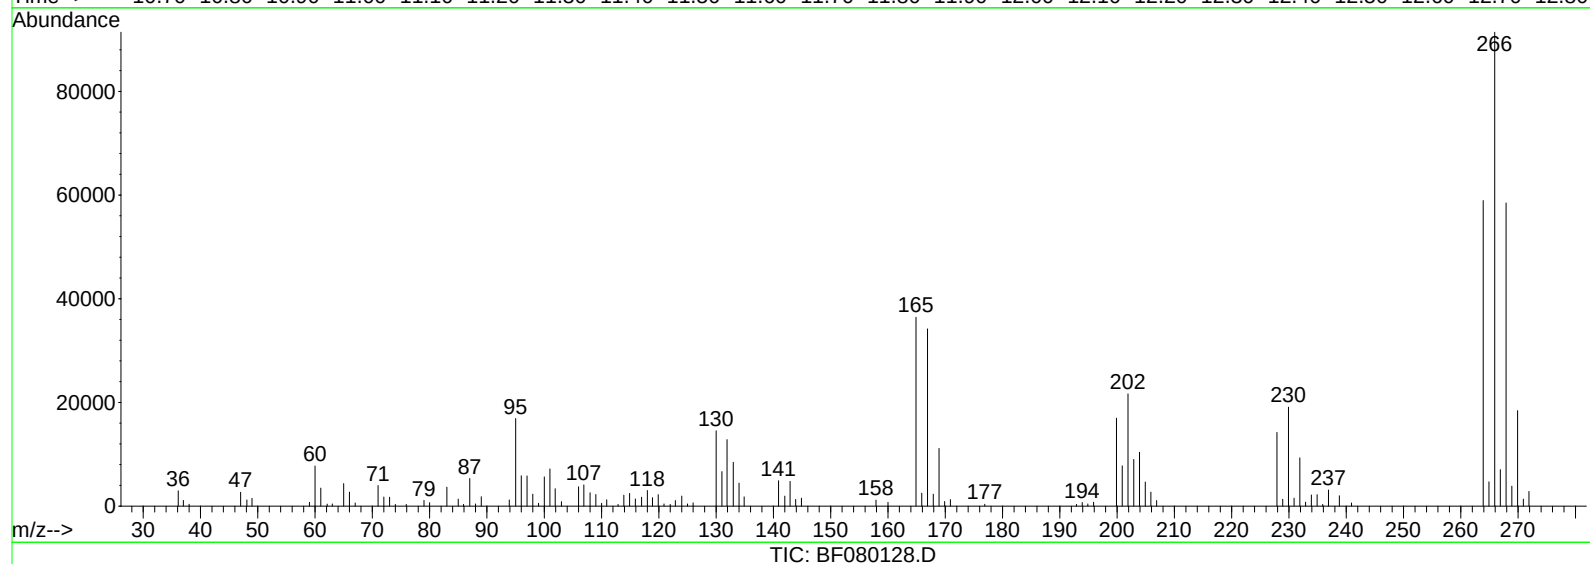


Data Path : Z:\HPCHEM1\BNA F\Data\BF062415\
Data File : BF080128.D
Acq On : 24 Jun 2015 11:19
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 01:22:51 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

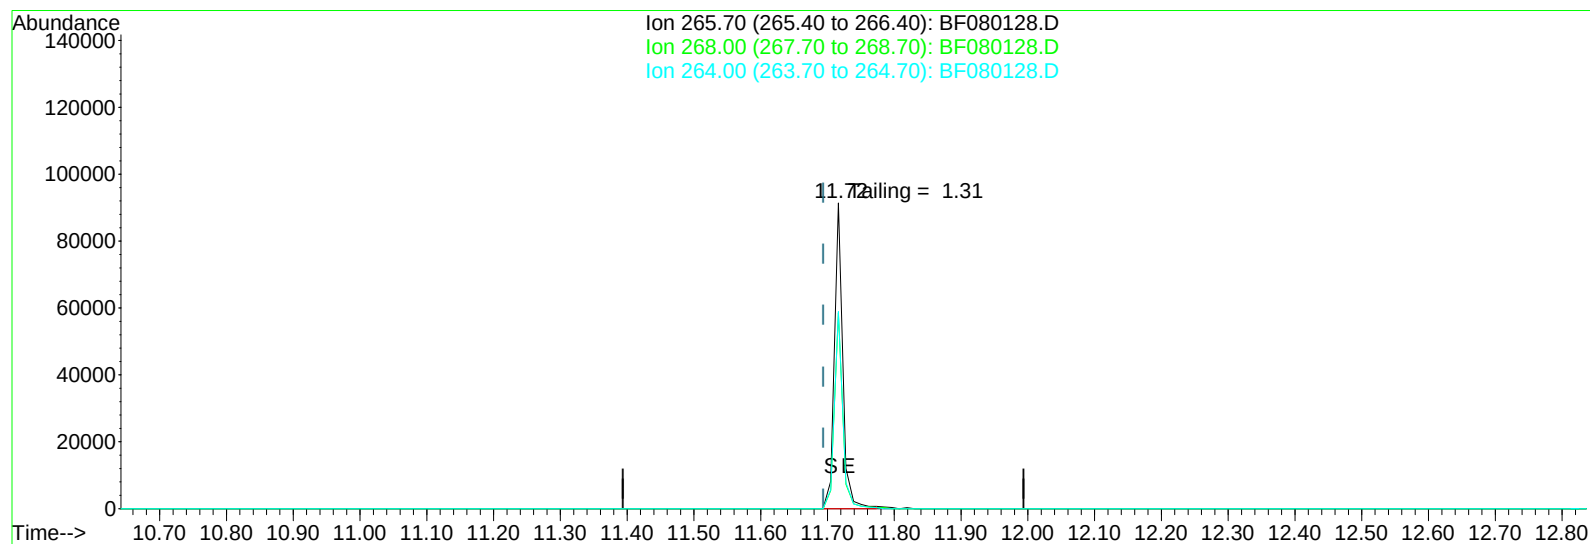

(69) Pentachlorophenol (C)



11.716min (+0.023) 0.00ng

response 80738

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.97
264.00	62.70	64.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF062415\
Data File : BF080128.D
Acq On : 24 Jun 2015 11:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 01:22:51 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

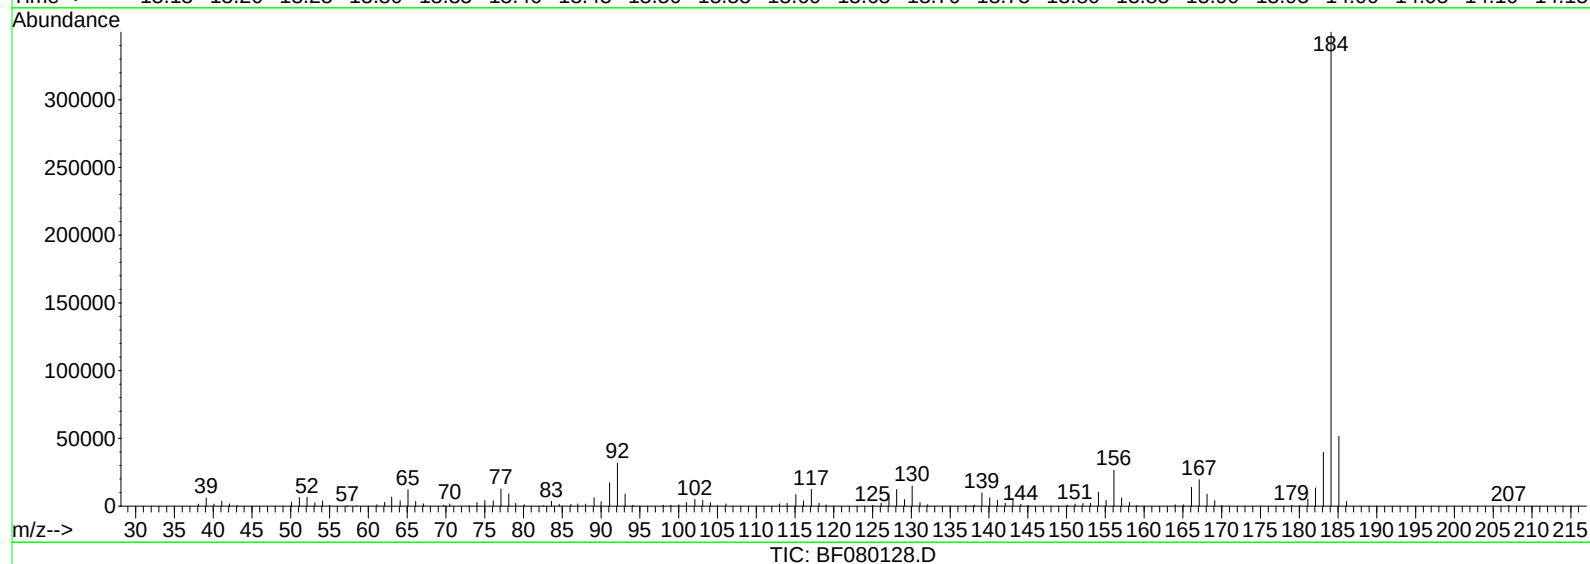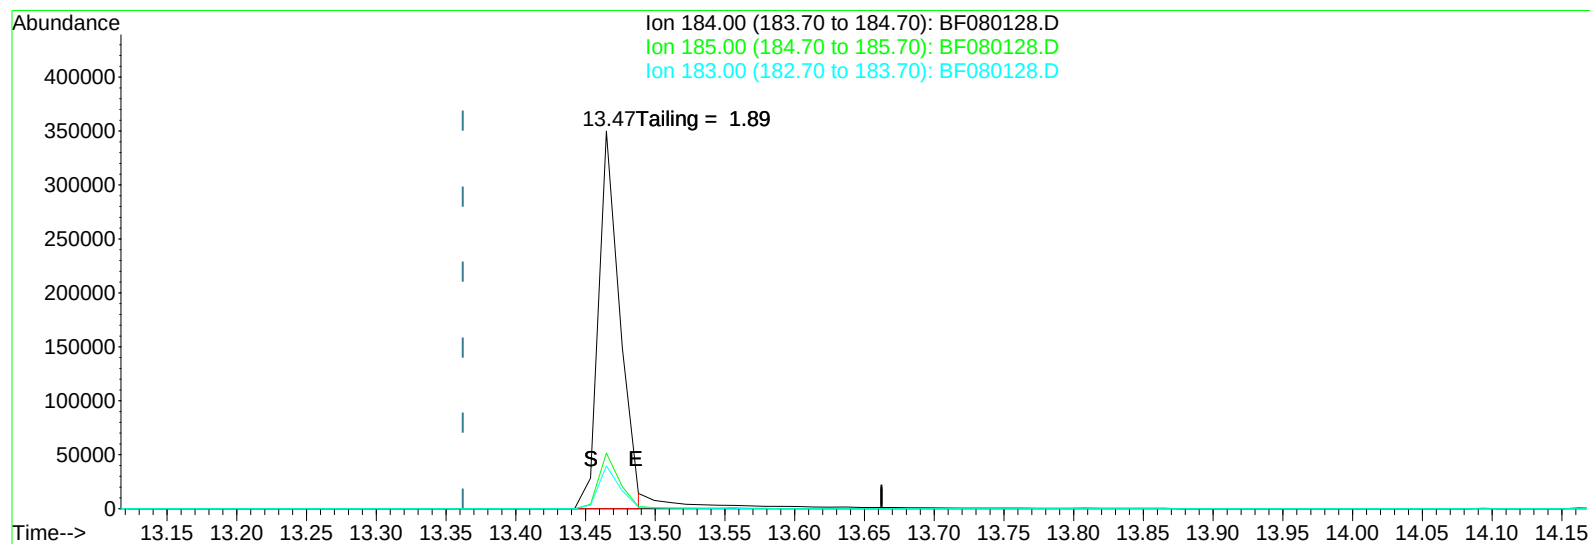

(76) Benzidine

13.465min (+0.103) 13015.42ng

response 403829

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.71
183.00	9.50	11.33
0.00	0.00	0.00