
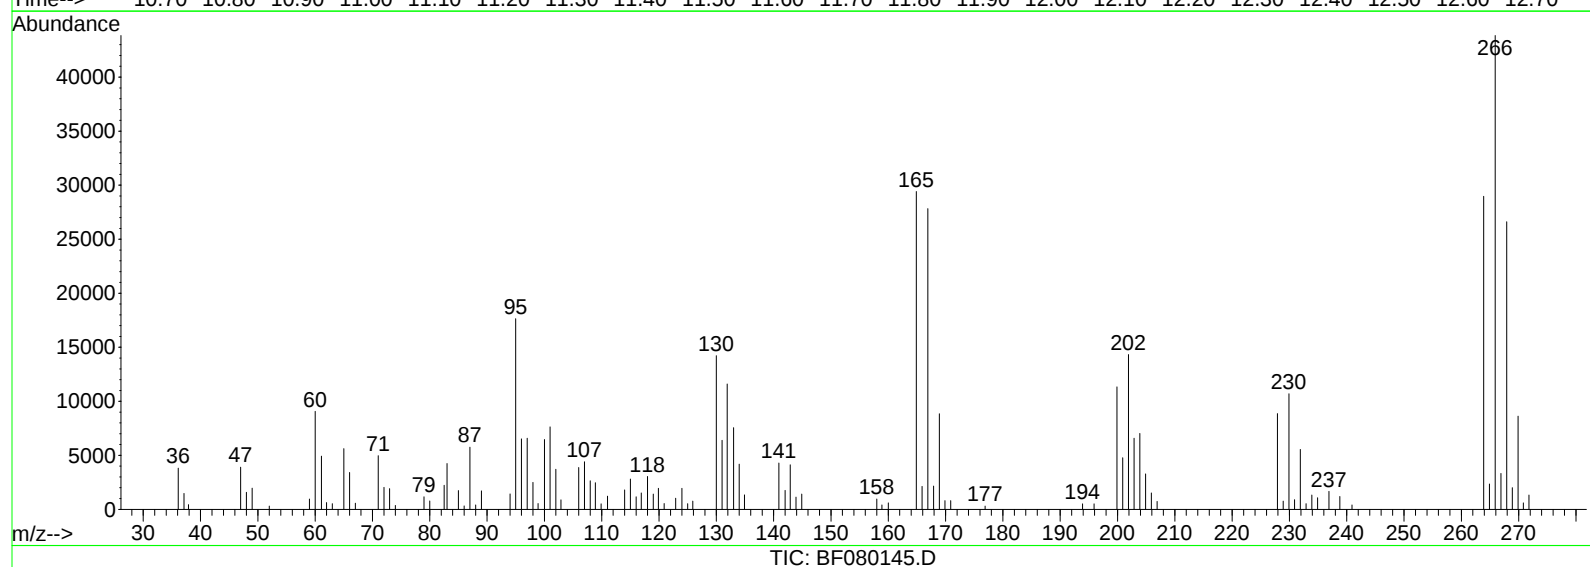


Data Path : Z:\HPCHEM1\BNA F\Data\BF062415\
Data File : BF080145.D
Acq On : 24 Jun 2015 23:14
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 02:03:04 2015
Quant Title :
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

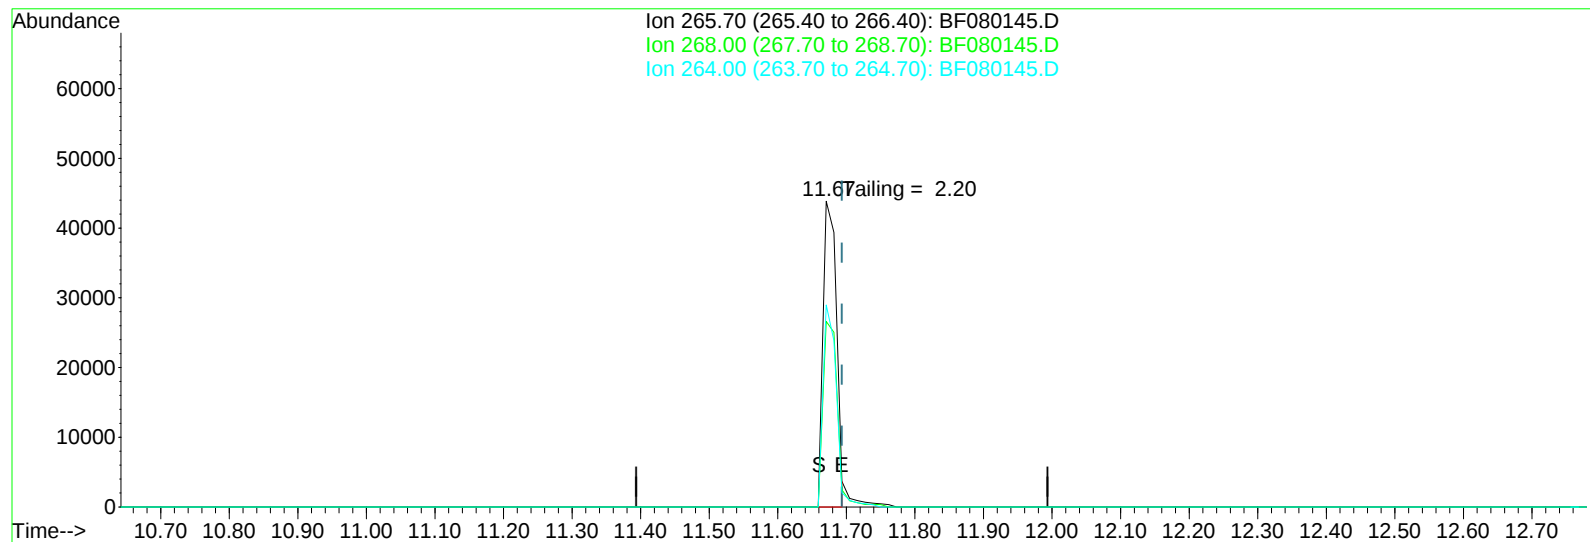

(69) Pentachlorophenol (C)



11.671min (-0.023) 44831.33ng

response 62444

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	60.69
264.00	62.70	66.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF062415\
Data File : BF080145.D
Acq On : 24 Jun 2015 23:14
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 02:03:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

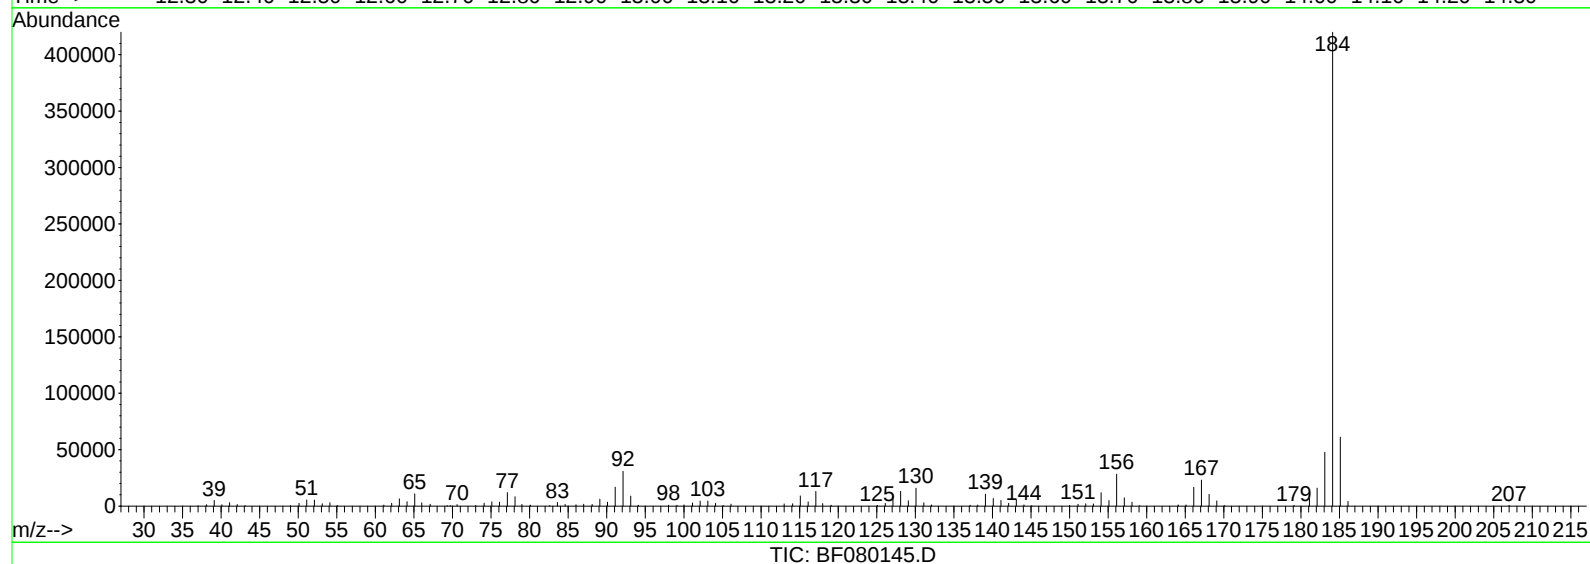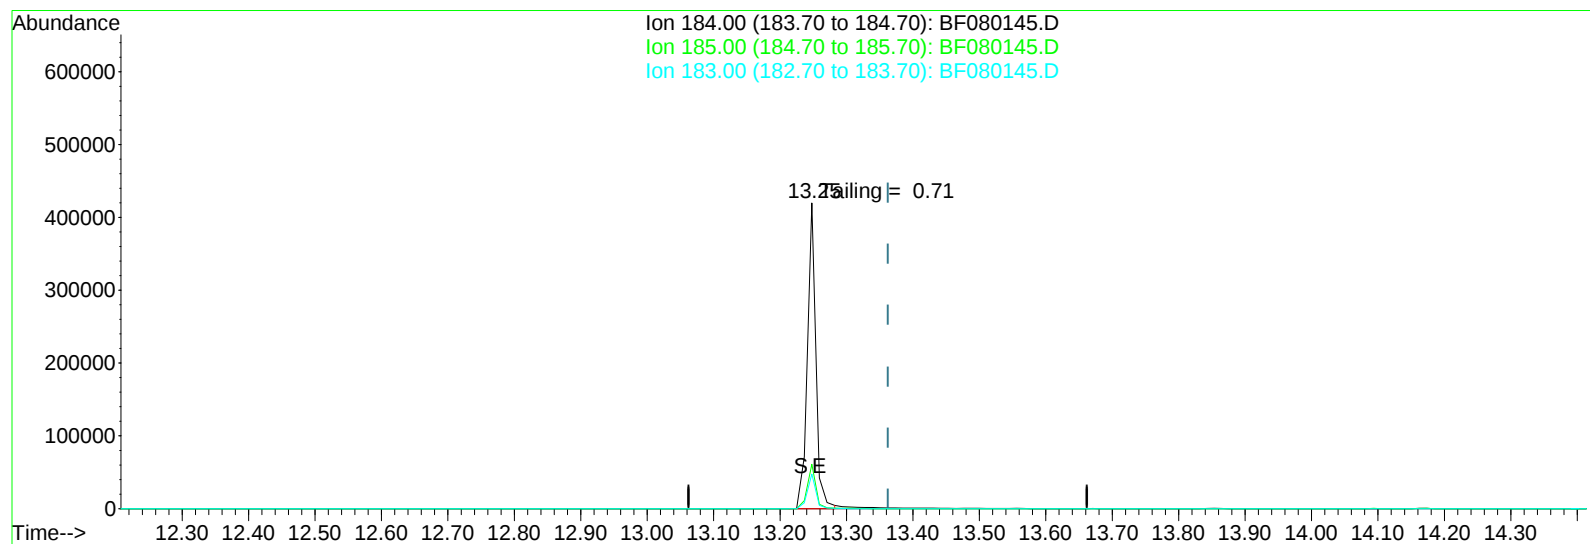

(76) Benzidine

13.248min (-0.114) 10388.19ng

response 383873

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.52
183.00	9.50	11.35
0.00	0.00	0.00