


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062415\
 Data File : BF080128.D
 Acq On : 24 Jun 2015 11:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 00:53:56 2015

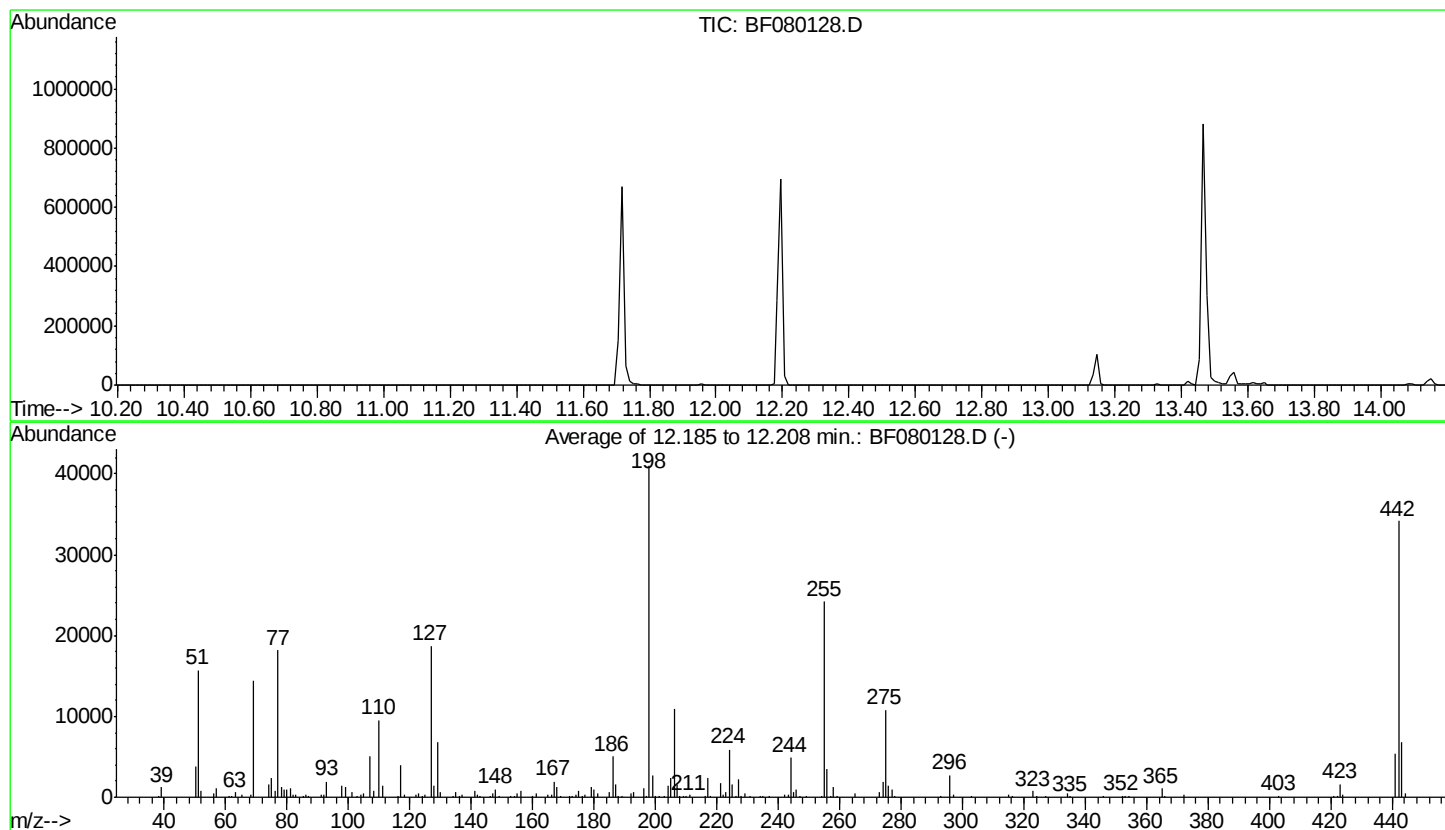

AutoFind: Scans 796, 797, 798; Background Corrected with Scan 793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	15685	PASS
68	69	0.00	2	1.9	280	PASS
69	198	0.00	100	35.2	14450	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	18700	PASS
197	198	0.00	2	0.4	173	PASS
198	198	100	100	100.0	41023	PASS
199	198	5	9	6.5	2685	PASS
275	198	10	60	26.3	10780	PASS
365	198	1	100	2.6	1048	PASS
441	442	0.01	24	15.6	5333	PASS
442	198	50	100	83.2	34144	PASS
443	442	15	24	19.8	6764	PASS