


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062415\
 Data File : BF080145.D
 Acq On : 24 Jun 2015 23:14
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 00:53:56 2015

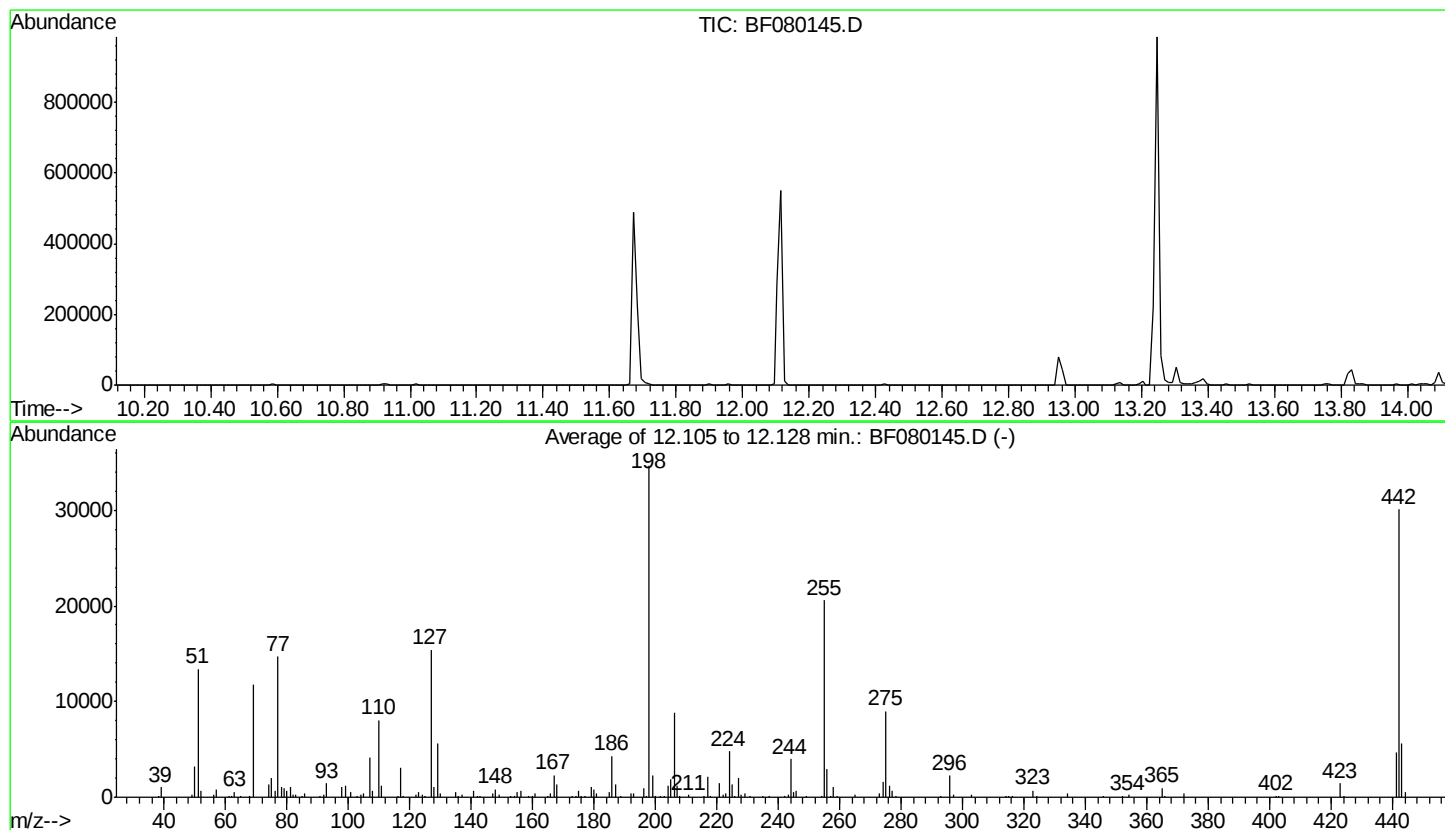

AutoFind: Scans 789, 790, 791; Background Corrected with Scan 786

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	13402	PASS
68	69	0.00	2	1.1	131	PASS
69	198	0.00	100	33.9	11741	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	15386	PASS
197	198	0.00	2	0.4	137	PASS
198	198	100	100	100.0	34656	PASS
199	198	5	9	6.4	2223	PASS
275	198	10	60	26.0	9011	PASS
365	198	1	100	2.9	1000	PASS
441	442	0.01	24	15.5	4659	PASS
442	198	50	100	86.7	30042	PASS
443	442	15	24	18.7	5613	PASS