


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062416\
 Data File : BF088330.D
 Acq On : 24 Jun 2016 14:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 04:27:12 2016

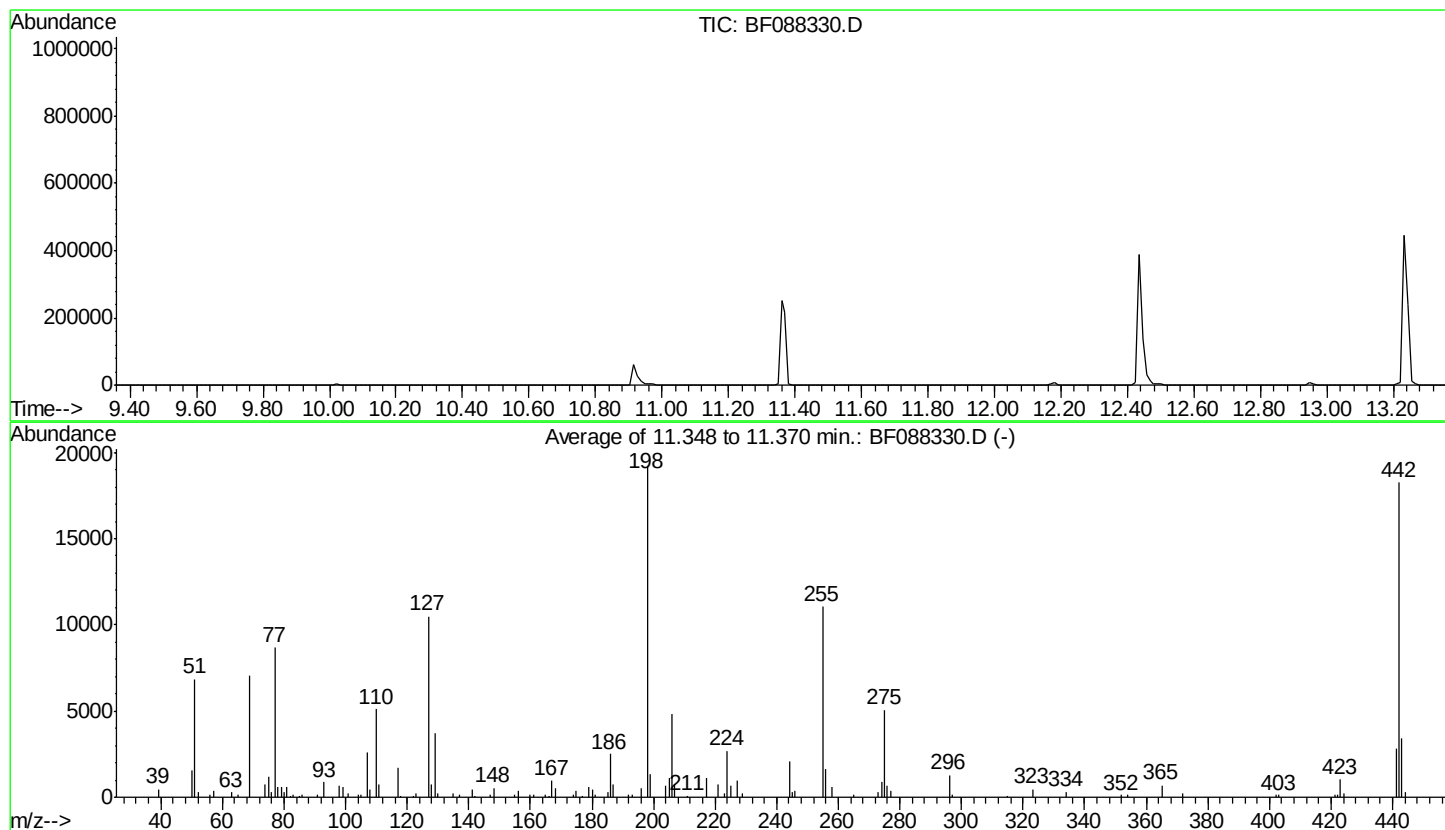

AutoFind: Scans 854, 855, 856; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	6834	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.8	7082	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.4	10473	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19236	PASS
199	198	5	9	7.0	1349	PASS
275	198	10	60	26.4	5075	PASS
365	198	1	100	3.5	676	PASS
441	442	0.01	24	15.4	2804	PASS
442	198	50	100	94.9	18246	PASS
443	442	15	24	18.7	3413	PASS