


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062416\
 Data File : BF088356.D
 Acq On : 25 Jun 2016 3:52
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 04:27:12 2016

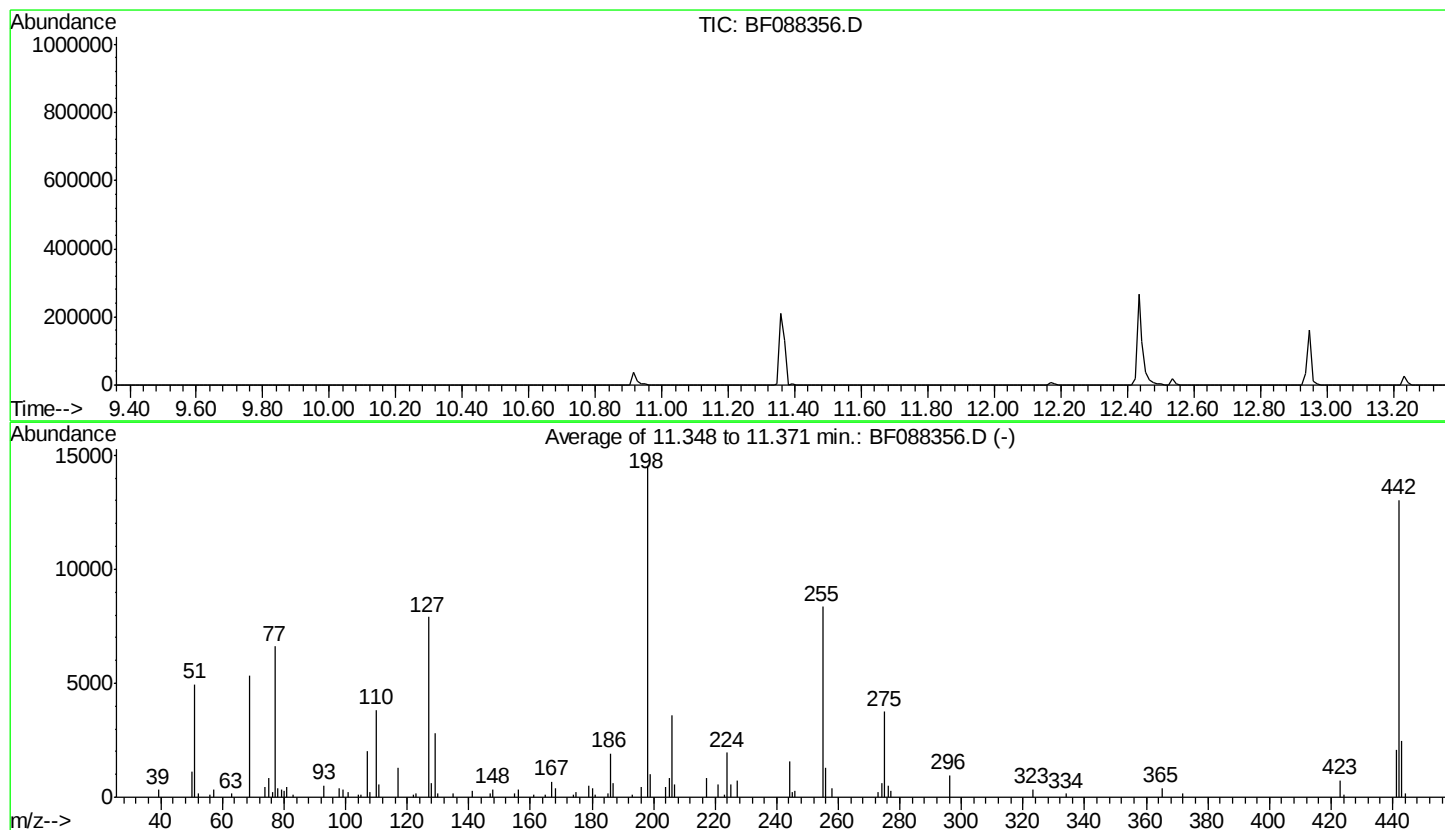

AutoFind: Scans 854, 855, 856; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	4945	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.7	5336	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.4	7915	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14542	PASS
199	198	5	9	6.8	985	PASS
275	198	10	60	25.8	3747	PASS
365	198	1	100	2.8	407	PASS
441	442	0.01	24	15.9	2072	PASS
442	198	50	100	89.6	13027	PASS
443	442	15	24	18.8	2450	PASS