
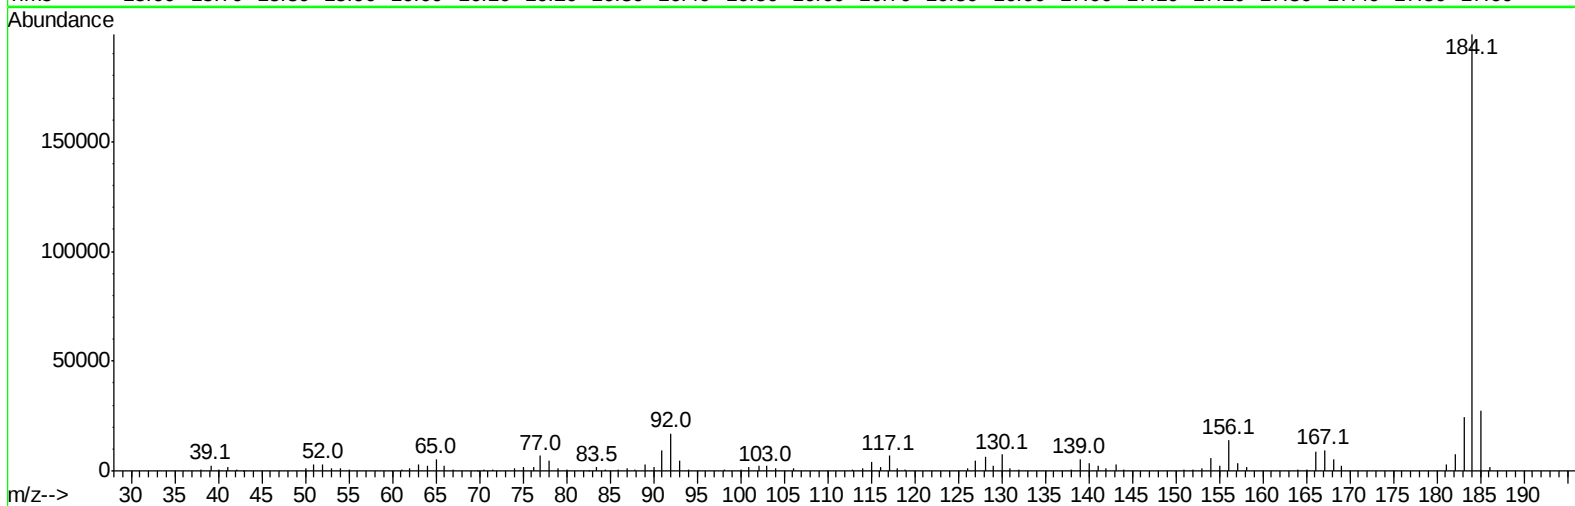


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096179.D
Acq On : 24 Jun 2017 9:03
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 08:55:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

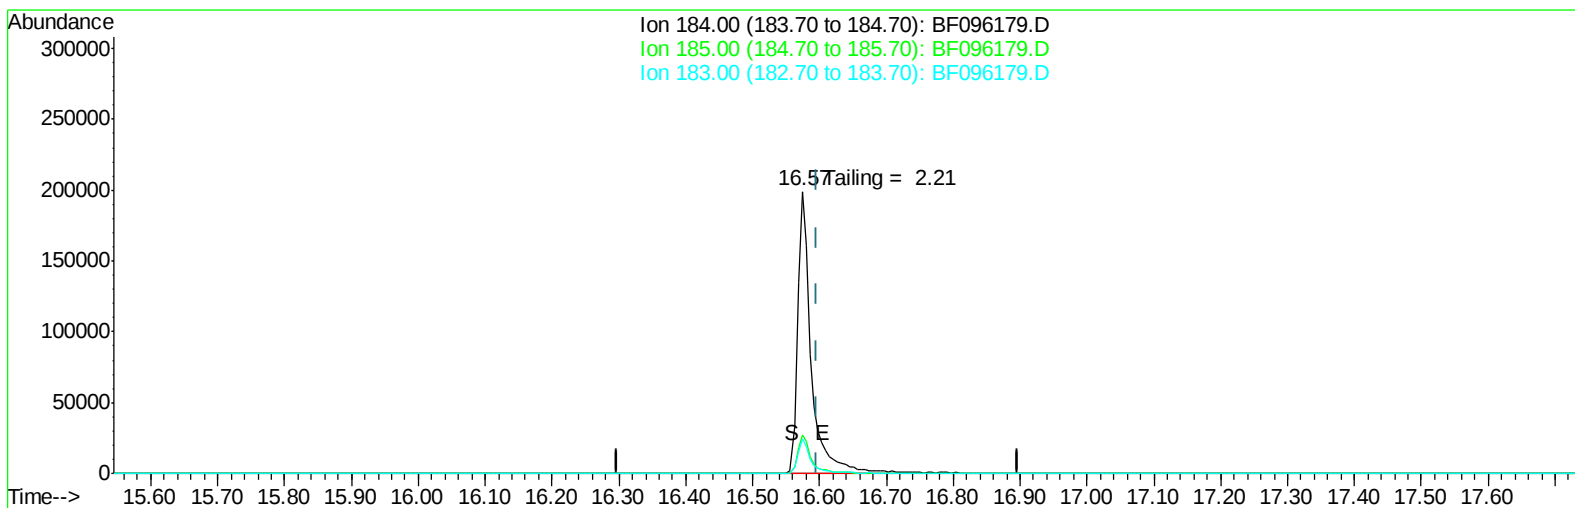

TIC: BF096179.D

(76) Benzidine



16.574min (-0.024) 0.00ng

response 283760

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.79#
183.00	12.20	12.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096179.D
Acq On : 24 Jun 2017 9:03
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 08:55:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

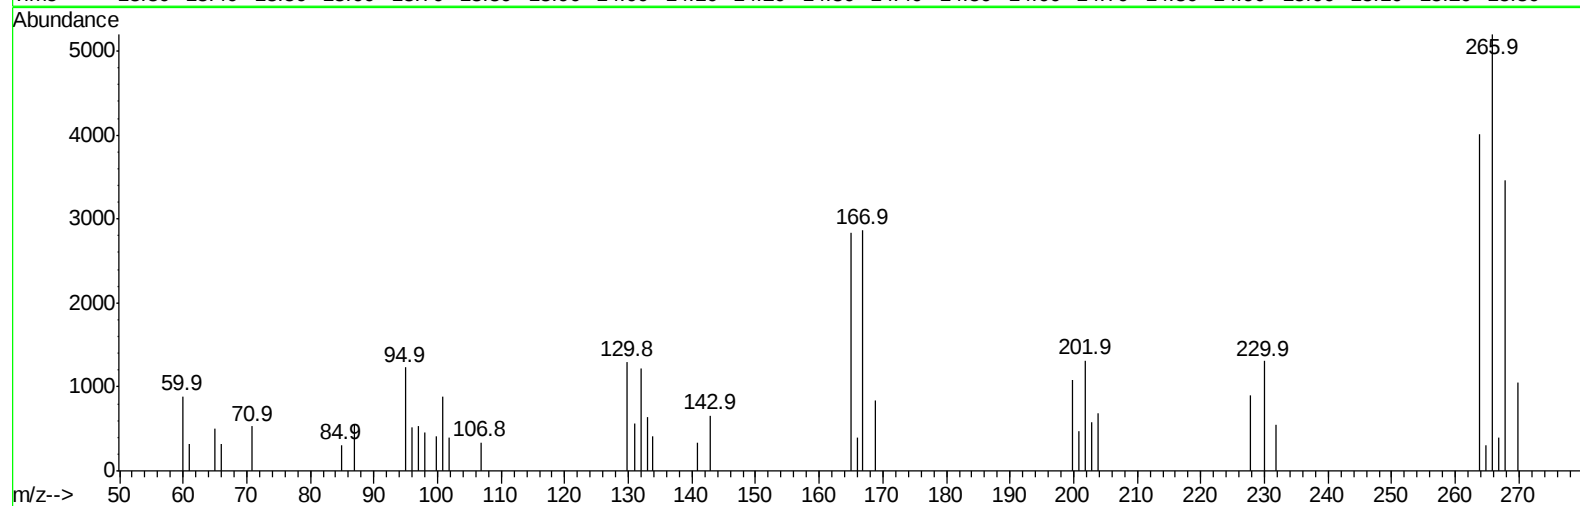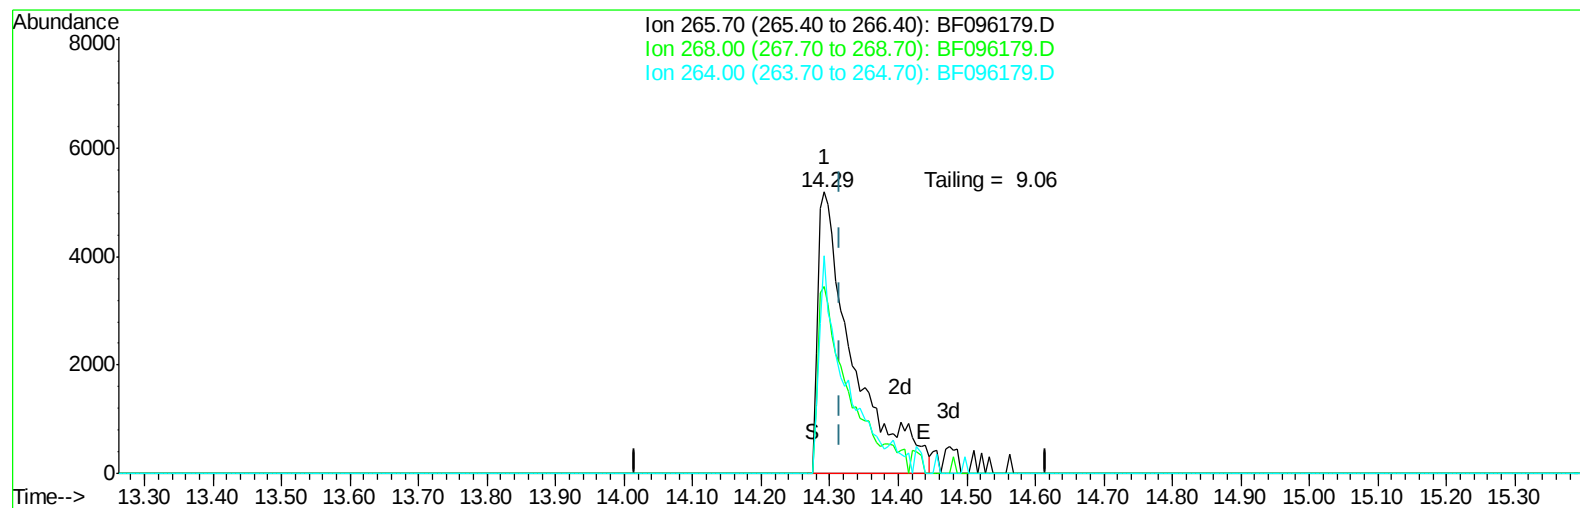

TIC: BF096179.D

(69) Pentachlorophenol (C)

14.292min (-0.024) 0.00ng

response 16960

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.45
264.00	64.60	77.15
0.00	0.00	0.00