
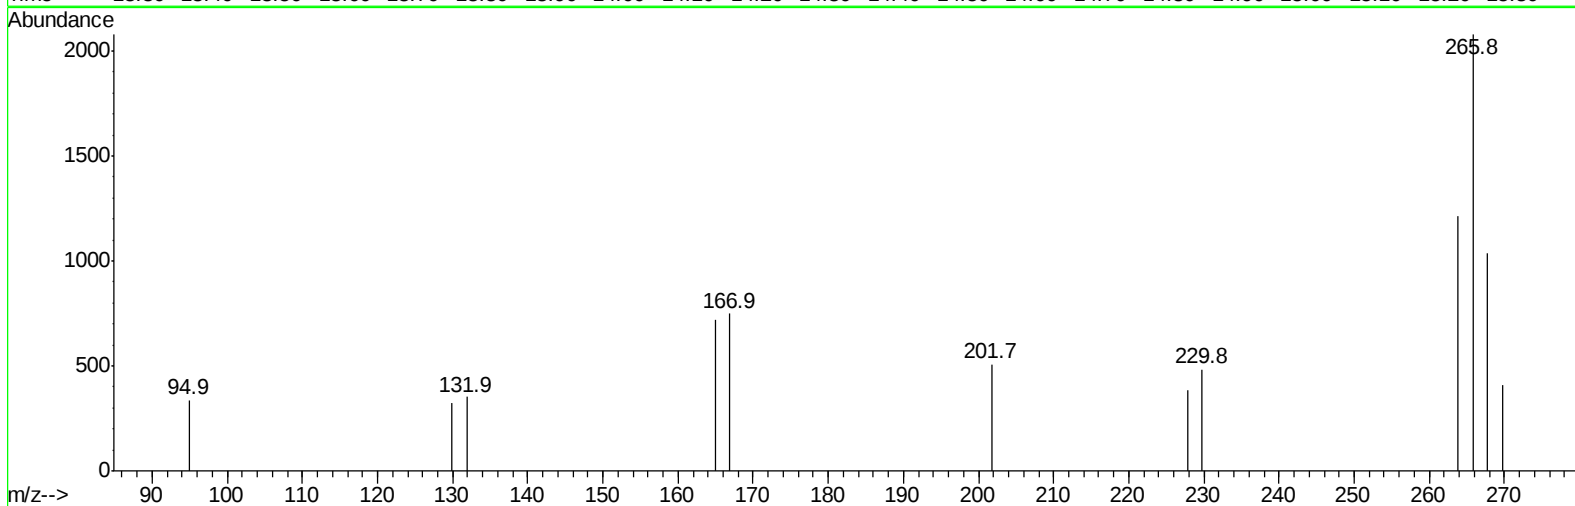


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096202.D
Acq On : 24 Jun 2017 23:28
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 09:01:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

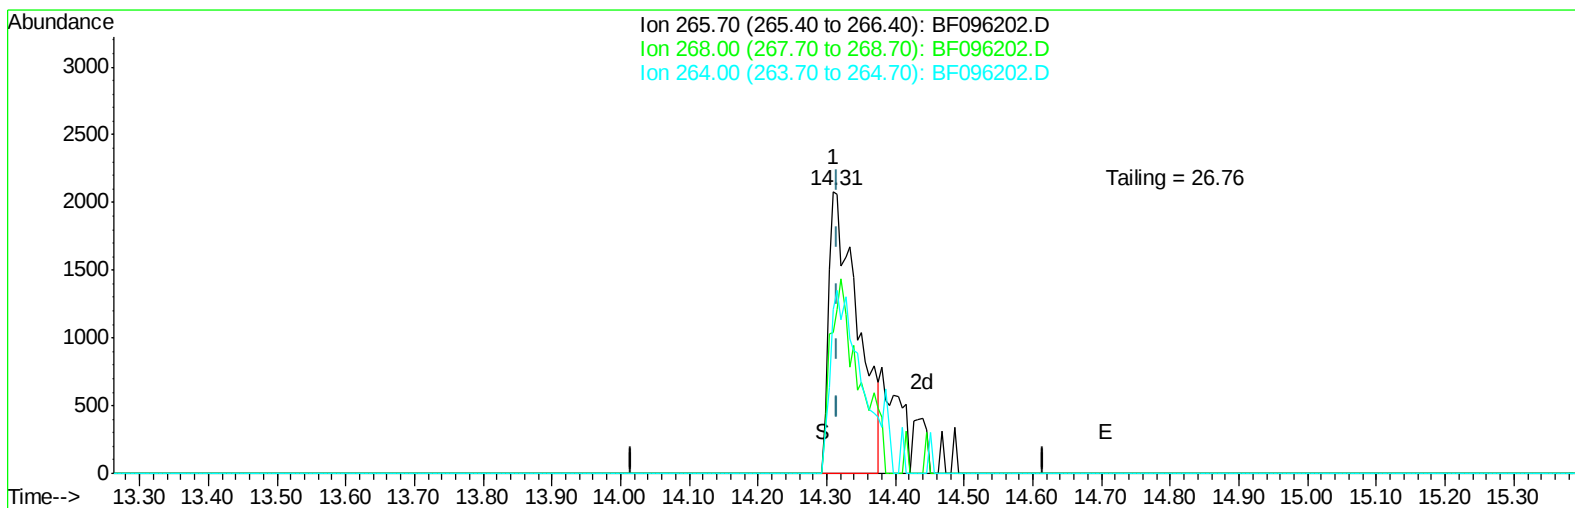

TIC: BF096202.D

(69) Pentachlorophenol (C)



14.309min (-0.006) 0.00ng m

response 6123

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	49.78#
264.00	64.60	58.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096202.D
Acq On : 24 Jun 2017 23:28
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 09:01:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

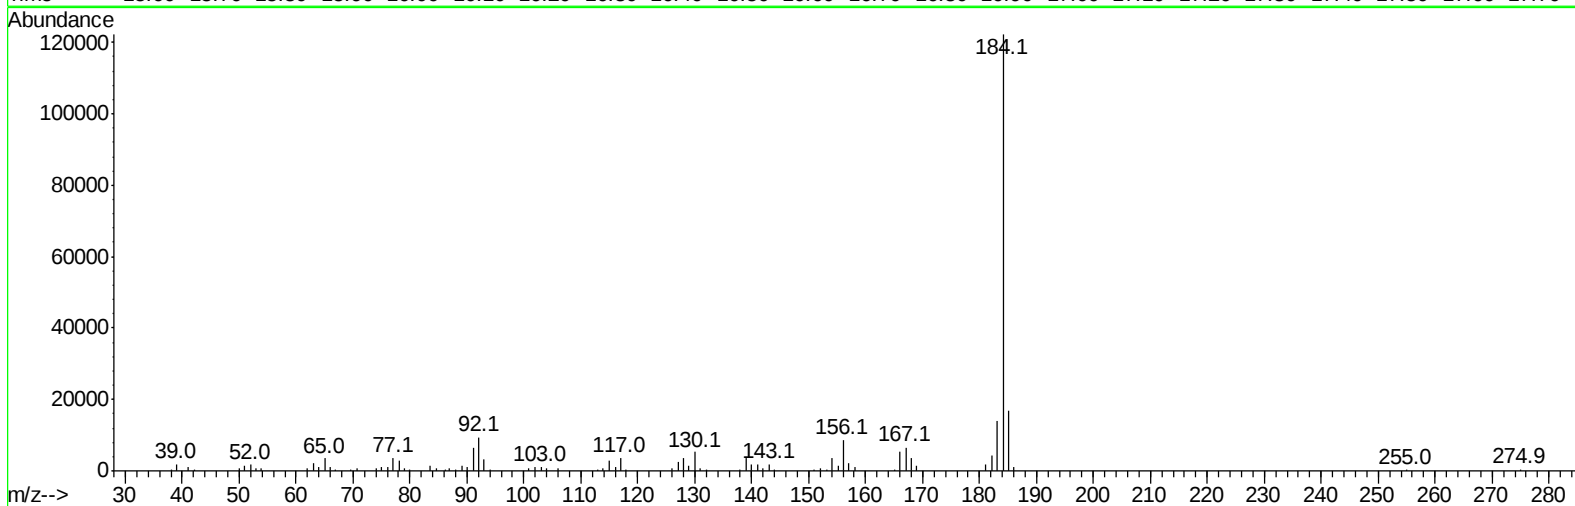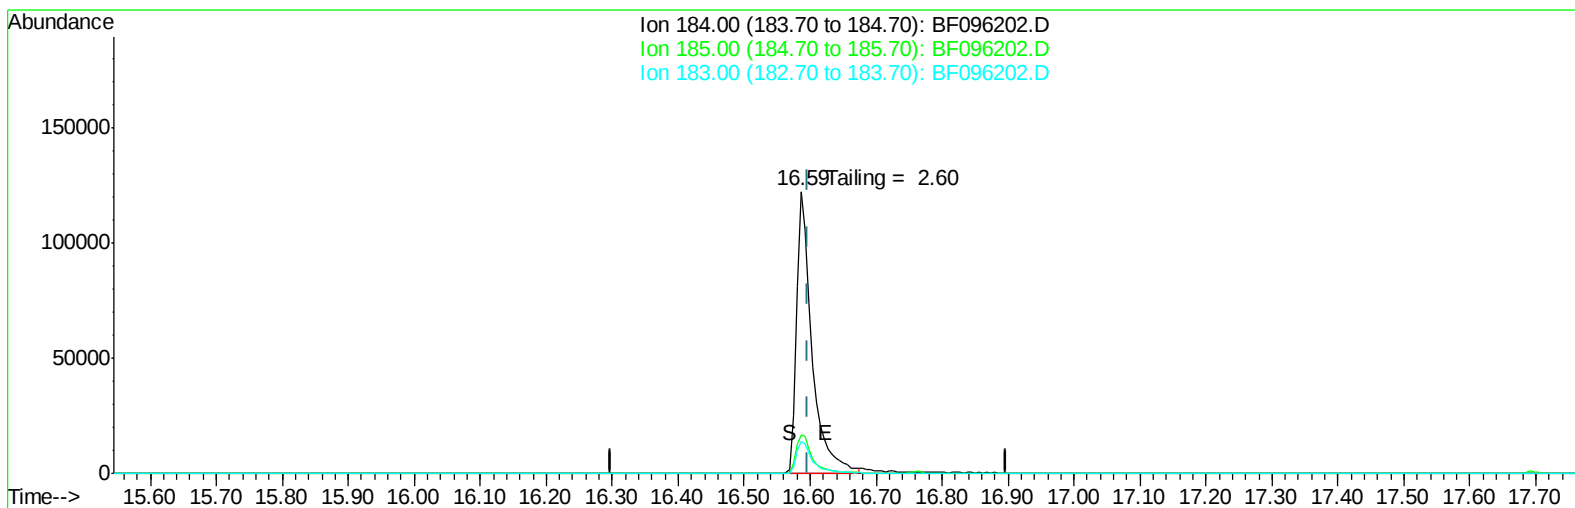

TIC: BF096202.D

(76) Benzidine

16.586min (-0.012) 0.00ng

response 205856

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.65#
183.00	12.20	11.48
0.00	0.00	0.00