

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
 Data File : BF096193.D
 Acq On : 24 Jun 2017 16:42
 Operator : SJ/MA
 Sample : I3851-07 4X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-34-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.546	7	10	25	rBV	62255	114540	29.06%	4.652%
2	7.016	935	940	947	rBV4	9793	27999	7.10%	1.137%
3	7.263	978	982	1003	rBV	184243	299515	75.99%	12.165%
4	7.516	1020	1025	1037	rBV	20793	38866	9.86%	1.579%
5	8.275	1151	1154	1159	rBV2	3849	7480	1.90%	0.304%
6	9.298	1324	1328	1348	rBV	251083	394151	100.00%	16.009%
7	11.086	1628	1632	1641	rBV	32393	49515	12.56%	2.011%
8	12.116	1803	1807	1826	rBV2	262795	376563	95.54%	15.294%
9	13.745	2080	2084	2085	rBV	4116	4437	1.13%	0.180%
10	14.474	2203	2208	2211	rBV	4309	6009	1.52%	0.244%
11	14.515	2211	2215	2229	rVB	228985	330021	83.73%	13.404%
12	15.162	2319	2325	2328	rBV2	3677	5315	1.35%	0.216%
13	15.774	2425	2429	2431	rBV2	4983	6150	1.56%	0.250%
14	16.327	2520	2523	2527	rBV2	6225	7038	1.79%	0.286%
15	16.668	2576	2581	2583	rBV5	7582	11541	2.93%	0.469%
16	16.903	2617	2621	2627	rBV	48757	61472	15.60%	2.497%
17	17.045	2643	2645	2649	rBV5	4040	4660	1.18%	0.189%
18	17.086	2650	2652	2654	rBV3	6744	4784	1.21%	0.194%
19	17.280	2680	2685	2687	rBV5	6367	11277	2.86%	0.458%
20	17.303	2687	2689	2693	rVV5	7416	10285	2.61%	0.418%
21	17.421	2706	2709	2712	rBV5	8204	11379	2.89%	0.462%
22	17.456	2712	2715	2718	rBV4	13220	18834	4.78%	0.765%
23	17.756	2763	2766	2768	rBV3	8004	8586	2.18%	0.349%
24	17.815	2774	2776	2778	rBV3	7682	5941	1.51%	0.241%
25	18.256	2847	2851	2858	rBV	289338	383284	97.24%	15.567%
26	19.933	3133	3136	3143	rBV	211389	262469	66.59%	10.660%


Sum of corrected areas: 2462111

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096193.D
Acq On : 24 Jun 2017 16:42
Operator : SJ/MA
Sample : I3851-07 4X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-34-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

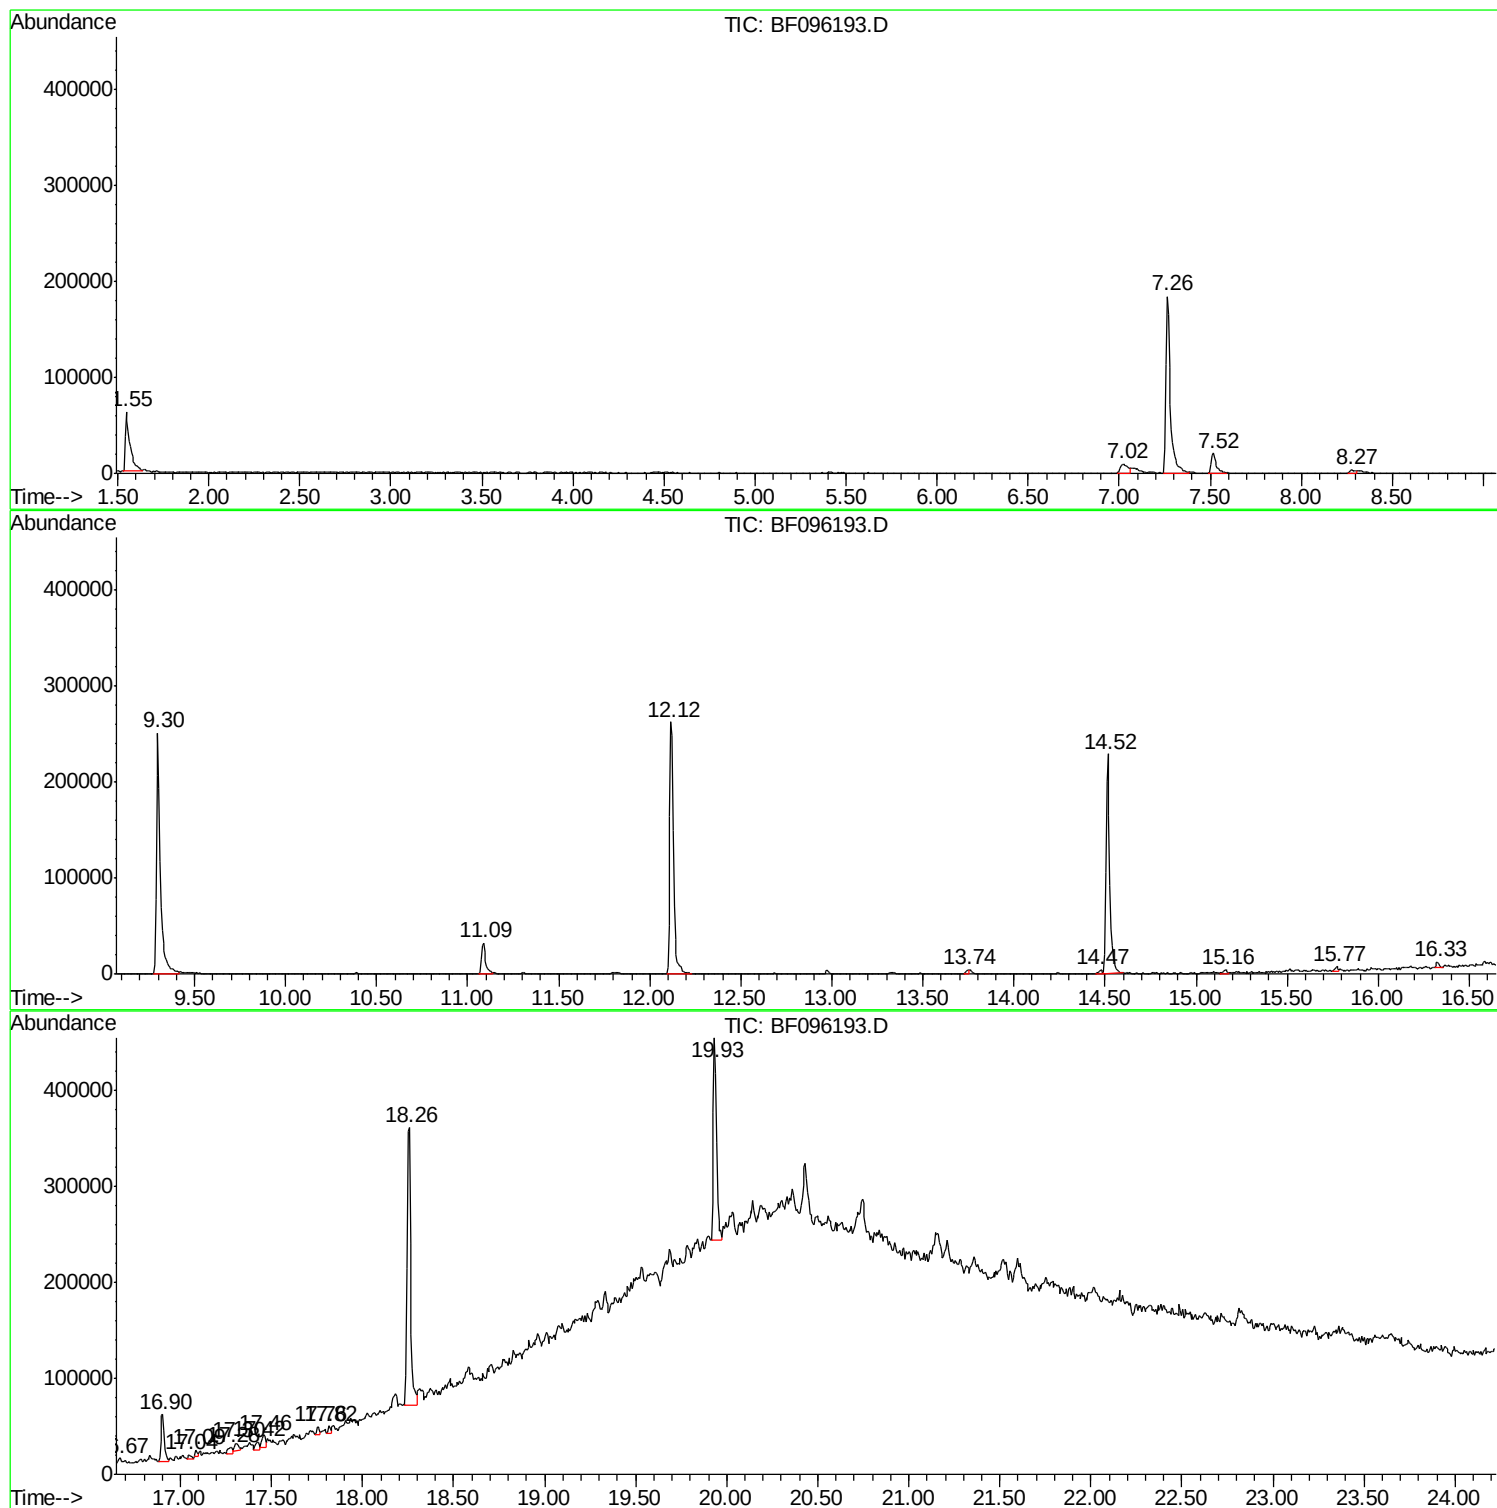

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data_File : BF096193.D
Acq_On : 24 Jun 2017 16:422
Operator : SJ/MAA
Sample : I3851-07.4XX
Misc :
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-34-0-1.5

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
