

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
 Data File : BF096194.D
 Acq On : 24 Jun 2017 17:15
 Operator : SJ/MA
 Sample : I3851-08 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-34-1.5-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.546	7	10	22	rBV	80104	150329	31.77%	3.407%
2	4.428	496	500	502	rBV2	5070	8178	1.73%	0.185%
3	5.204	629	632	651	rBV	30240	125905	26.61%	2.853%
4	6.904	918	921	926	rBV3	35610	83095	17.56%	1.883%
5	6.951	926	929	948	rVB	99131	292916	61.90%	6.638%
6	7.263	978	982	995	rBV	252439	349464	73.85%	7.920%
7	7.504	1018	1023	1044	rBV	105921	176930	37.39%	4.010%
8	8.216	1140	1144	1158	rBV2	28135	86657	18.31%	1.964%
9	8.310	1158	1160	1165	rVB2	5440	5981	1.26%	0.136%
10	9.298	1324	1328	1343	rBV	304690	458076	96.81%	10.381%
11	10.386	1509	1513	1518	rBB2	4063	4860	1.03%	0.110%
12	10.486	1528	1530	1537	rBV	3270	5979	1.26%	0.136%
13	10.633	1551	1555	1562	rBB	2957	5496	1.16%	0.125%
14	11.074	1626	1630	1651	rBV	177449	239592	50.63%	5.430%
15	11.304	1664	1669	1674	rBV2	5227	7102	1.50%	0.161%
16	11.615	1716	1722	1724	rBV2	2827	5000	1.06%	0.113%
17	11.651	1724	1728	1732	rVB4	3099	4778	1.01%	0.108%
18	11.786	1747	1751	1756	rBV	12203	22910	4.84%	0.519%
19	11.904	1768	1771	1777	rBV	3984	6241	1.32%	0.141%
20	11.980	1778	1784	1788	rVB5	3426	6305	1.33%	0.143%
21	12.115	1803	1807	1814	rBV2	312645	432298	91.36%	9.797%
22	12.686	1897	1904	1907	rVB3	3451	5212	1.10%	0.118%
23	12.974	1950	1953	1958	rVB	7749	9142	1.93%	0.207%
24	13.333	2011	2014	2019	rVB3	3916	6227	1.32%	0.141%
25	13.433	2027	2031	2040	rBV2	41366	73229	15.48%	1.660%
26	13.745	2077	2084	2086	rBV2	9821	15689	3.32%	0.356%
27	13.762	2086	2087	2091	rVB2	10560	10587	2.24%	0.240%
28	14.474	2203	2208	2210	rBV3	7861	11207	2.37%	0.254%
29	14.515	2210	2215	2229	rVB2	277757	411345	86.93%	9.322%
30	14.656	2237	2239	2245	rVB2	5247	7608	1.61%	0.172%
31	15.162	2319	2325	2330	rBV6	6693	11187	2.36%	0.254%
32	15.339	2352	2355	2358	rVB3	4071	5168	1.09%	0.117%
33	15.380	2358	2362	2367	rBV2	8049	13136	2.78%	0.298%
34	15.492	2377	2381	2384	rBV4	5179	8128	1.72%	0.184%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096194.D
Acq On : 24 Jun 2017 17:15
Operator : SJ/MA
Sample : I3851-08 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-34-1.5-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.533	2384	2388	2390	rBV3	6200	8071	1.71%	0.183%
36	15.774	2425	2429	2434	rBV6	6422	10235	2.16%	0.232%
37	16.003	2465	2468	2472	rVB6	4146	5266	1.11%	0.119%
38	16.045	2472	2475	2477	rBV3	3501	4862	1.03%	0.110%
39	16.145	2488	2492	2495	rBV6	8576	11392	2.41%	0.258%
40	16.180	2495	2498	2504	rVV6	5049	9572	2.02%	0.217%
41	16.262	2508	2512	2516	rVV4	7040	9042	1.91%	0.205%
42	16.327	2519	2523	2524	rBV2	8232	7884	1.67%	0.179%
43	16.350	2524	2527	2532	rVB	42809	50530	10.68%	1.145%
44	16.456	2542	2545	2549	rVB5	4323	6108	1.29%	0.138%
45	16.592	2565	2568	2572	rBV4	4170	6878	1.45%	0.156%
46	16.656	2575	2579	2586	rVV	52684	70284	14.85%	1.593%
47	16.845	2608	2611	2616	rBV5	4452	8803	1.86%	0.200%
48	16.897	2616	2620	2626	rVB	179780	206393	43.62%	4.677%
49	16.980	2629	2634	2637	rBV6	7866	14122	2.98%	0.320%
50	17.045	2642	2645	2646	rBV3	4903	4847	1.02%	0.110%
51	17.109	2649	2656	2659	rBV8	11402	25875	5.47%	0.586%
52	17.262	2680	2682	2688	rBV5	8872	11737	2.48%	0.266%
53	17.309	2688	2690	2694	rVB5	4989	5609	1.19%	0.127%
54	17.380	2697	2702	2705	rBV5	6199	11407	2.41%	0.259%
55	17.456	2713	2715	2720	rVB6	6803	6119	1.29%	0.139%
56	18.109	2824	2826	2831	rBV6	10603	13566	2.87%	0.307%
57	18.168	2833	2836	2840	rVV6	12477	19445	4.11%	0.441%
58	18.256	2846	2851	2856	rBV	348664	473176	100.00%	10.723%
59	18.327	2860	2863	2867	rVB	45237	52689	11.14%	1.194%
60	19.933	3132	3136	3141	rBV	232210	292657	61.85%	6.632%


Sum of corrected areas: 4412526

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096194.D
Acq On : 24 Jun 2017 17:15
Operator : SJ/MA
Sample : I3851-08 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-34-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

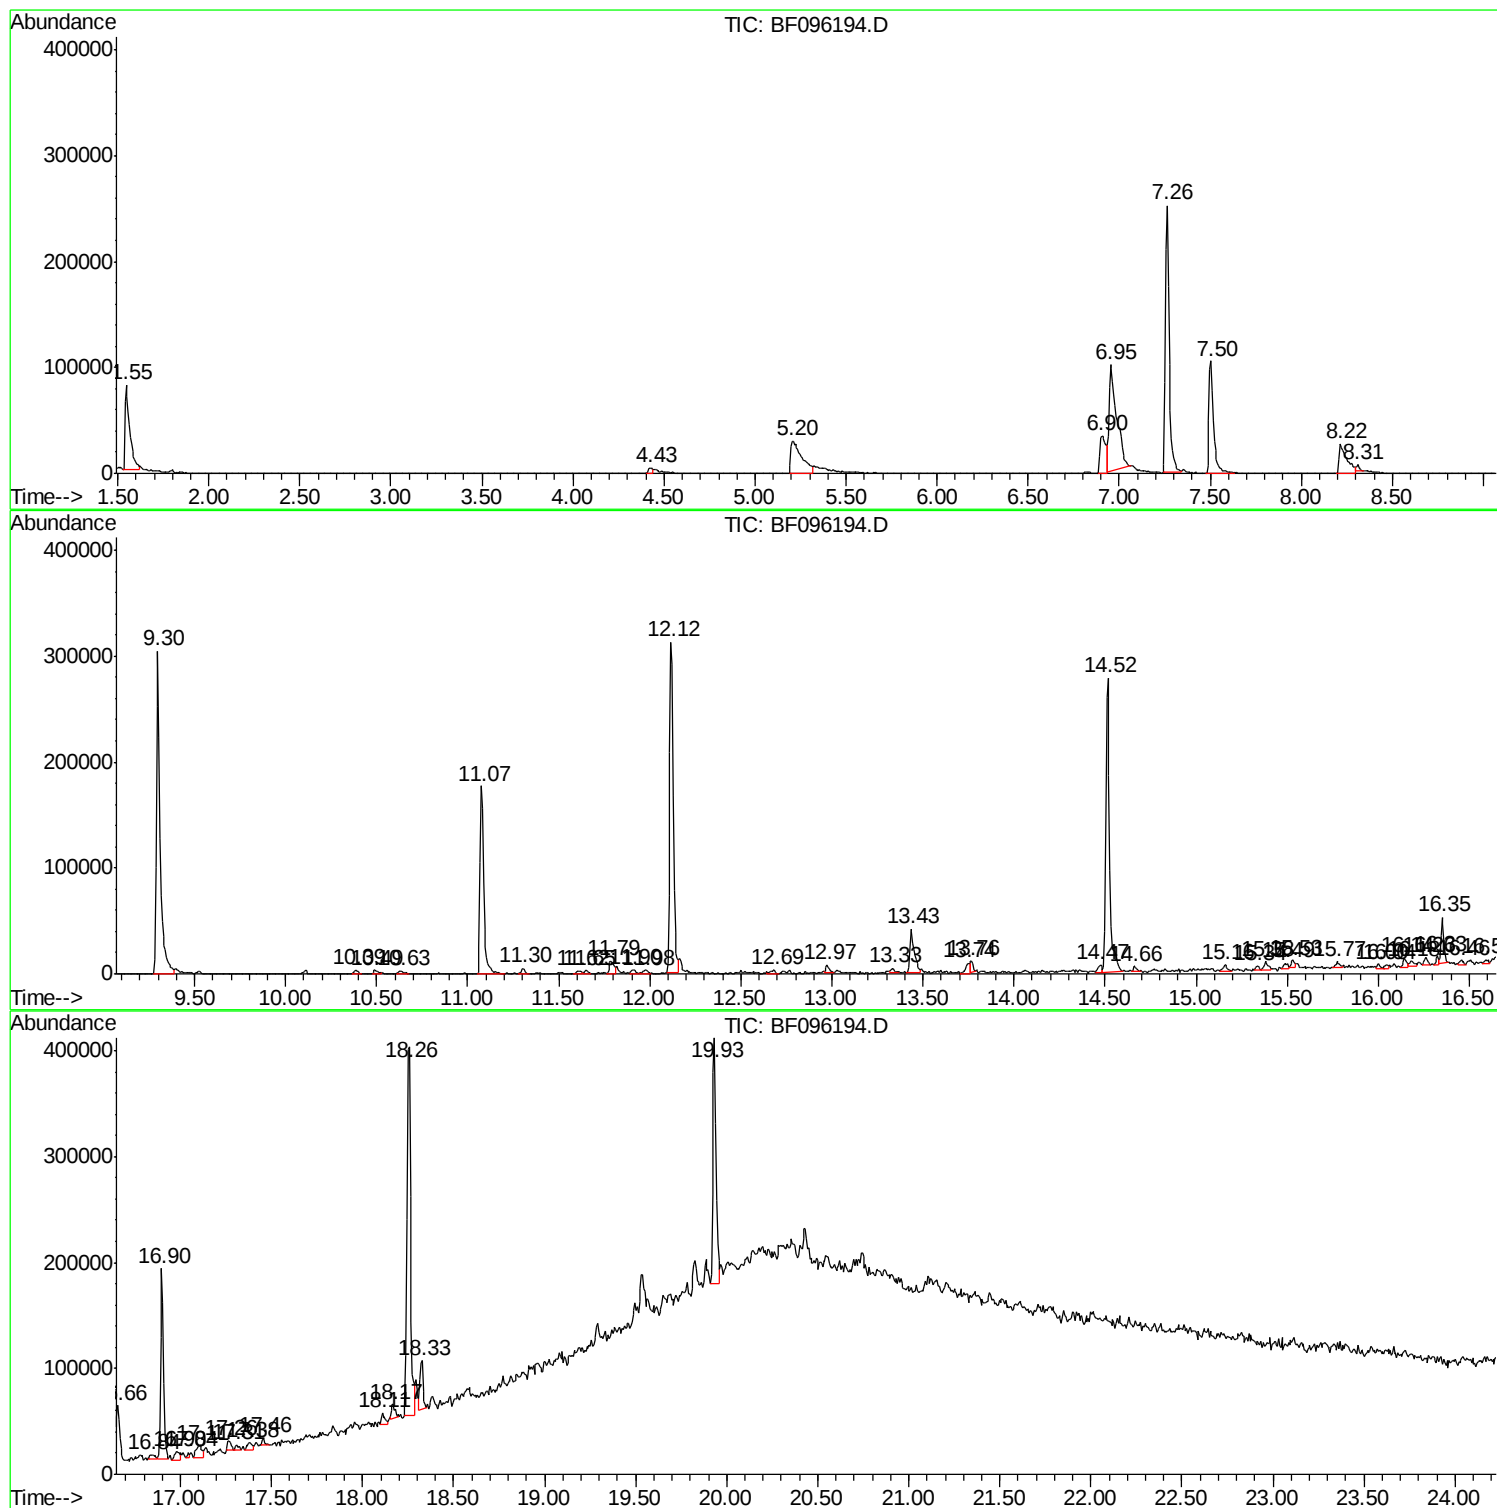

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data_File : BF096194.D
Acq_On : 24 Jun 2017 17:155
Operator : SJ/MAA
Sample : I3851-08_5XX
Misc :
ALS_Vial : 16 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-34-1.5-3

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
