

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
 Data File : BF096195.D
 Acq On : 24 Jun 2017 17:47
 Operator : SJ/MA
 Sample : I3851-03 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-30-0-1.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.546	7	10	34	rVB	258362	507833	100.00%	15.249%
2	4.428	496	500	503	rBV2	3493	6388	1.26%	0.192%
3	5.245	637	639	640	rBV	7767	6897	1.36%	0.207%
4	6.951	925	929	930	rBV2	12787	18788	3.70%	0.564%
5	6.975	930	933	942	rVV2	34163	86617	17.06%	2.601%
6	7.263	978	982	996	rBV	215557	328225	64.63%	9.856%
7	7.504	1019	1023	1034	rBV	49639	84409	16.62%	2.535%
8	8.239	1145	1148	1152	rBV3	8844	16755	3.30%	0.503%
9	9.298	1324	1328	1345	rBV	285481	425557	83.80%	12.778%
10	11.080	1627	1631	1650	rBB	82986	121460	23.92%	3.647%
11	12.116	1803	1807	1821	rBV2	291562	411821	81.09%	12.366%
12	13.457	2031	2035	2039	rBV2	5407	8616	1.70%	0.259%
13	13.745	2080	2084	2086	rBV	4724	6897	1.36%	0.207%
14	13.763	2086	2087	2091	rVB3	5512	5608	1.10%	0.168%
15	14.474	2203	2208	2210	rBV2	4959	5714	1.13%	0.172%
16	14.515	2210	2215	2227	rVB	258214	365573	71.99%	10.977%
17	15.162	2321	2325	2328	rBV2	3872	5301	1.04%	0.159%
18	16.362	2525	2529	2534	rVV	10947	14102	2.78%	0.423%
19	16.662	2576	2580	2586	rBV	17439	26523	5.22%	0.796%
20	16.898	2617	2620	2627	rBV	105497	118400	23.31%	3.555%
21	16.986	2631	2635	2638	rBV5	5910	10142	2.00%	0.305%
22	17.274	2680	2684	2685	rBV4	5771	7447	1.47%	0.224%
23	17.315	2689	2691	2694	rVB4	6835	6115	1.20%	0.184%
24	17.415	2706	2708	2711	rBV4	7405	8858	1.74%	0.266%
25	17.456	2712	2715	2717	rBV4	6601	7305	1.44%	0.219%
26	17.756	2763	2766	2769	rBV5	11141	13931	2.74%	0.418%
27	18.256	2846	2851	2860	rBV	319487	433625	85.39%	13.020%
28	19.933	3133	3136	3141	rBV	218751	271448	53.45%	8.151%


Sum of corrected areas: 3330355

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096195.D
Acq On : 24 Jun 2017 17:47
Operator : SJ/MA
Sample : I3851-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-30-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

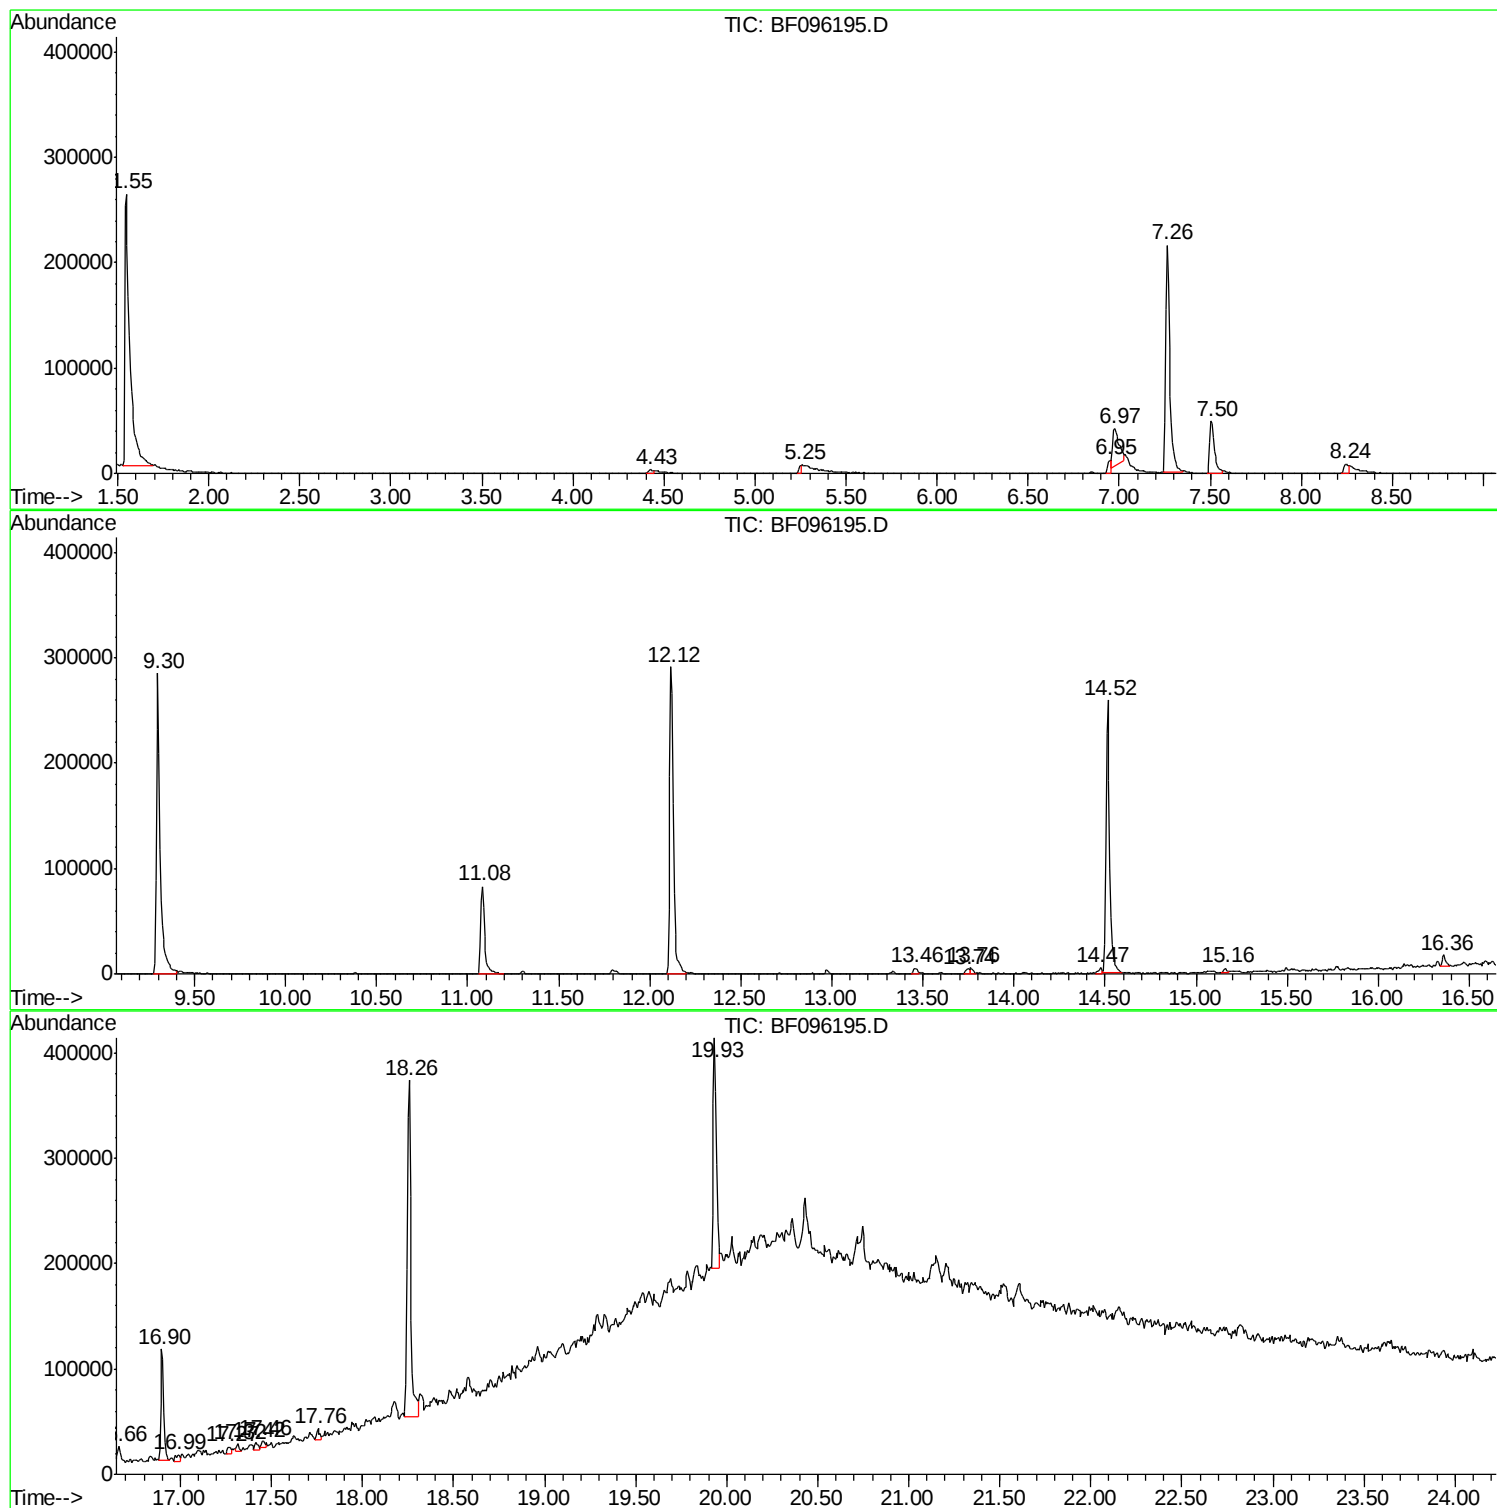

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data_File : BF096195.D
Acq_On : 24 Jun 2017 17:477
Operator : SJ/MAA
Sample : I3851-03_5XX
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-30-0-1.5

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
