

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
 Data File : BF096197.D
 Acq On : 24 Jun 2017 18:52
 Operator : SJ/MA
 Sample : I3851-12 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-35-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.546	7	10	36	rVB	164358	314393	74.94%	11.755%
2	7.004	935	938	945	rBV6	11910	34432	8.21%	1.287%
3	7.087	951	952	959	rVB2	4946	5098	1.22%	0.191%
4	7.263	978	982	998	rBV	192994	315568	75.22%	11.799%
5	7.510	1021	1024	1040	rBB	17572	34256	8.17%	1.281%
6	9.298	1324	1328	1352	rBV	273240	419527	100.00%	15.686%
7	11.086	1628	1632	1646	rBV	28511	44121	10.52%	1.650%
8	12.116	1803	1807	1825	rBV2	289268	407565	97.15%	15.239%
9	13.463	2033	2036	2044	rBB2	2920	5193	1.24%	0.194%
10	14.516	2210	2215	2228	rVB	247353	356086	84.88%	13.314%
11	16.904	2617	2621	2625	rBV	46106	53850	12.84%	2.013%
12	17.274	2680	2684	2685	rBV4	3523	4411	1.05%	0.165%
13	17.362	2695	2699	2701	rBV5	3259	4549	1.08%	0.170%
14	17.451	2712	2714	2718	rBV5	6390	9071	2.16%	0.339%
15	17.486	2718	2720	2723	rVB4	5049	4945	1.18%	0.185%
16	18.256	2847	2851	2860	rBV	314342	395834	94.35%	14.800%
17	18.351	2865	2867	2868	rBV2	7844	4527	1.08%	0.169%
18	19.933	3133	3136	3142	rBV	206794	261111	62.24%	9.763%


Sum of corrected areas: 2674537

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096197.D
Acq On : 24 Jun 2017 18:52
Operator : SJ/MA
Sample : I3851-12 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-35-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

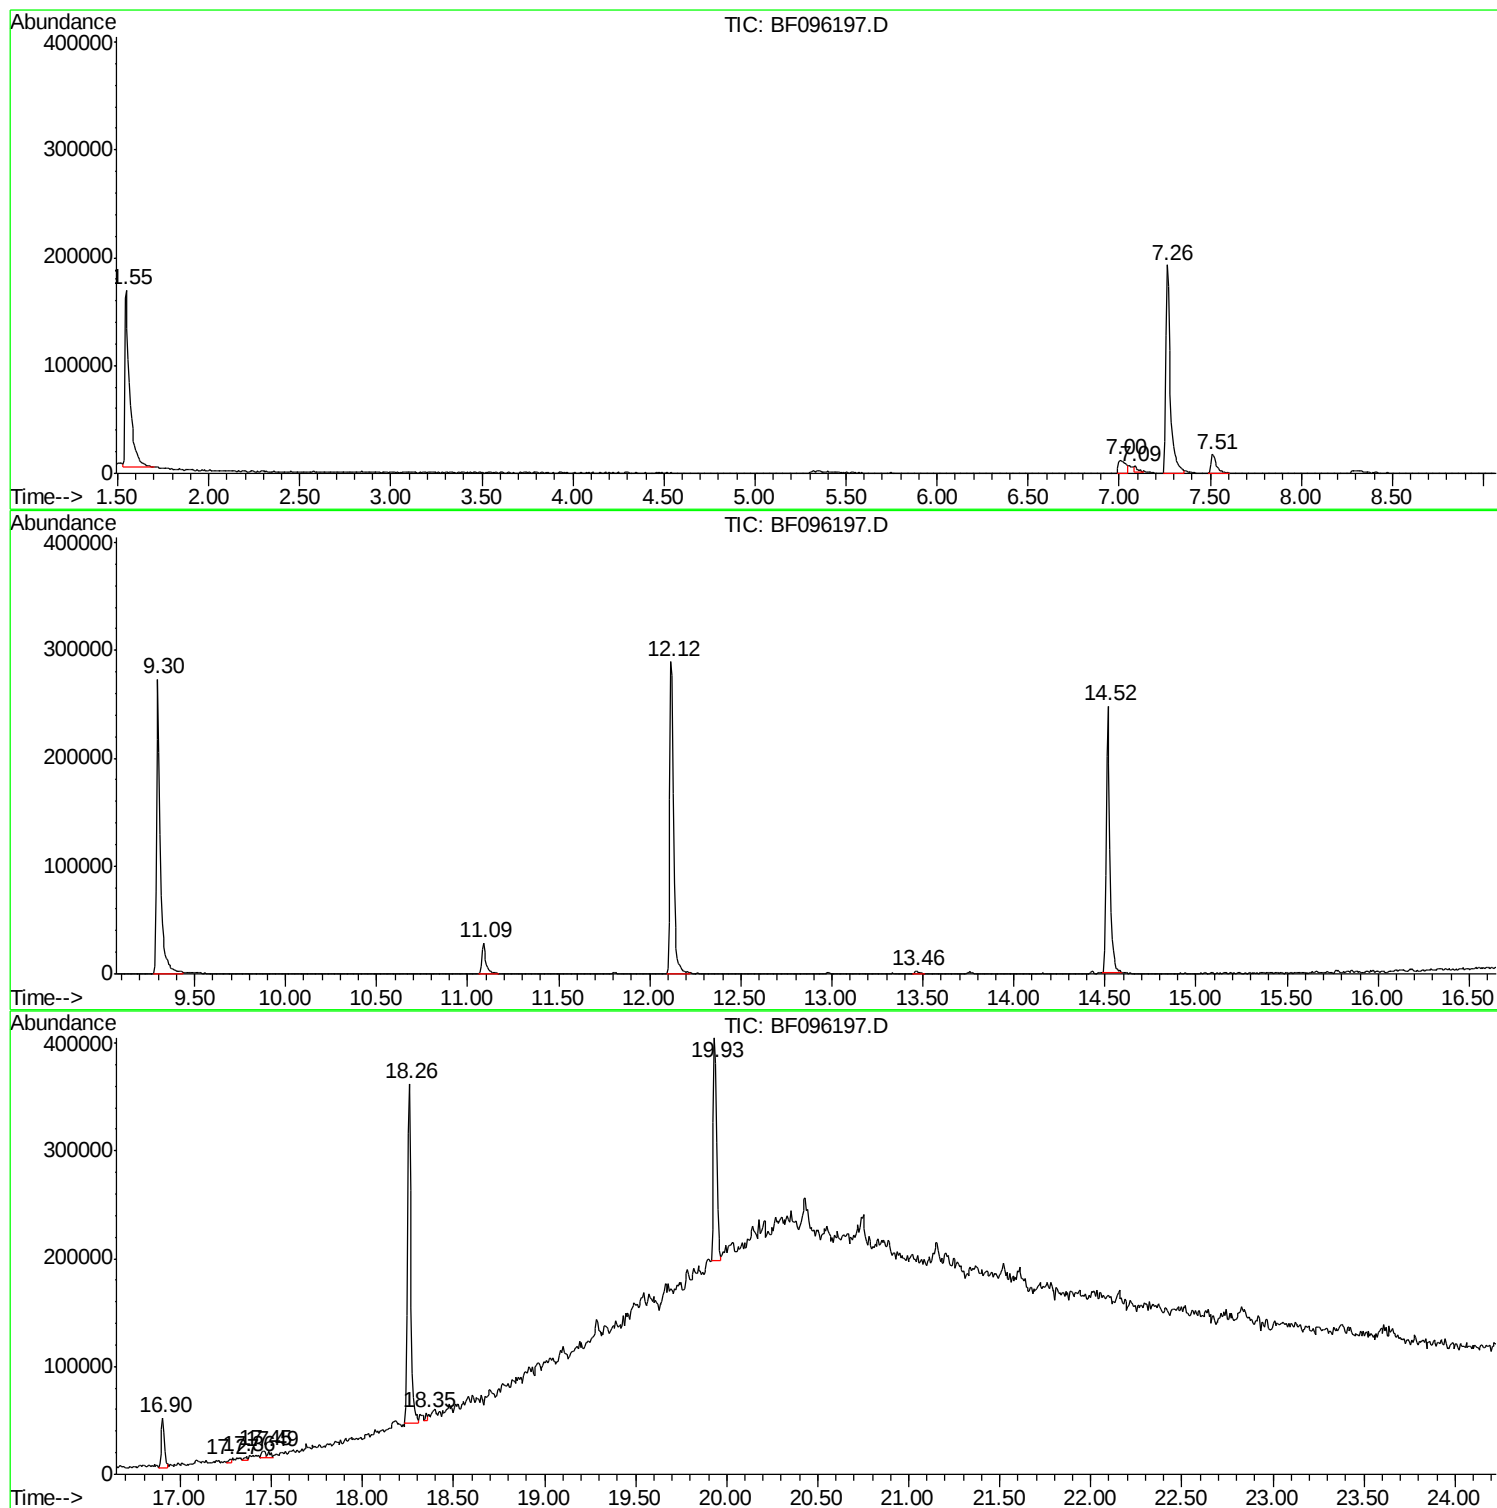

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data_File : BF096197.D
Acq_On : 24 Jun 2017 18:522
Operator : SJ/MAA
Sample : I3851-12_10XX
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-35-1.5-3

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
