

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
 Data File : BF096198.D
 Acq On : 24 Jun 2017 19:25
 Operator : SJ/MA
 Sample : I3851-02 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-26-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.540	7	9	39	rVB	599394	1121129	100.00%	31.067%
2	6.987	929	935	939	rBV5	23887	52638	4.70%	1.459%
3	7.263	979	982	996	rBV	181411	297747	26.56%	8.251%
4	7.510	1020	1024	1042	rBV3	28045	54354	4.85%	1.506%
5	8.257	1148	1151	1157	rBV2	5271	12692	1.13%	0.352%
6	9.298	1324	1328	1343	rBV	257564	386047	34.43%	10.698%
7	11.080	1627	1631	1638	rBV	62635	76414	6.82%	2.117%
8	11.822	1750	1757	1762	rVB4	8654	14857	1.33%	0.412%
9	12.116	1803	1807	1814	rBV2	269446	368972	32.91%	10.224%
10	13.339	2008	2015	2018	rBV	8014	13501	1.20%	0.374%
11	13.451	2030	2034	2040	rBV5	11192	21011	1.87%	0.582%
12	13.768	2079	2088	2094	rBV2	20301	36445	3.25%	1.010%
13	14.515	2211	2215	2221	rBV	252627	350251	31.24%	9.706%
14	15.380	2358	2362	2369	rVB5	6658	13116	1.17%	0.363%
15	16.145	2488	2492	2494	rBV5	10050	13089	1.17%	0.363%
16	16.357	2525	2528	2533	rBV	20672	27349	2.44%	0.758%
17	16.662	2576	2580	2585	rVB2	25548	34552	3.08%	0.957%
18	16.904	2617	2621	2626	rVV	71797	88689	7.91%	2.458%
19	17.104	2650	2655	2656	rBV5	8902	14631	1.31%	0.405%
20	18.256	2847	2851	2858	rBV	285085	363772	32.45%	10.080%
21	19.933	3133	3136	3142	rVB	191375	247462	22.07%	6.857%


Sum of corrected areas: 3608718

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096198.D
Acq On : 24 Jun 2017 19:25
Operator : SJ/MA
Sample : I3851-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-26-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

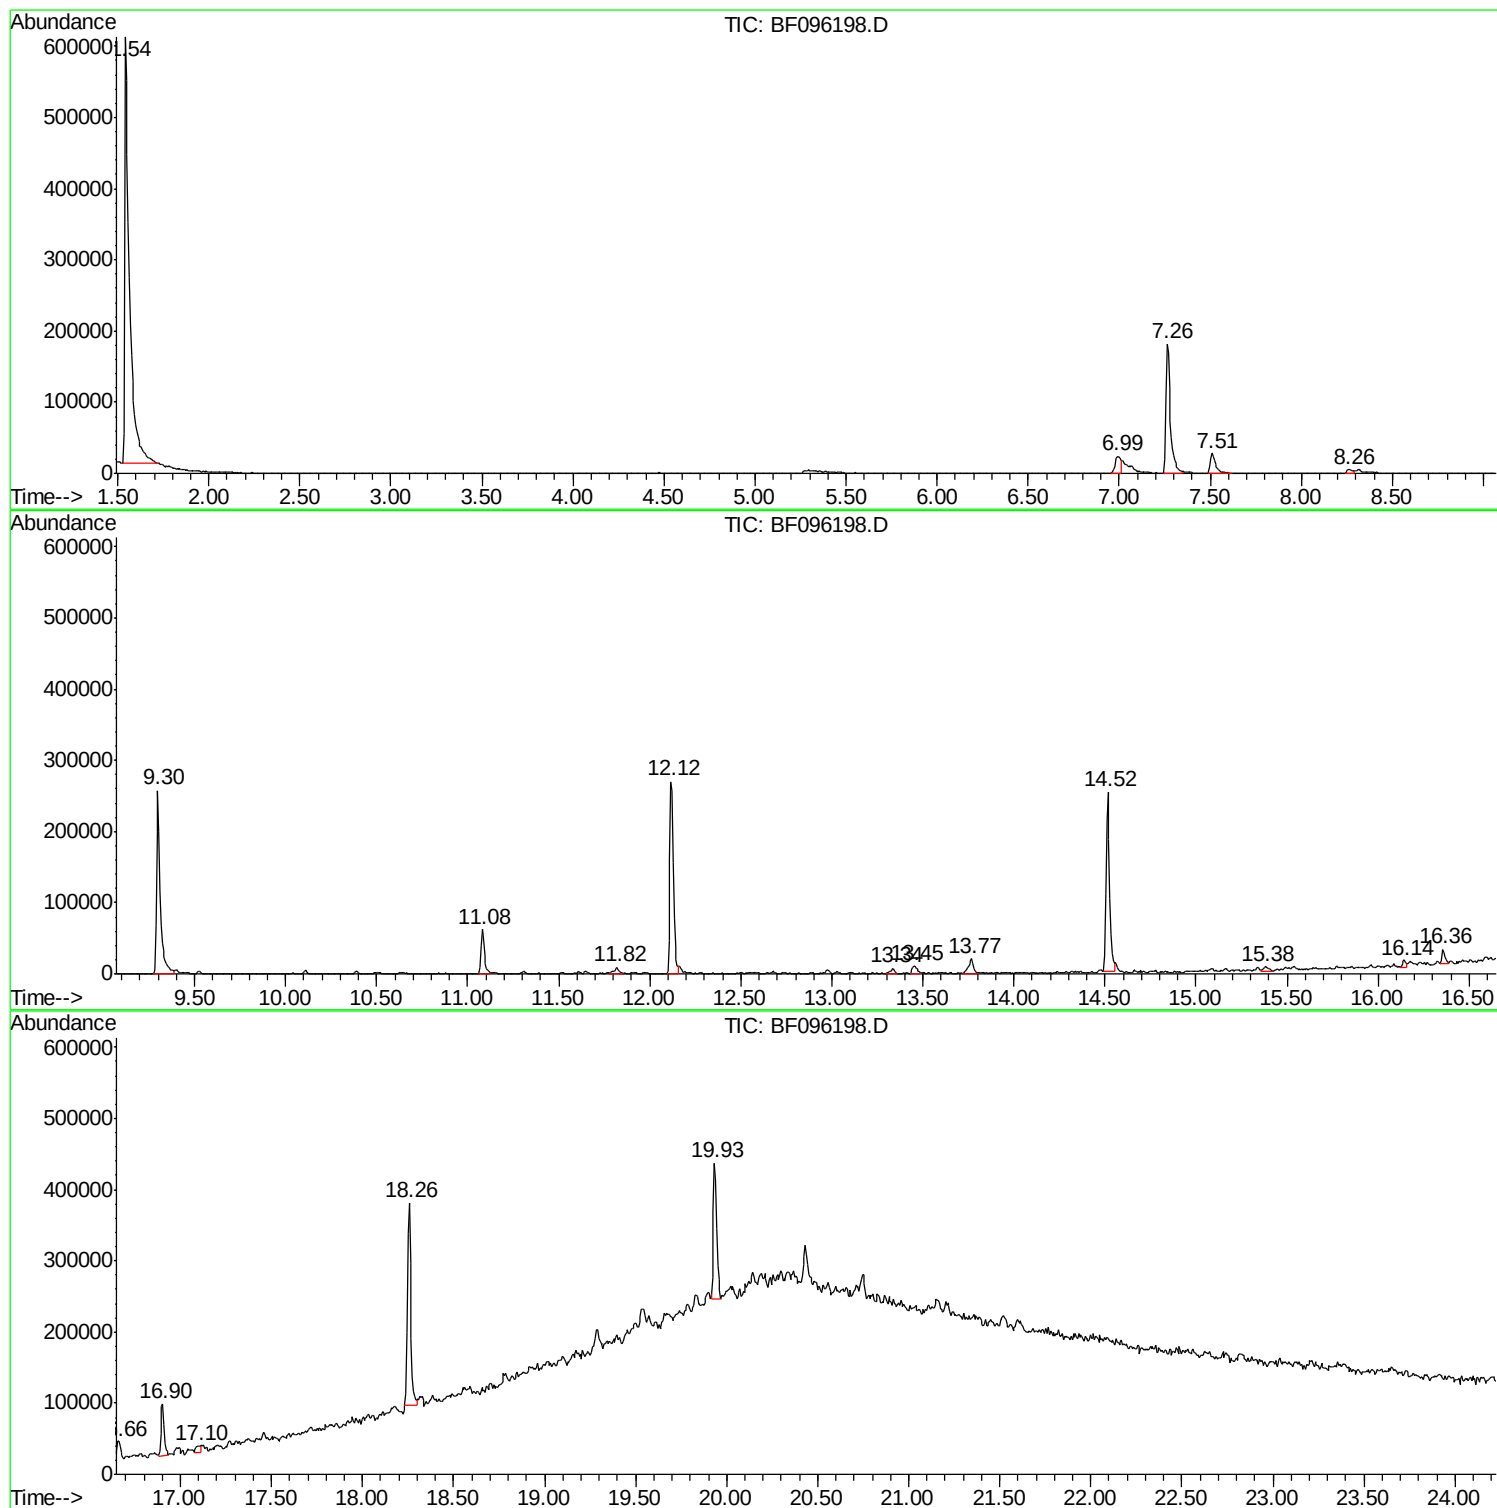

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096198.D
Acq On : 24 Jun 2017 19:25
Operator : SJ/MA
Sample : I3851-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
G-26-1.5-3

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Hexadecane, 2,6,11,15-tetra... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.77	2.08 ng	36445	Phenanthrene-d10	14.52	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexadecane, 2,6,11,15-tetramethyl-	282	C20H42	000504-44-9	86
2	Dodecane, 2,6,11-trimethyl-	212	C15H32	031295-56-4	72
3	Heptadecane, 7-methyl-	254	C18H38	020959-33-5	64
4	Dodecane, 2,7,10-trimethyl-	212	C15H32	074645-98-0	64
5	Dodecane, 2,6,10-trimethyl-	212	C15H32	003891-98-3	59

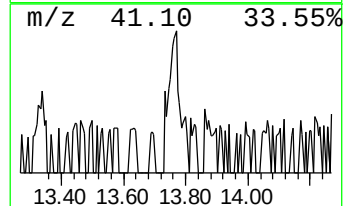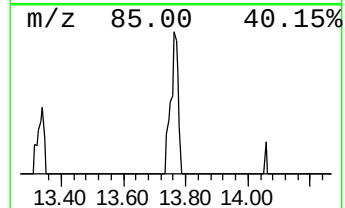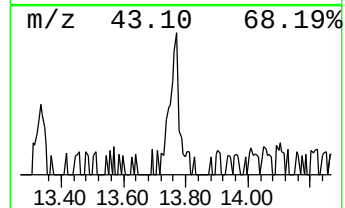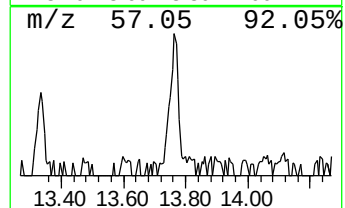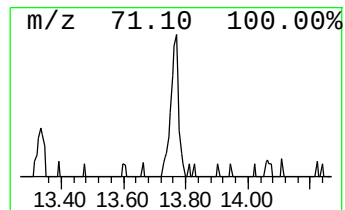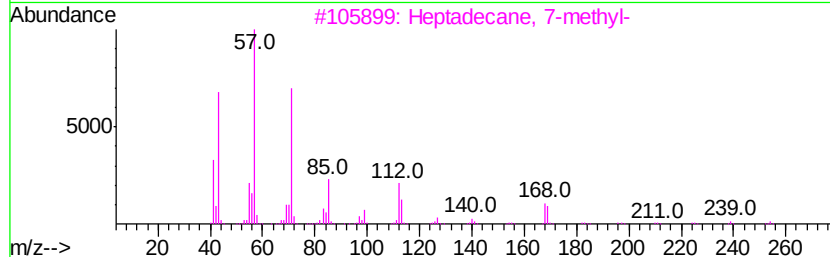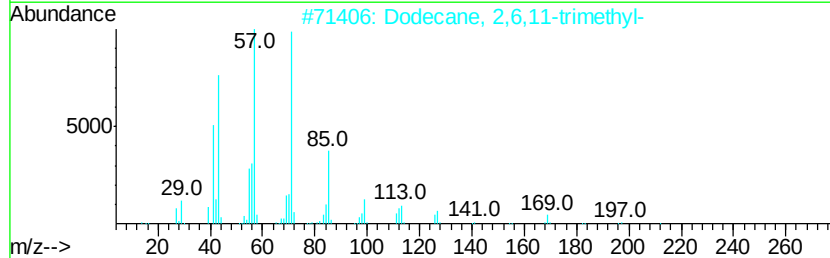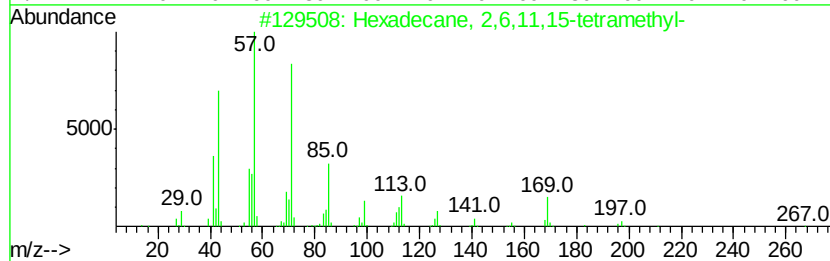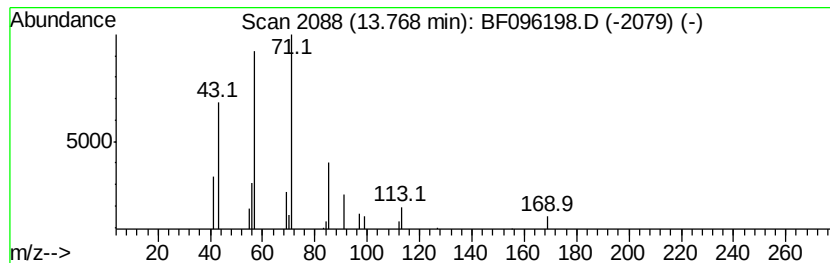

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096198.D
Acq On : 24 Jun 2017 19:25
Operator : SJ/MA
Sample : I3851-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-26-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexadecane, 2,6,1...	13.77	2.1	ng	36445	4	14.52	350251	20.0