

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
 Data File : BF096200.D
 Acq On : 24 Jun 2017 20:30
 Operator : SJ/MA
 Sample : I3852-06 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-31-1.5-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.546	8	10	36	rVB	90298	175300	41.53%	6.325%
2	7.022	935	941	942	rBV3	10991	19833	4.70%	0.716%
3	7.098	952	954	961	rVB4	3763	6101	1.45%	0.220%
4	7.263	979	982	1006	rVB	193583	319158	75.61%	11.516%
5	7.516	1021	1025	1037	rBV2	16340	32541	7.71%	1.174%
6	9.298	1324	1328	1341	rBV	276913	412139	97.64%	14.871%
7	11.086	1628	1632	1642	rBV	27723	43458	10.30%	1.568%
8	11.827	1754	1758	1762	rVB3	4726	6216	1.47%	0.224%
9	12.122	1803	1808	1824	rBV2	288608	422105	100.00%	15.231%
10	13.333	2009	2014	2018	rBB3	3994	5814	1.38%	0.210%
11	13.457	2032	2035	2042	rBB3	4710	8016	1.90%	0.289%
12	13.763	2081	2087	2092	rBV2	8487	15300	3.62%	0.552%
13	14.516	2211	2215	2229	rVB	278506	395204	93.63%	14.260%
14	15.086	2308	2312	2315	rBV3	3407	5596	1.33%	0.202%
15	15.339	2353	2355	2358	rBV2	3143	4309	1.02%	0.155%
16	15.786	2426	2431	2434	rBV6	3854	6211	1.47%	0.224%
17	15.833	2434	2439	2442	rVV5	3573	5659	1.34%	0.204%
18	15.957	2457	2460	2465	rBV5	4280	7225	1.71%	0.261%
19	16.145	2488	2492	2495	rBV5	5407	8225	1.95%	0.297%
20	16.227	2504	2506	2509	rBV3	3974	4660	1.10%	0.168%
21	16.333	2520	2524	2526	rBV4	4969	7576	1.79%	0.273%
22	16.362	2526	2529	2532	rBV2	9497	10373	2.46%	0.374%
23	16.462	2545	2546	2551	rVB5	4931	6196	1.47%	0.224%
24	16.510	2551	2554	2559	rBV5	5561	9774	2.32%	0.353%
25	16.586	2565	2567	2572	rBV6	4480	7476	1.77%	0.270%
26	16.674	2577	2582	2584	rBV4	11824	16625	3.94%	0.600%
27	16.780	2595	2600	2602	rBV5	8246	12778	3.03%	0.461%
28	16.904	2617	2621	2628	rVB	49072	63751	15.10%	2.300%
29	16.986	2632	2635	2640	rVB6	14837	17084	4.05%	0.616%
30	17.098	2651	2654	2659	rBV6	9395	20355	4.82%	0.734%
31	17.274	2679	2684	2686	rBV5	10785	18825	4.46%	0.679%
32	17.362	2697	2699	2703	rBV5	10830	18379	4.35%	0.663%
33	18.256	2847	2851	2859	rBV	310750	400720	94.93%	14.459%
34	19.939	3133	3137	3143	rBV	202514	258383	61.21%	9.323%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062417\
Data File : BF096200.D
Acq On : 24 Jun 2017 20:30
Operator : SJ/MA
Sample : I3852-06 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-1.5-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 2771365

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096200.D
Acq On : 24 Jun 2017 20:30
Operator : SJ/MA
Sample : I3852-06 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

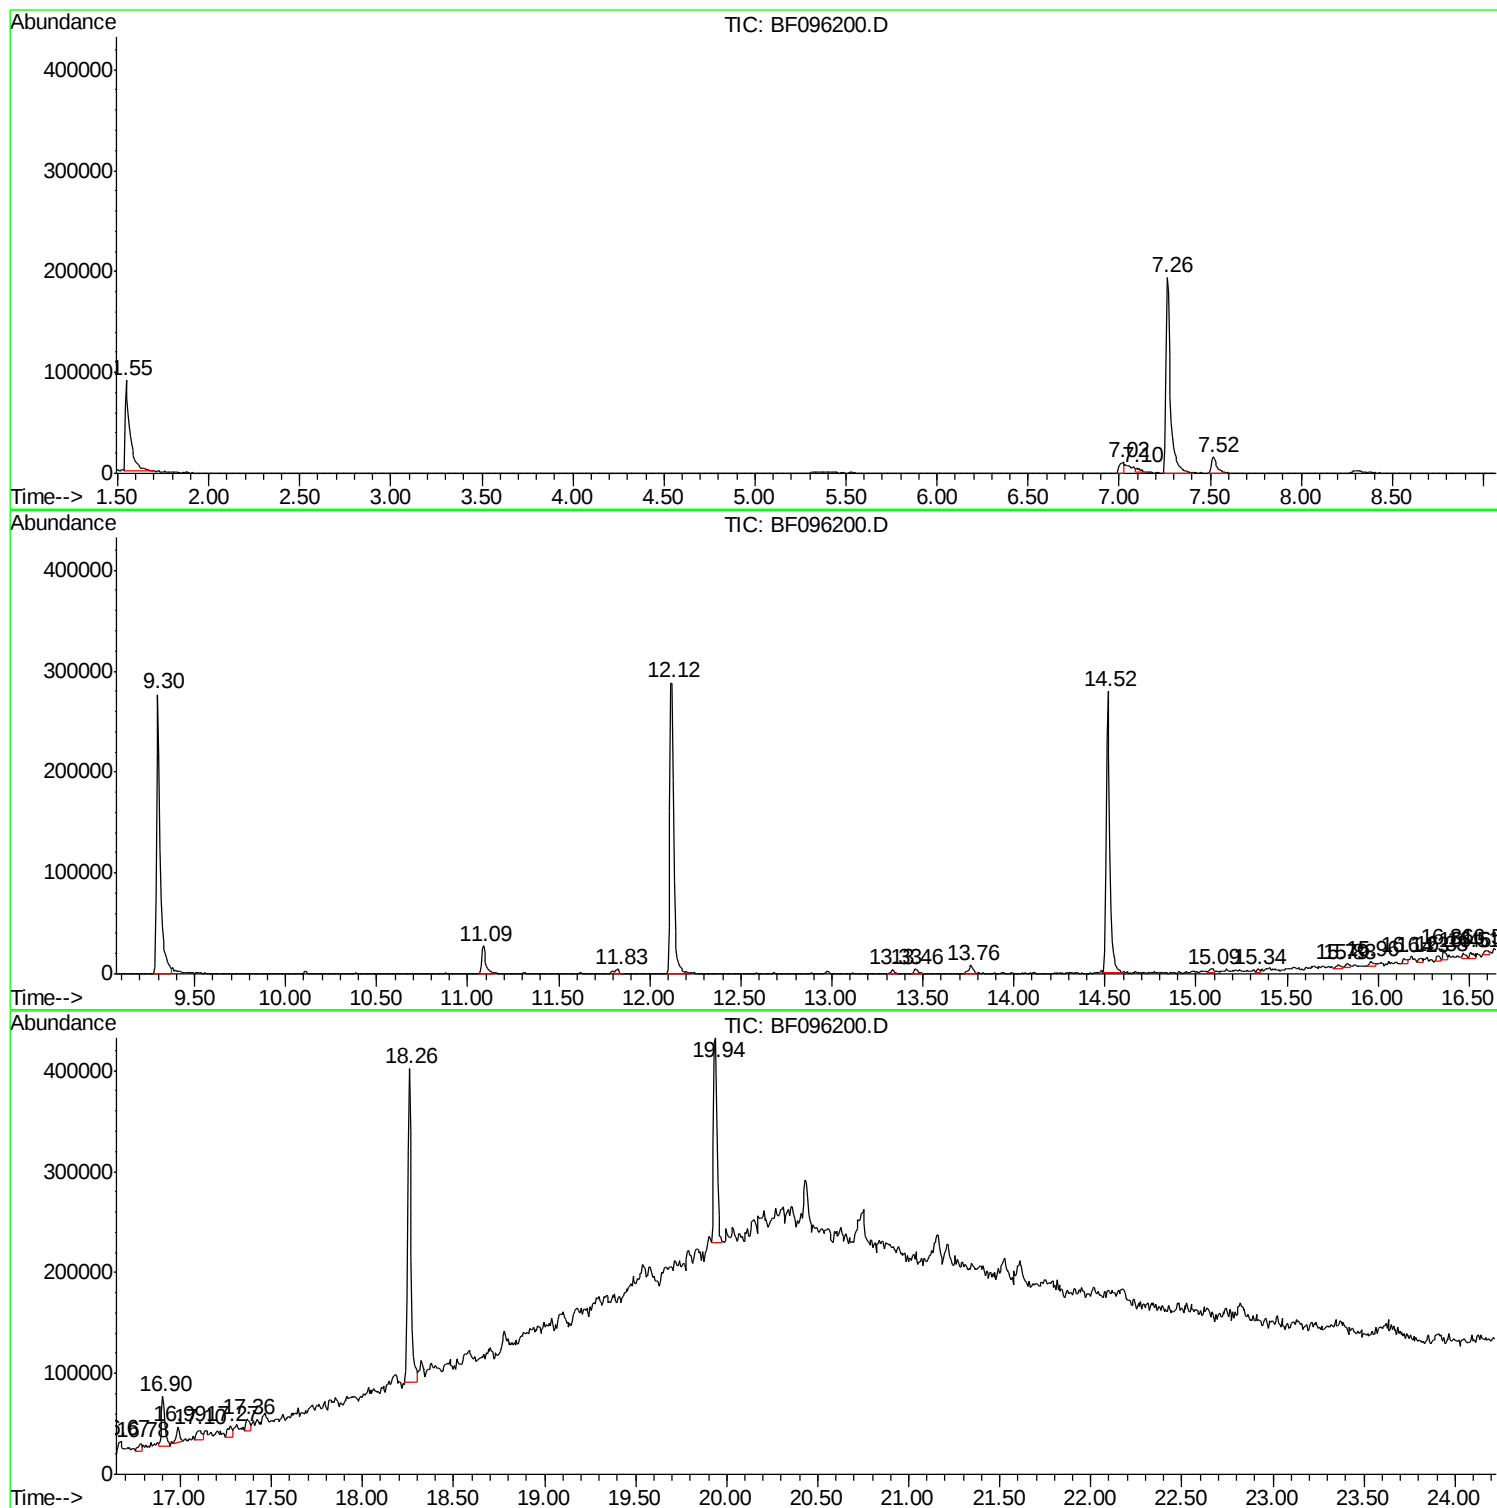

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data_File : BF096200.D
Acq_On : 24 Jun 2017 20:300
Operator : SJ/MAA
Sample : I3852-06-5XX
Misc :
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-31-1.5-3

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
