

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
 Data File : BF096201.D
 Acq On : 24 Jun 2017 21:03
 Operator : SJ/MA
 Sample : I3852-08 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-28-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.540	7	9	41	rVB	352638	718685	100.00%	21.180%
2	7.028	937	942	945	rBV2	5868	12345	1.72%	0.364%
3	7.263	978	982	1003	rBV	229797	370630	51.57%	10.923%
4	7.522	1021	1026	1034	rBV	11545	21723	3.02%	0.640%
5	9.298	1324	1328	1347	rBV	332088	484911	67.47%	14.291%
6	11.086	1629	1632	1647	rBV	15536	27072	3.77%	0.798%
7	12.122	1803	1808	1822	rBV2	325009	463637	64.51%	13.664%
8	14.516	2210	2215	2228	rBV	303978	427223	59.45%	12.590%
9	16.362	2526	2529	2536	rBV2	9292	14186	1.97%	0.418%
10	16.662	2577	2580	2585	rBV2	12250	15778	2.20%	0.465%
11	16.904	2618	2621	2627	rVB	26082	28507	3.97%	0.840%
12	18.256	2846	2851	2861	rBV	351061	489867	68.16%	14.437%
13	19.933	3133	3136	3142	rBV	263928	318654	44.34%	9.391%


Sum of corrected areas: 3393218

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data File : BF096201.D
Acq On : 24 Jun 2017 21:03
Operator : SJ/MA
Sample : I3852-08 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-28-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

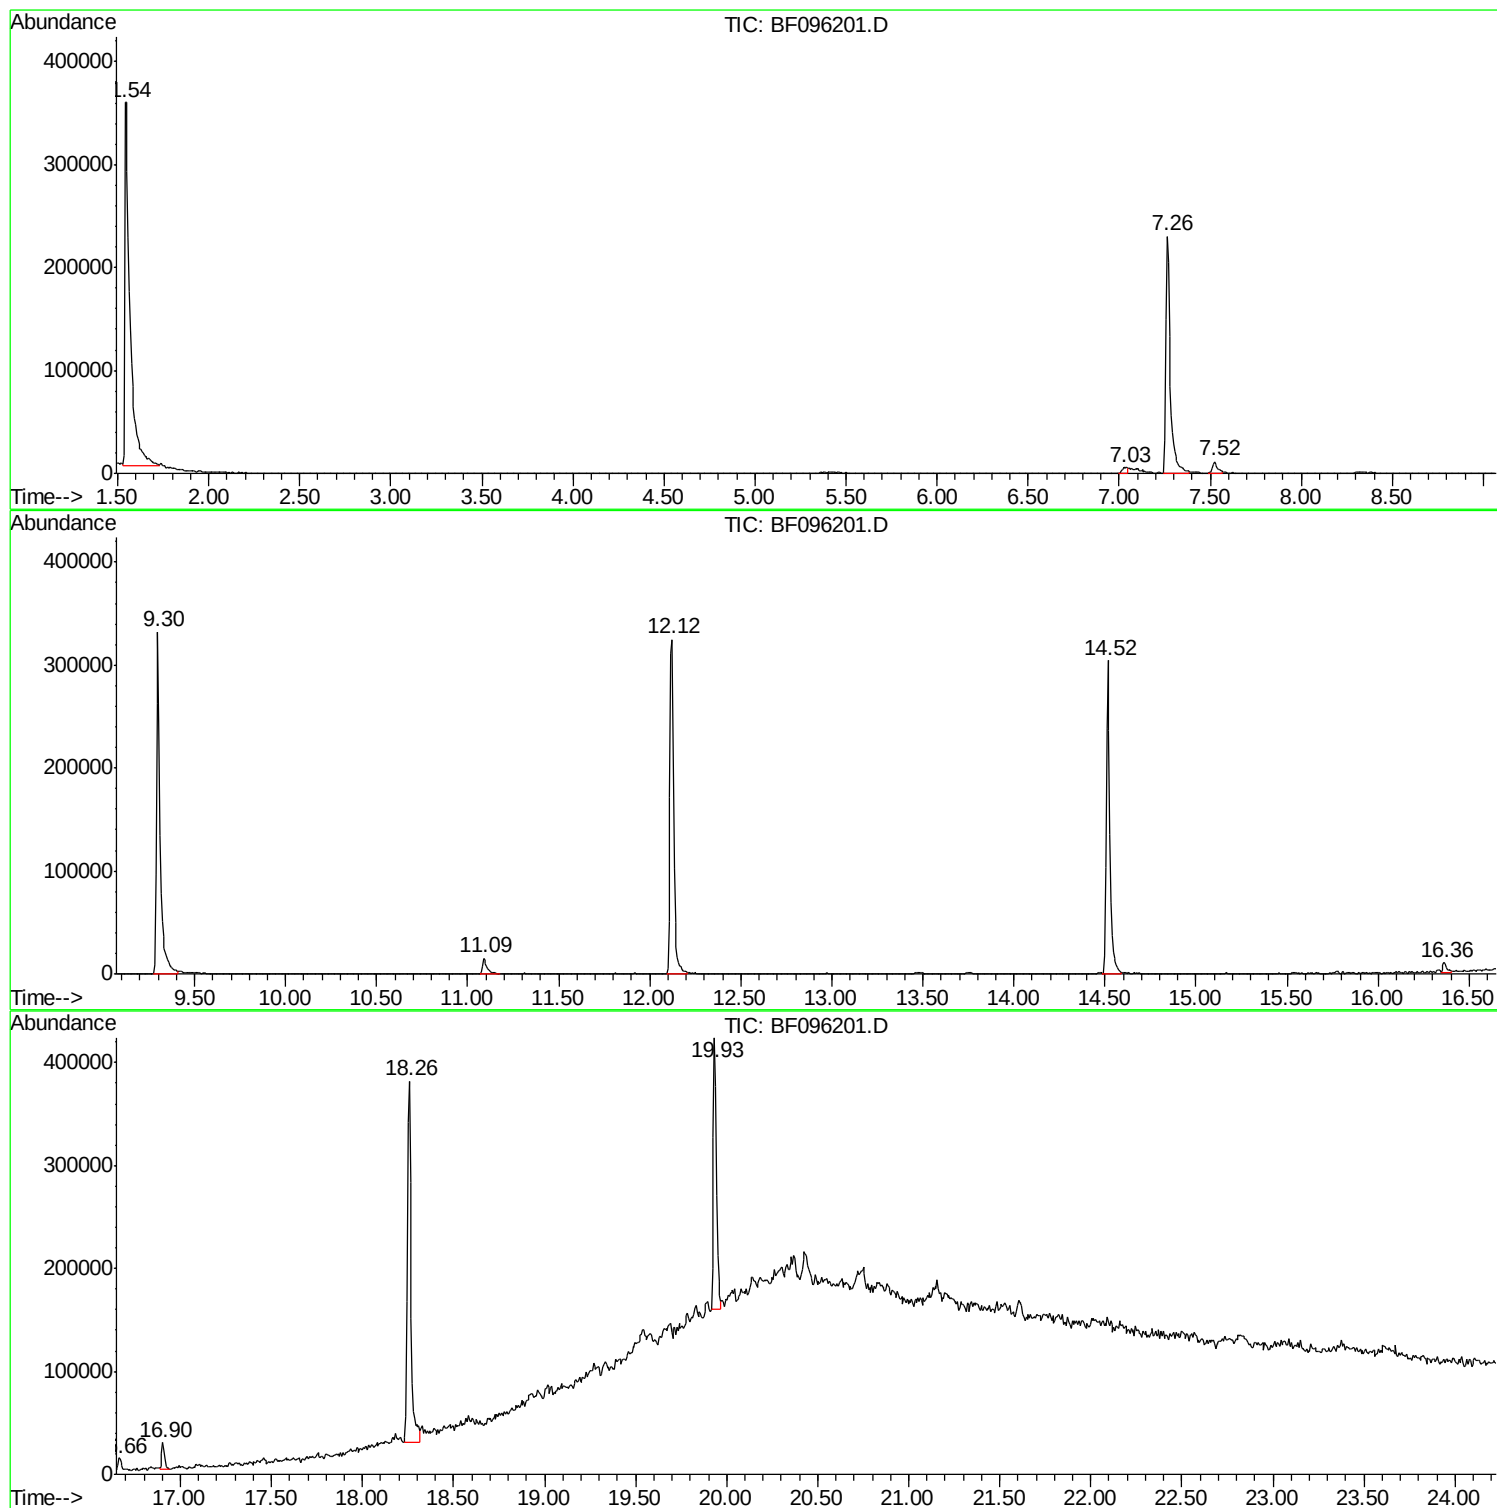

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062417\
Data_File : BF096201.D
Acq_On : 24 Jun 2017 21:033
Operator : SJ/MAA
Sample : I3852-08_5XX
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-28-1.5-3

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
