


Data Path : Z:\HPCHEM1\BNA_F\Data\BF062417\
 Data File : BF096179.D
 Acq On : 24 Jun 2017 9:03
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

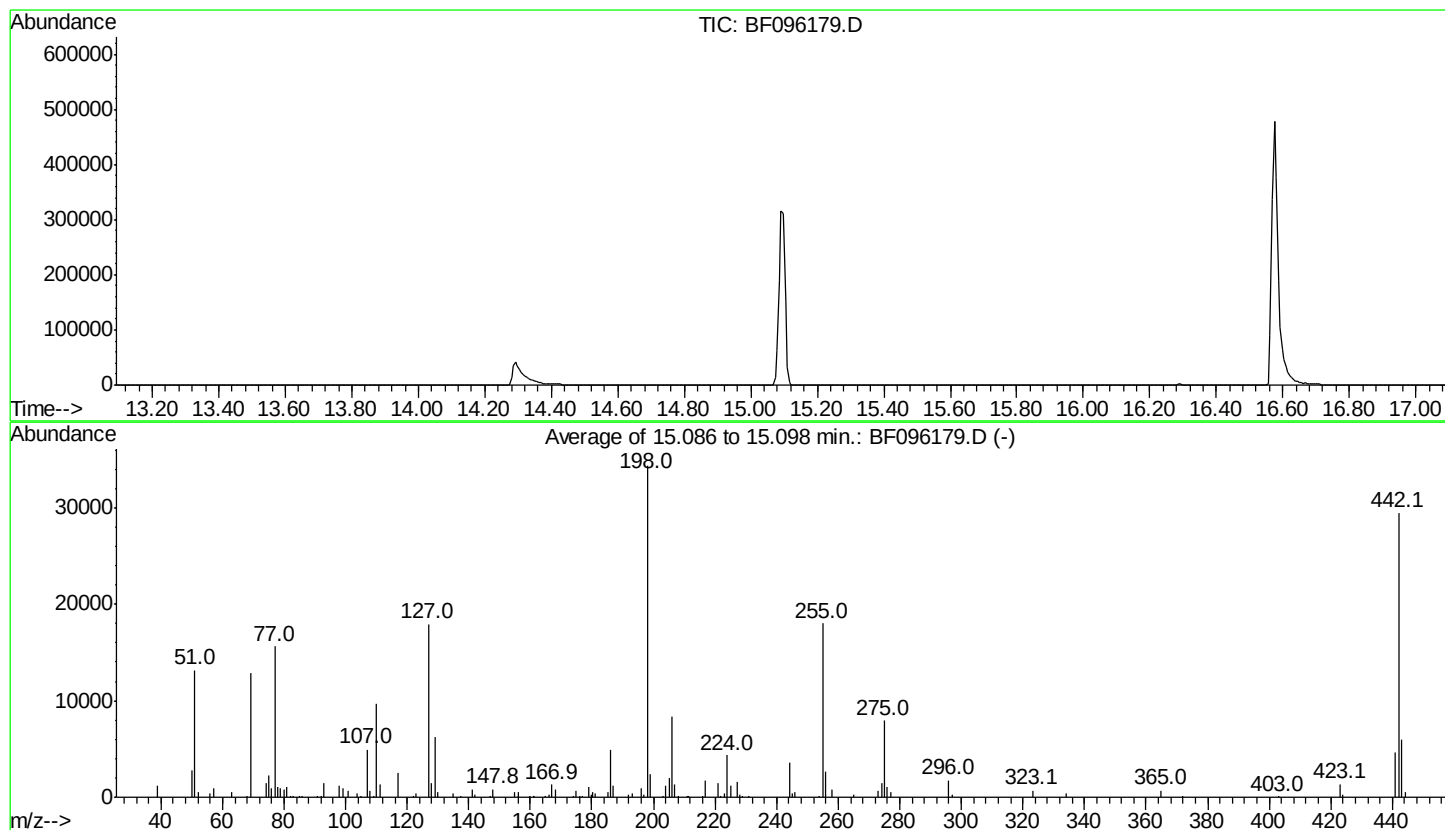

AutoFind: Scans 2312, 2313, 2314; Background Corrected with Scan 2306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	13134	PASS
68	69	0.00	2	0.8	107	PASS
69	198	0.00	100	37.6	12905	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	17964	PASS
197	198	0.00	2	0.7	248	PASS
198	198	100	100	100.0	34362	PASS
199	198	5	9	6.9	2374	PASS
275	198	10	60	23.1	7922	PASS
365	198	1	100	2.1	705	PASS
441	442	0.01	24	15.8	4656	PASS
442	198	50	100	85.8	29499	PASS
443	442	15	24	20.3	5975	PASS