


Data Path : Z:\HPCHEM1\BNA F\Data\BF062417\
 Data File : BF096202.D
 Acq On : 24 Jun 2017 23:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

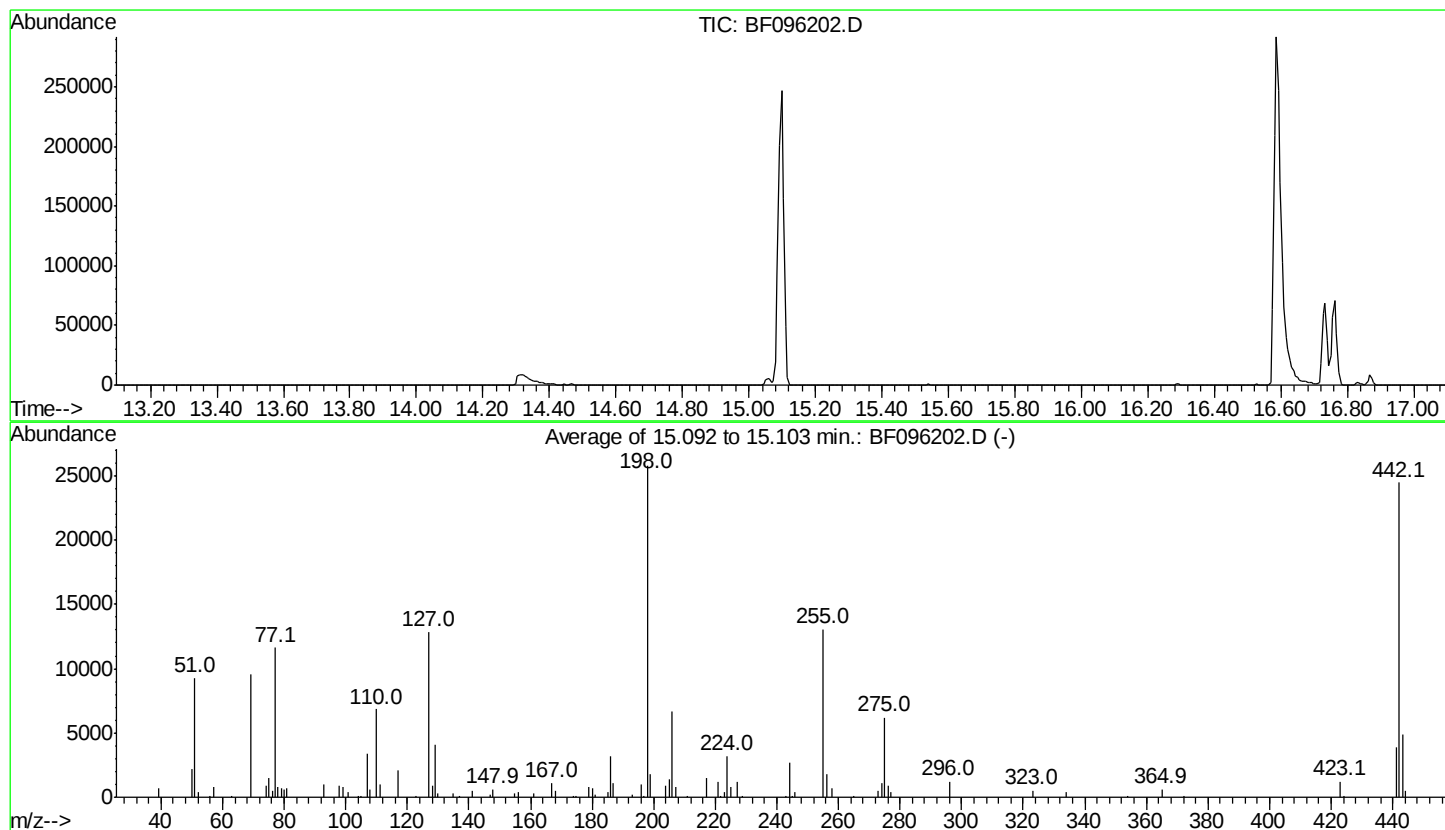

AutoFind: Scans 2313, 2314, 2315; Background Corrected with Scan 2307

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	9288	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.9	9512	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	12867	PASS
197	198	0.00	2	0.4	105	PASS
198	198	100	100	100.0	25789	PASS
199	198	5	9	7.0	1794	PASS
275	198	10	60	23.9	6173	PASS
365	198	1	100	2.4	623	PASS
441	442	0.01	24	15.9	3889	PASS
442	198	50	100	94.9	24472	PASS
443	442	15	24	19.9	4862	PASS