
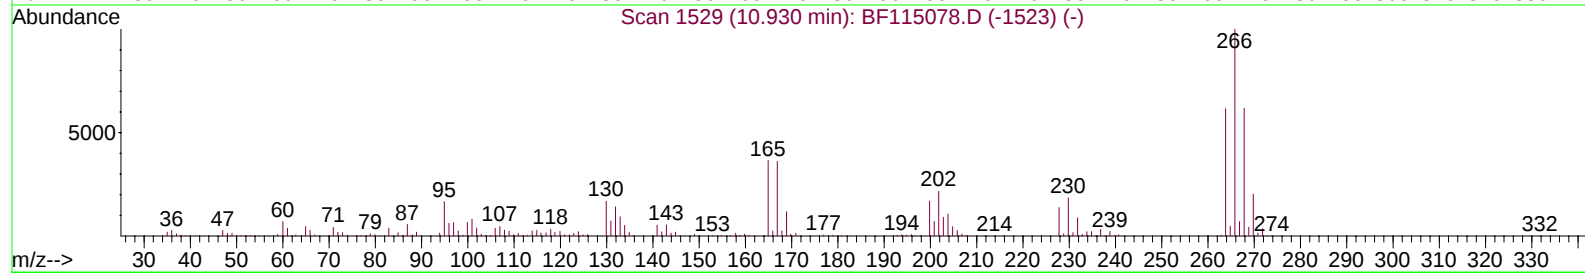
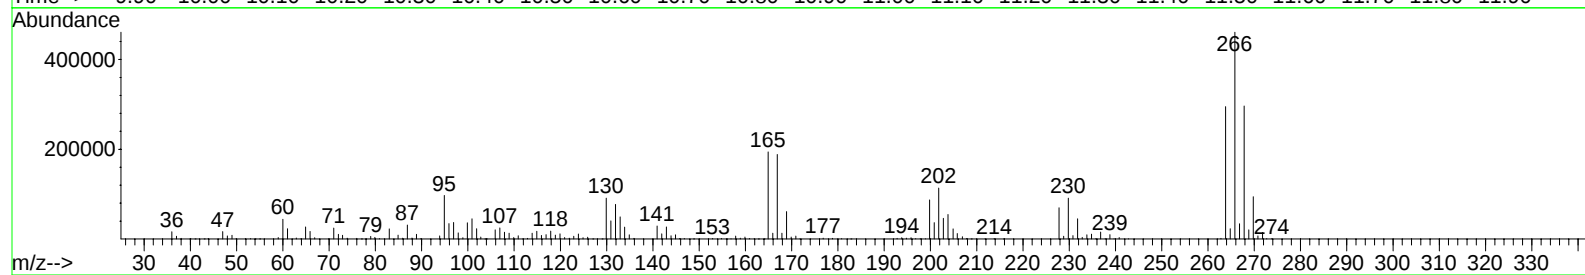


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062419\  
Data File   : BF115152.D  
Acq On      : 24 Jun 2019   17:36  
Operator    : HP/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 25 10:03:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

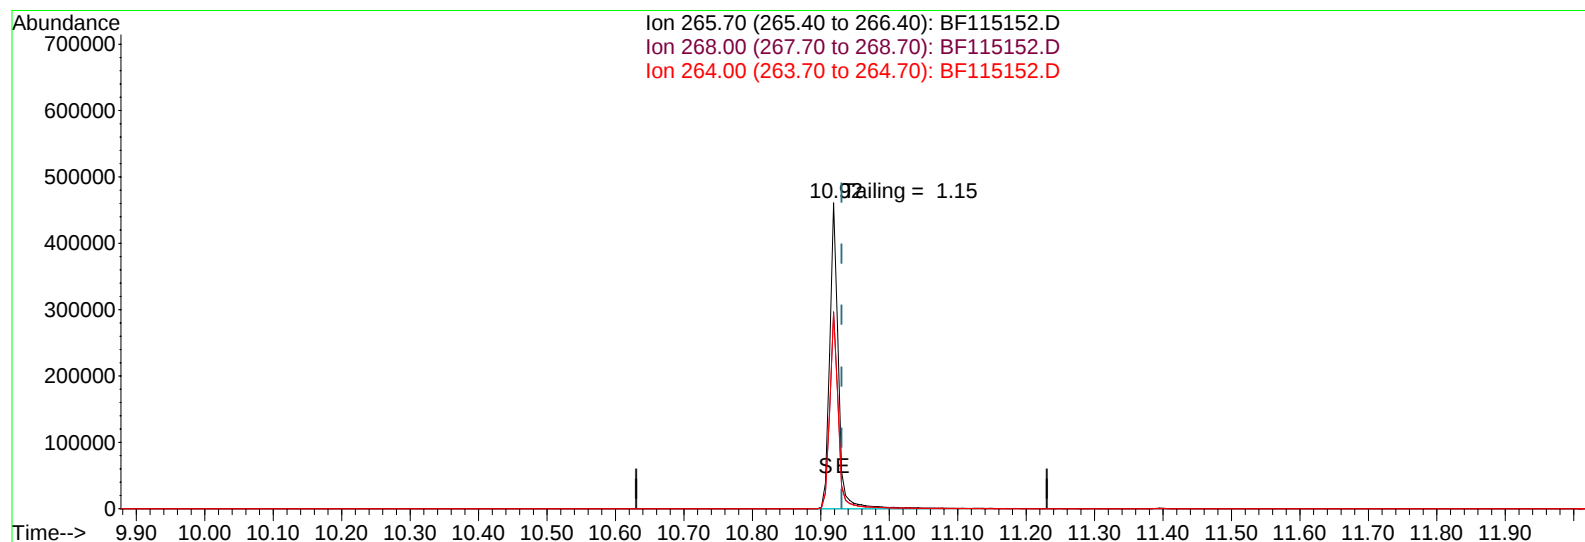

TIC: BF115152.D

(70) Pentachlorophenol (C)




10.919min (-0.012) 0.00ng

response 401924

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	64.34
264.00	61.60	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062419\
 Data File : BF115152.D
 Acq On : 24 Jun 2019 17:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 10:03:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 04:21:29 2019
 Response via : Initial Calibration

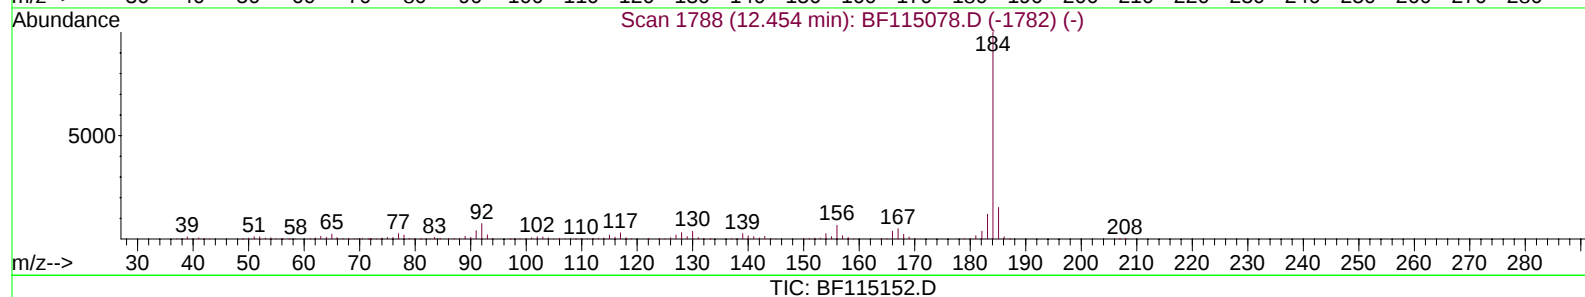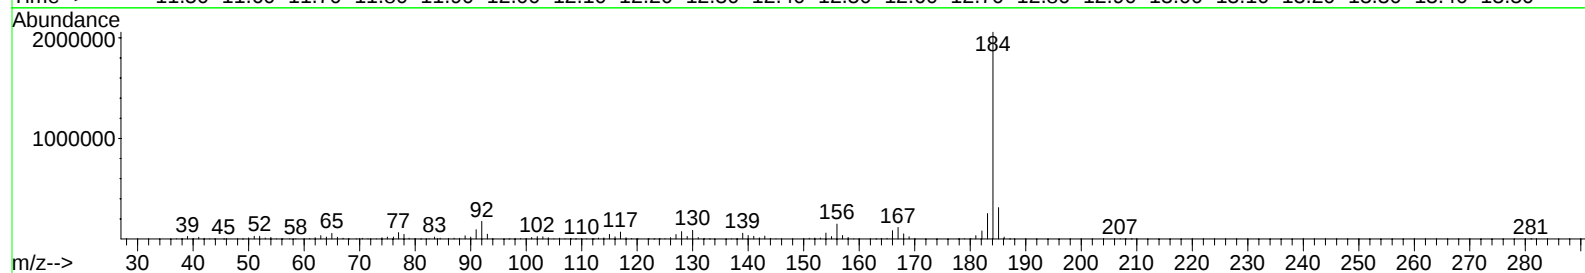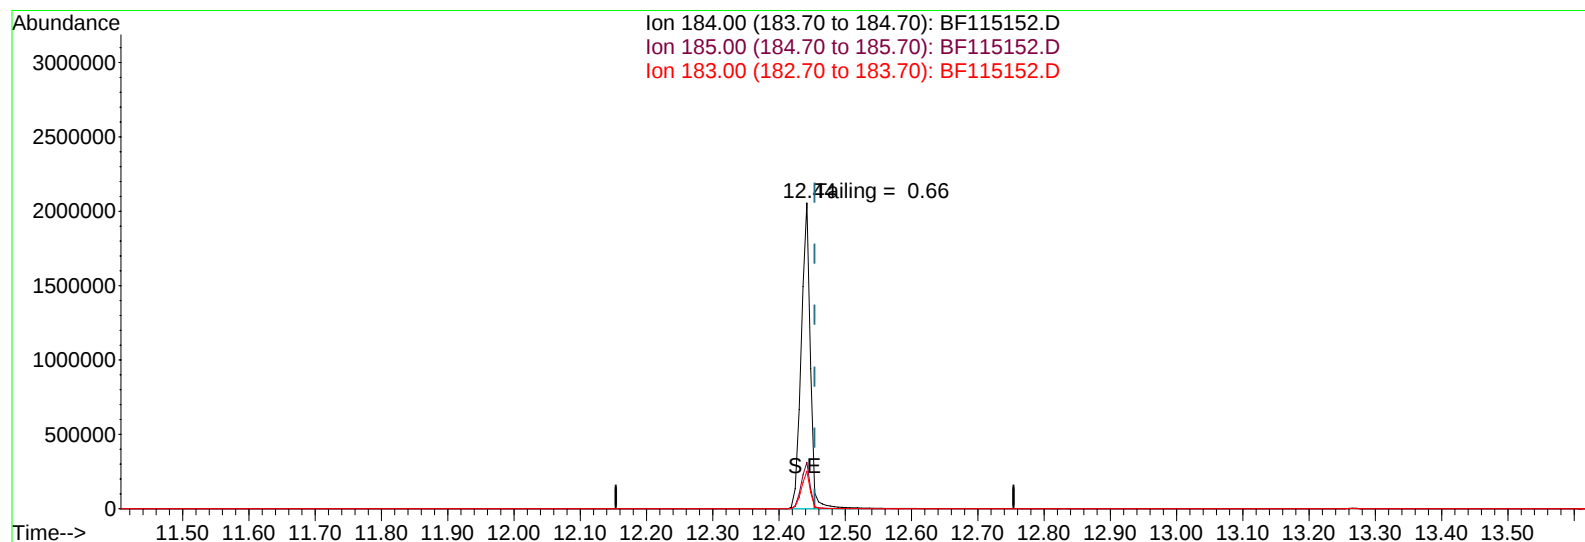

(77) Benzidine

12.442min (-0.012) 182766.59ng

response 1988314

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.18
183.00	12.00	12.29
0.00	0.00	0.00