

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062419\
 Data File : BF115168.D
 Acq On : 25 Jun 2019 00:48
 Operator : HP/JU
 Sample : K3487-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-048

Quant Time: Jun 25 08:32:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 04:21:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.61	152	301195	20.00	ng	0.00
21) Naphthalene-d8	7.89	136	1147881	20.00	ng	-0.01
39) Acenaphthene-d10	9.64	164	576831	20.00	ng	-0.01
64) Phenanthrene-d10	11.11	188	1128922	20.00	ng	-0.01
76) Chrysene-d12	13.72	240	784772	20.00	ng	-0.02
87) Perylene-d12	15.09	264	690165	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.21	112	1265451	64.84	ng	0.00
7) Phenol-d6	6.25	99	1574605	66.47	ng	0.00
23) Nitrobenzene-d5	7.17	82	938666	50.30	ng	-0.01
42) 2,4,6-Tribromophenol	10.42	330	395205	64.97	ng	-0.01
45) 2-Fluorobiphenyl	8.97	172	1671174	49.21	ng	-0.02
79) Terphenyl-d14	12.69	244	1789409	48.48	ng	-0.02
Target Compounds						
50) Dimethylphthalate	9.36	163	197022	4.643	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062419\
Data File : BF115168.D
Acq On : 25 Jun 2019 00:48
Operator : HP/JU
Sample : K3487-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-048

Quant Time: Jun 25 08:32:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

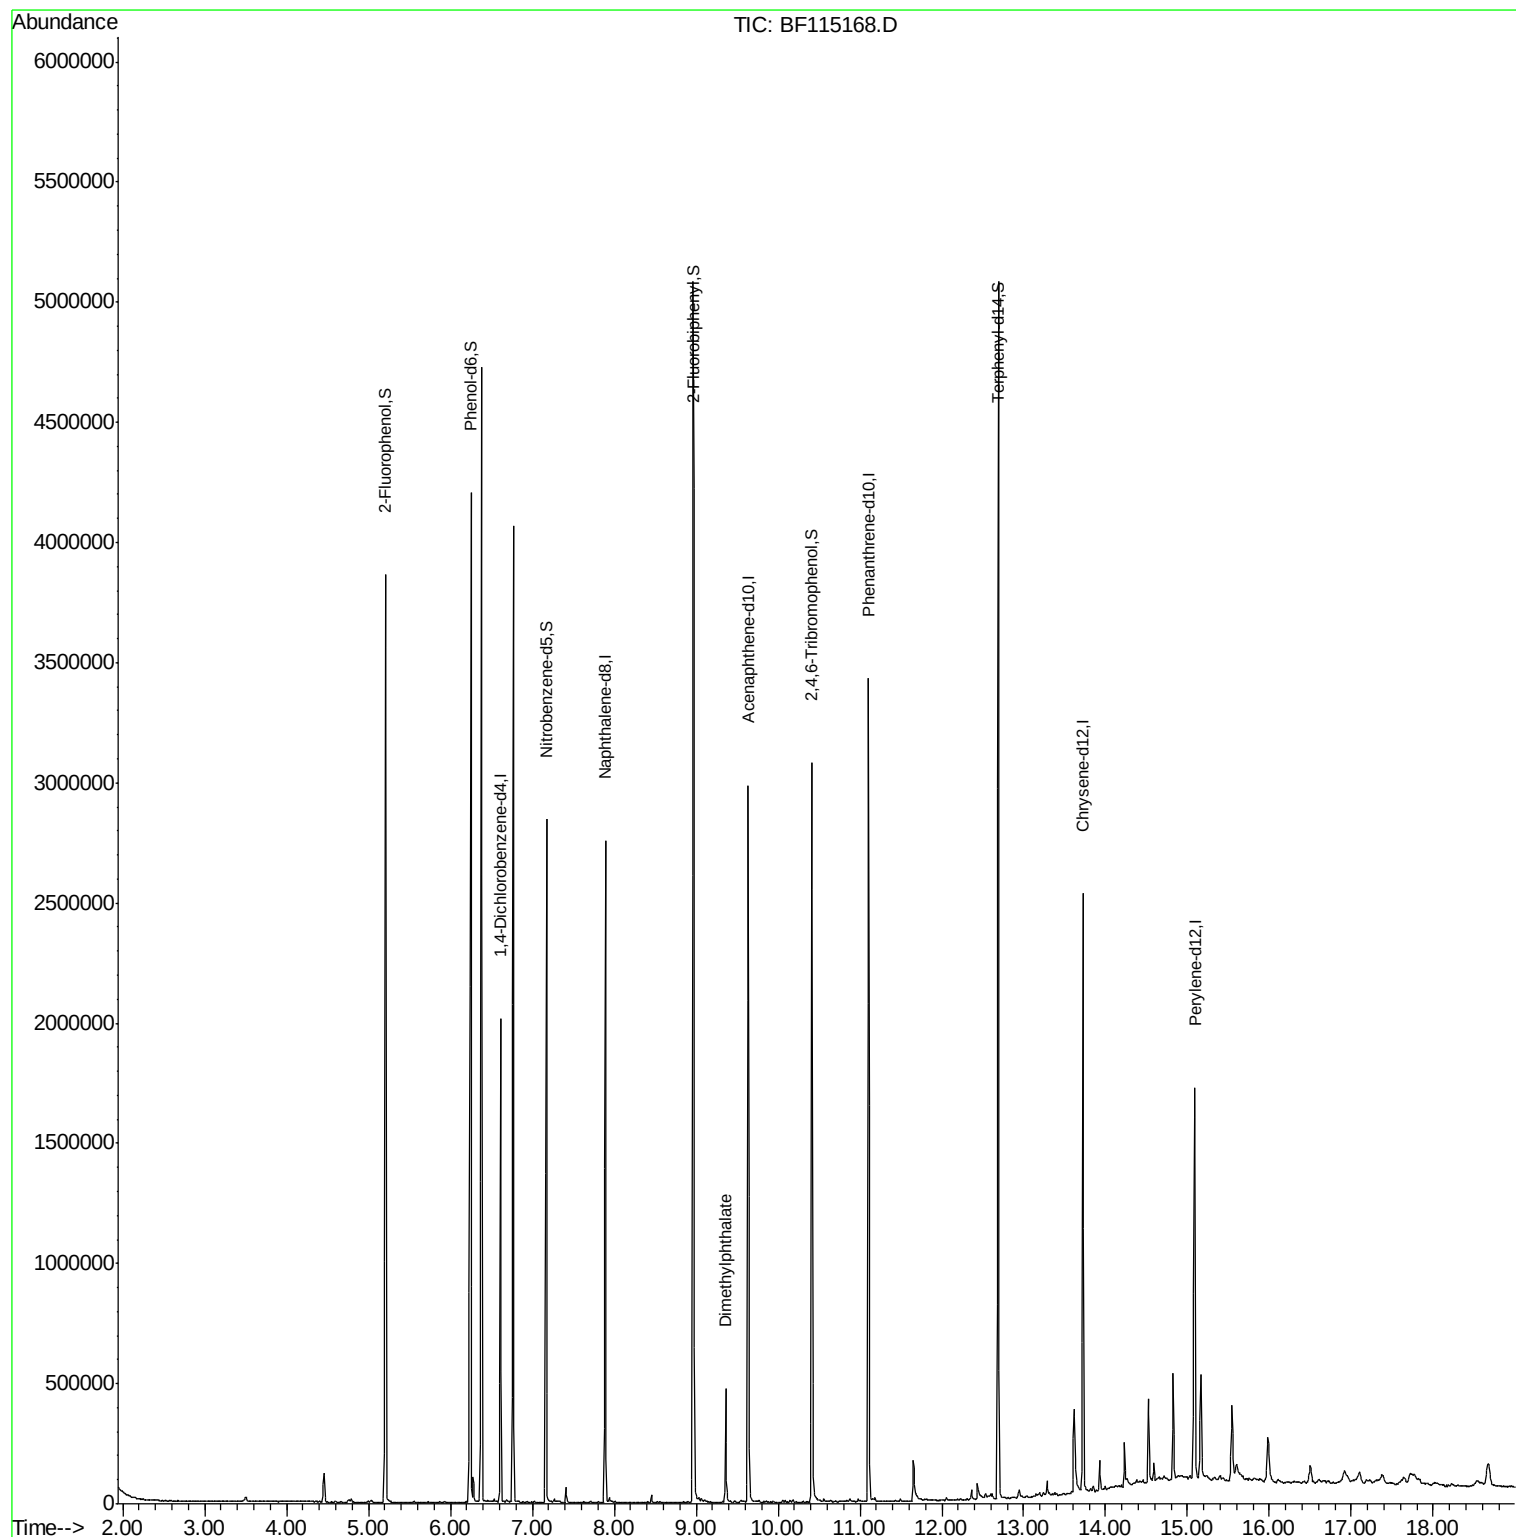

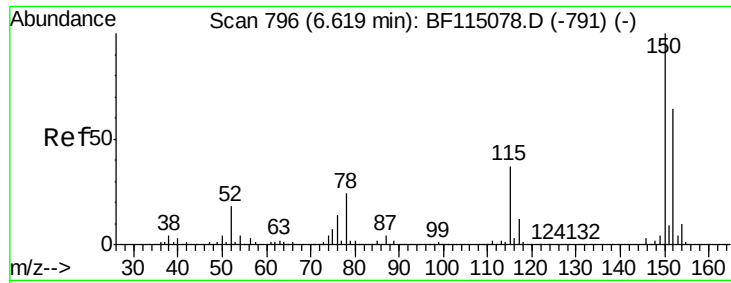


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.61 min Scan# 795
Delta R.T. -0.01 min
Lab File: BF115168.D
Acq: 25 Jun 2019 00:48

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-048

Tot Ion:152 Resp: 301195
Ion Ratio Lower Upper
152 100
150 153.4 124.2 186.2
115 55.5 46.1 69.1

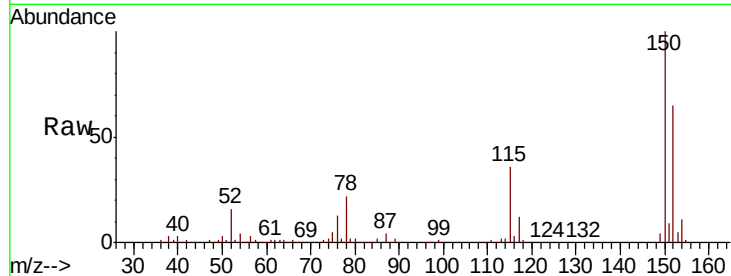


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

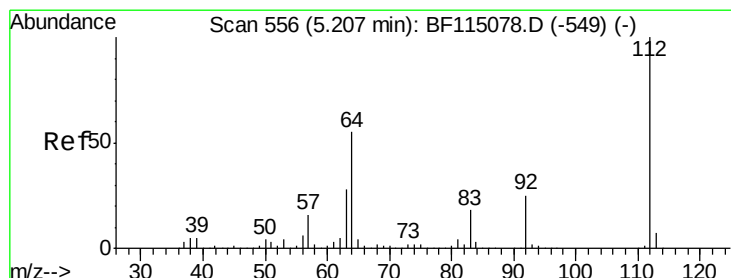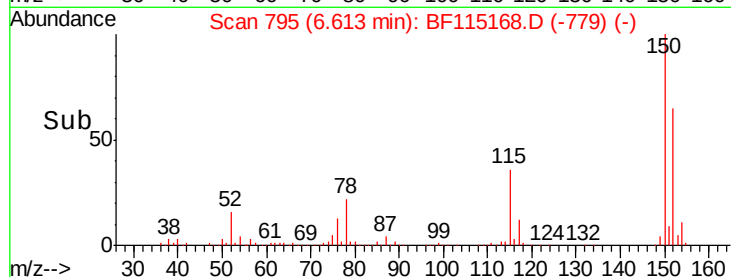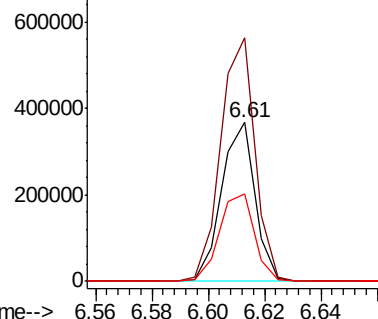



#5


2-Fluorophenol
Concen: 64.835 ng
RT: 5.21 min Scan# 556
Delta R.T. -0.00 min
Lab File: BF115168.D
Acq: 25 Jun 2019 00:48

Tgt Ion:112 Resp: 1265451
Ion Ratio Lower Upper
112 100
64 56.3 43.8 65.6
63 28.4 22.2 33.4

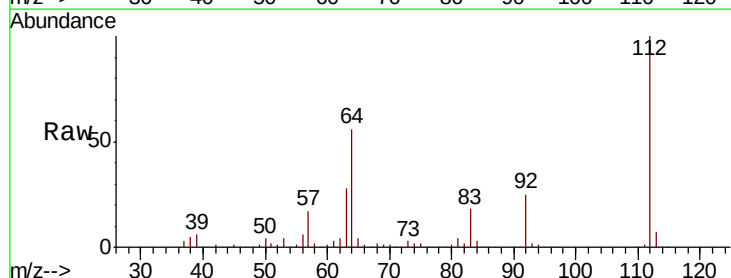

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

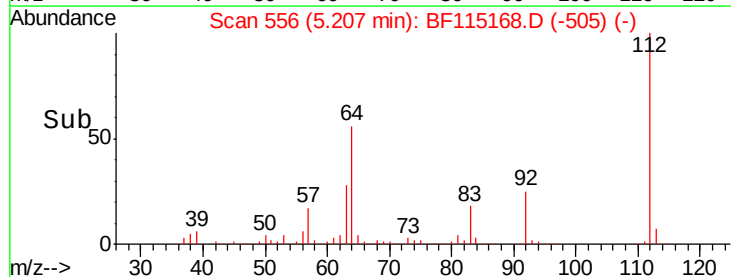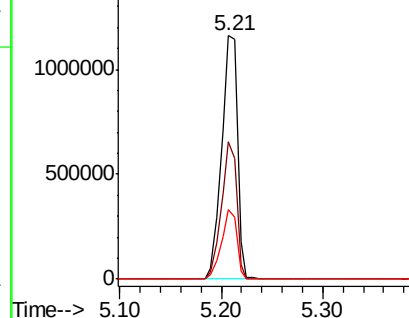

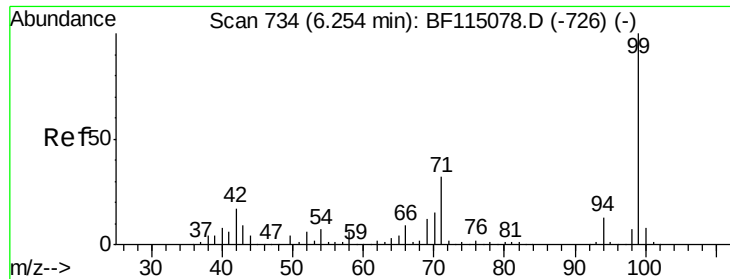

#7

Phenol-d6

Concen: 66.467 ng

RT: 6.25 min Scan# 733

Delta R.T. -0.01 min

Lab File: BF115168.D

Acq: 25 Jun 2019 00:48

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-048





Tot Ion: 99 Resp: 1574605

Ion Ratio Lower Upper

99 100

42 16.5 13.6 20.4

71 32.3 25.5 38.3

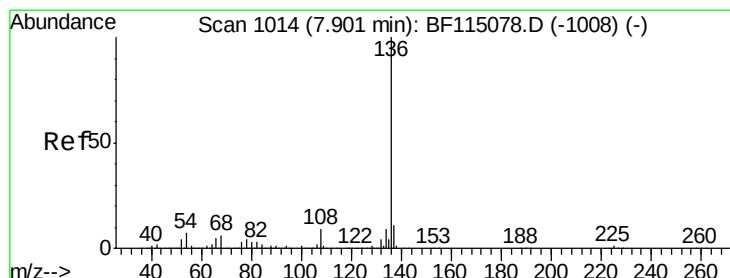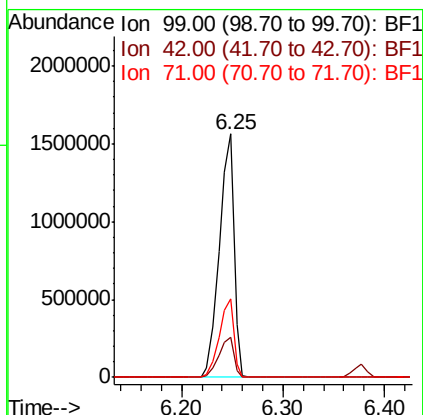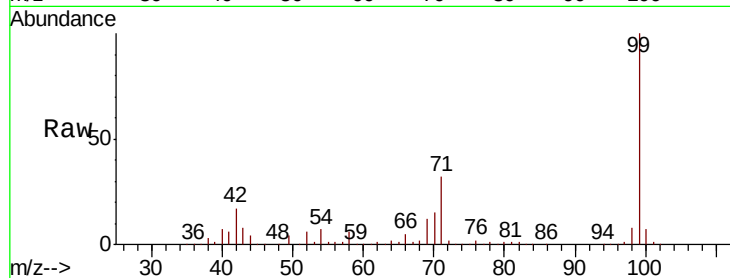

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.89 min Scan# 1012

Delta R.T. -0.01 min

Lab File: BF115168.D

Acq: 25 Jun 2019 00:48

Tgt Ion: 136 Resp: 1147881




Ion Ratio Lower Upper


136 100

137 11.4 8.9 13.3

54 7.1 5.6 8.4

68 6.3 4.8 7.2

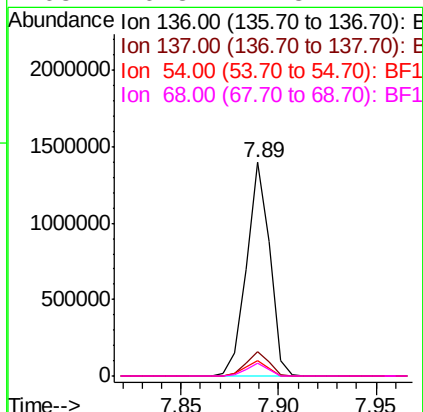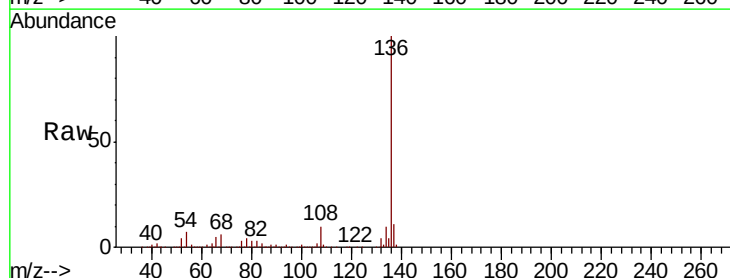







#23
 Nitrobenzene-d5
 Concen: 50.303 ng
 RT: 7.17 min Scan# 890
 Delta R.T. -0.01 min
 Lab File: BF115168.D
 Acq: 25 Jun 2019 00:48

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-048

Tot Ion: 82 Resp: 938666
 Ion Ratio Lower Upper
 82 100
 128 51.7 40.4 60.6
 54 45.2 37.5 56.3

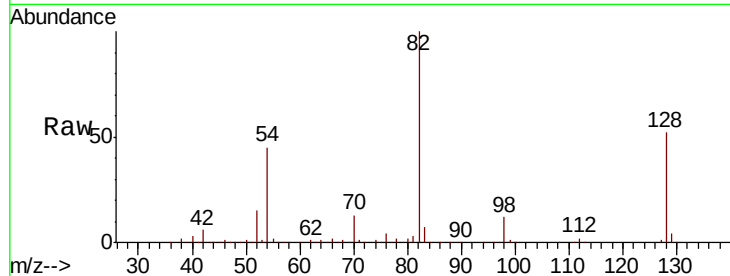


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

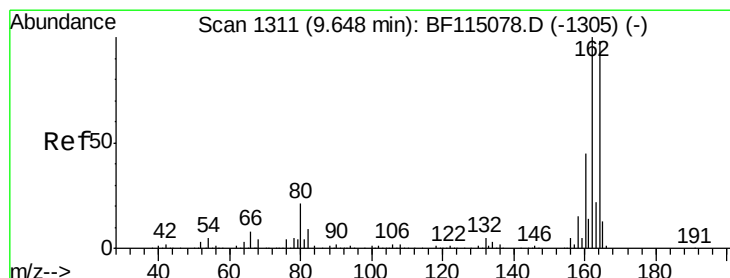
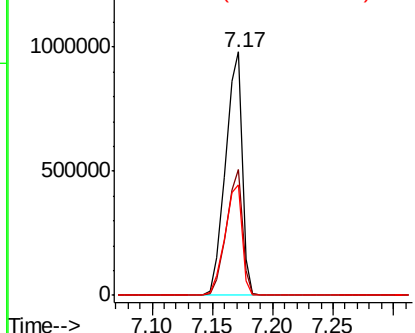



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.64 min Scan# 1309
 Delta R.T. -0.01 min
 Lab File: BF115168.D
 Acq: 25 Jun 2019 00:48

Tgt Ion:164 Resp: 576831
 Ion Ratio Lower Upper
 164 100
 162 102.0 81.7 122.5
 160 46.8 37.0 55.4

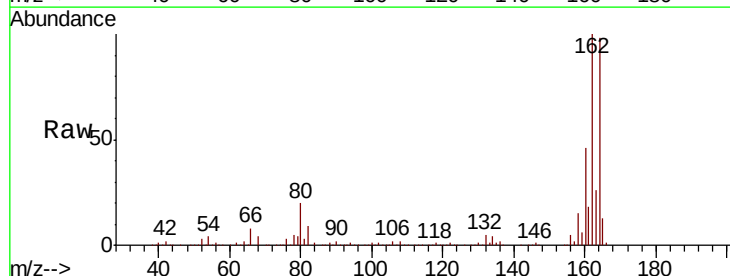

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

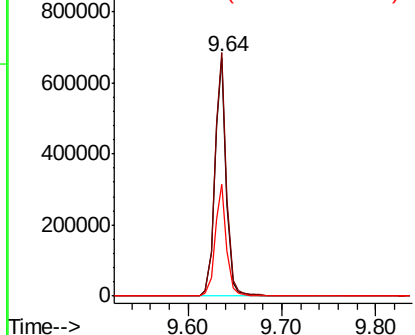



#42

2,4,6-Tribromophenol

Concen: 64.970 ng

RT: 10.42 min Scan# 1442

Delta R.T. -0.01 min

Lab File: BF115168.D

Acq: 25 Jun 2019 00:48

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-048


Tot Ion:330 Resp: 395205

Ion Ratio Lower Upper




330 100

332 96.7 77.3 115.9

141 33.4 28.2 42.2

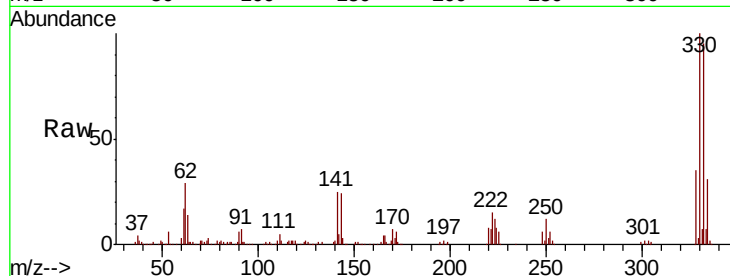

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

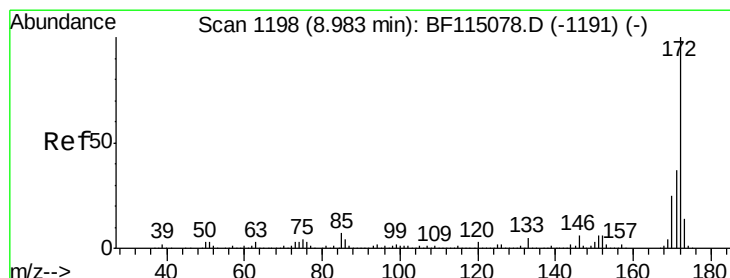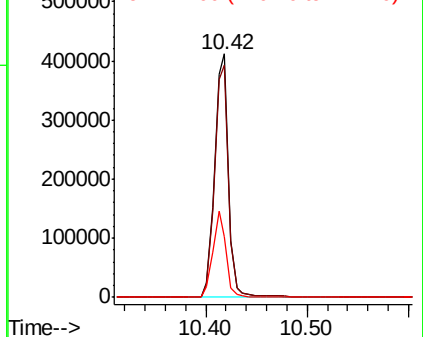

#45

2-Fluorobiphenyl

Concen: 49.212 ng

RT: 8.97 min Scan# 1195

Delta R.T. -0.02 min

Lab File: BF115168.D

Acq: 25 Jun 2019 00:48


Tgt Ion:172 Resp: 1671174

Ion Ratio Lower Upper



172 100


171 37.0 29.8 44.6

170 24.9 20.3 30.5

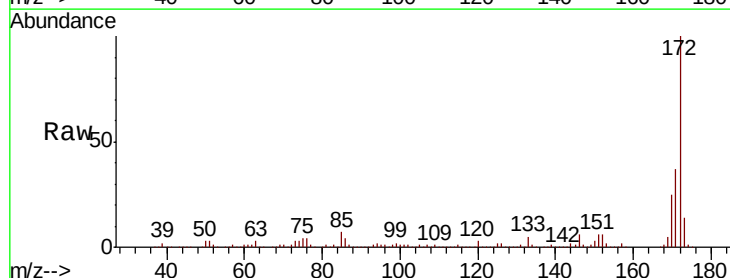

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

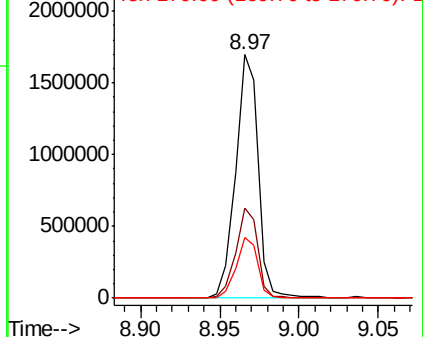


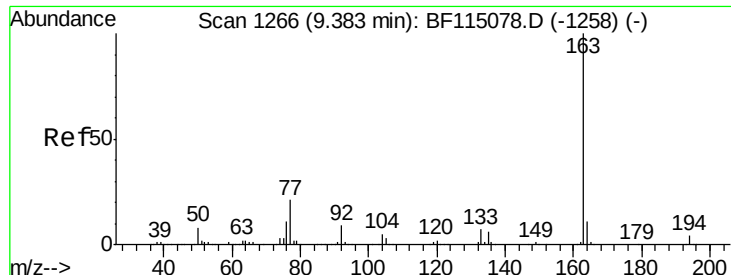




#50
Dimethylphthalate
Concen: 4.643 ng
RT: 9.36 min Scan# 1262
Delta R.T. -0.02 min
Lab File: BF115168.D
Acq: 25 Jun 2019 00:48

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-048

Tot Ion:163 Resp: 197022
Ion Ratio Lower Upper
163 100
194 3.6 3.2 4.8
164 10.0 8.6 13.0

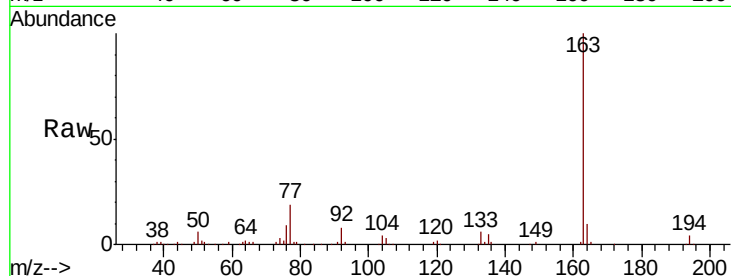


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

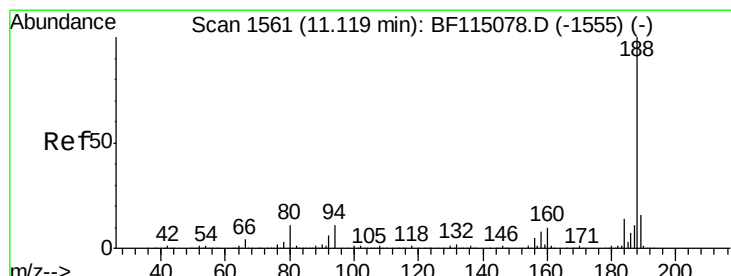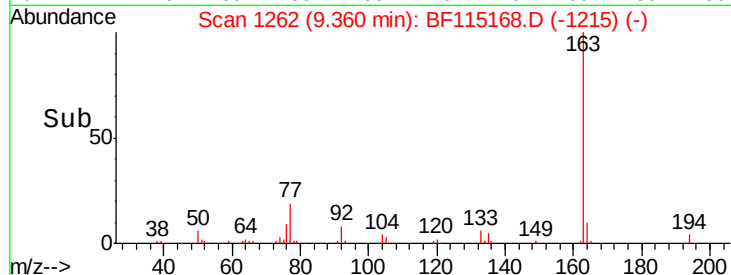
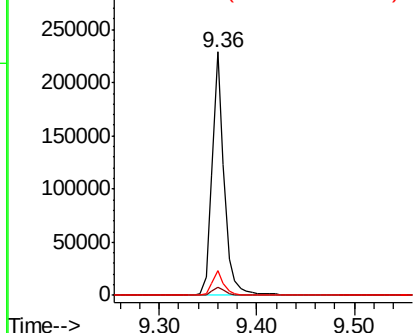



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.11 min Scan# 1559
Delta R.T. -0.01 min
Lab File: BF115168.D
Acq: 25 Jun 2019 00:48

Tgt Ion:188 Resp: 1128922
Ion Ratio Lower Upper
188 100
94 9.8 8.6 12.8
80 10.2 8.8 13.2

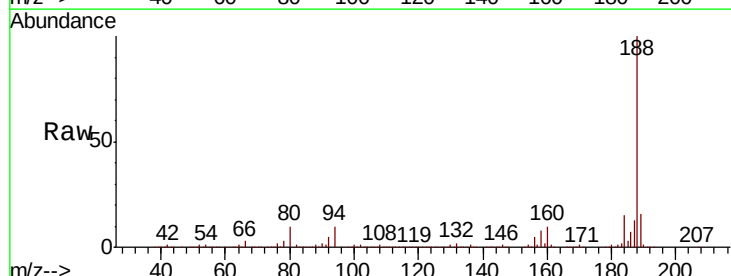

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

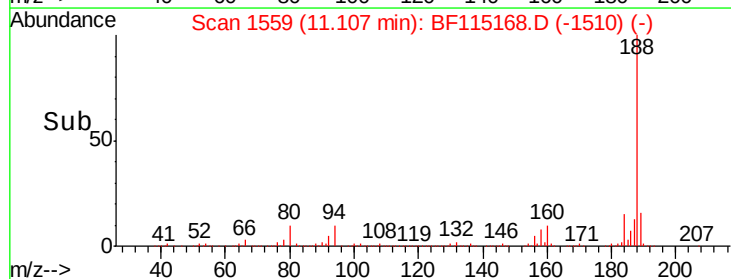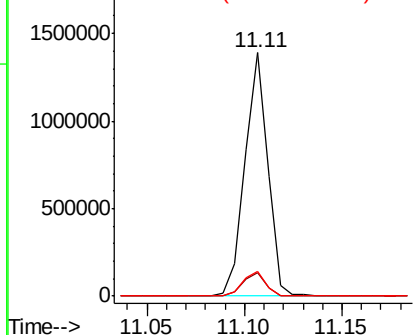







#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.72 min Scan# 2004
 Delta R.T. -0.02 min
 Lab File: BF115168.D
 Acq: 25 Jun 2019 00:48

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-048

Tot Ion:240 Resp: 784772
 Ion Ratio Lower Upper
 240 100
 120 11.8 9.4 14.2
 236 27.0 21.7 32.5

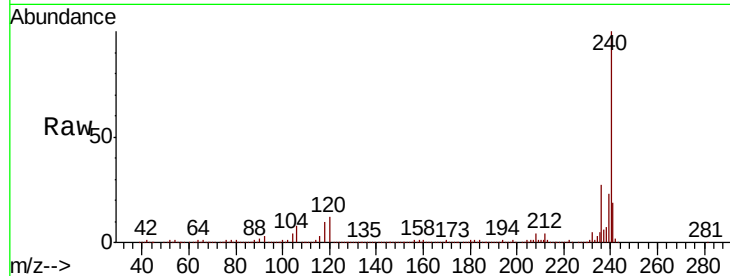


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

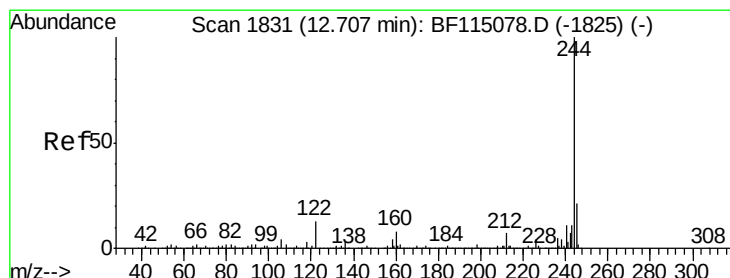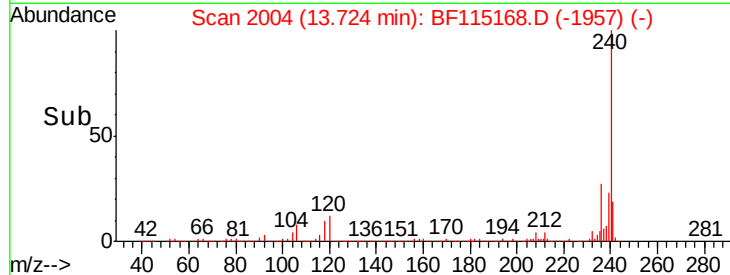
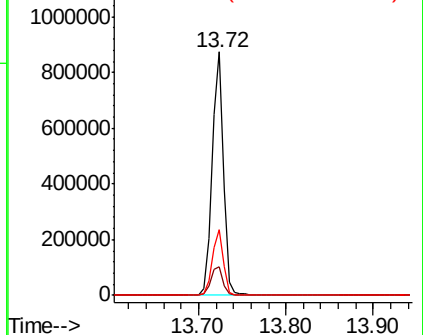



#79
 Terphenyl-d14
 Concen: 48.480 ng
 RT: 12.69 min Scan# 1828
 Delta R.T. -0.02 min
 Lab File: BF115168.D
 Acq: 25 Jun 2019 00:48

Tgt Ion:244 Resp: 1789409
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.8 8.6
 122 12.9 10.4 15.6

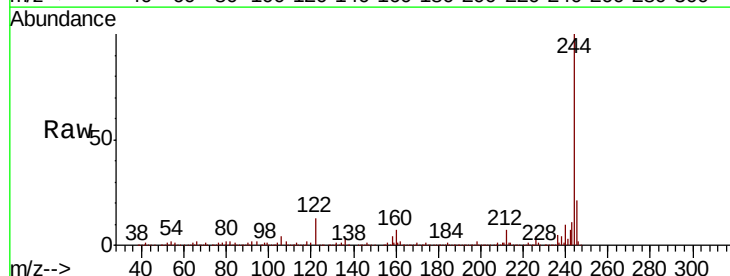

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

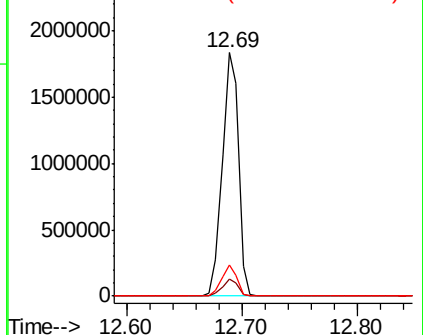

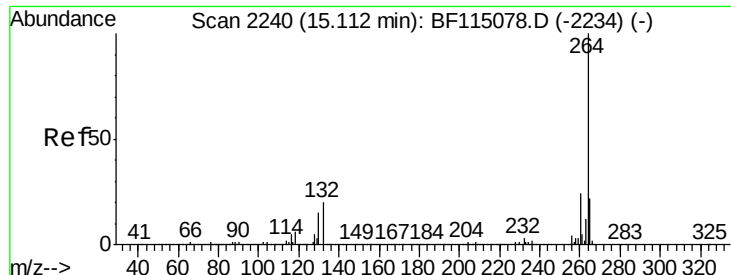

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.09 min Scan# 2236
 Delta R.T. -0.02 min
 Lab File: BF115168.D
 Acq: 25 Jun 2019 00:48

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-048

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.6	29.4
265	21.7	17.3	25.9

