

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062419\
 Data File : BF115145.D
 Acq On : 24 Jun 2019 12:58
 Operator : HP/JU
 Sample : PB120809BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120809BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.225	553	559	562	rBV	6090584	6910754	76.53%	9.870%
2	6.254	727	734	737	rBV	5999260	7020129	77.74%	10.027%
3	6.384	750	756	759	rBV	6699724	7343132	81.31%	10.488%
4	6.613	791	795	798	rBV	2062452	1810817	20.05%	2.586%
5	6.766	817	821	825	rBV	5780017	5977449	66.19%	8.537%
6	7.172	884	890	893	rBV	4258060	4735224	52.43%	6.763%
7	7.890	1007	1012	1015	rBV	2512053	2328260	25.78%	3.325%
8	8.972	1189	1196	1199	rBV	8006809	8857905	98.09%	12.651%
9	9.636	1303	1309	1323	rBV	2877057	2707613	29.98%	3.867%
10	10.419	1435	1442	1445	rBV	5127677	5345230	59.19%	7.634%
11	11.107	1554	1559	1563	rBV	3329910	2926276	32.40%	4.180%
12	12.701	1824	1830	1833	rBV	7873102	9030714	100.00%	12.898%
13	13.724	2000	2004	2008	rBV	2659046	2572196	28.48%	3.674%
14	15.101	2230	2238	2247	rBV	1819073	2206170	24.43%	3.151%
15	15.177	2248	2251	2263	rVB	104231	140762	1.56%	0.201%
16	15.560	2312	2316	2322	rBV	72492	102280	1.13%	0.146%


Sum of corrected areas: 70014911

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062419\
Data File : BF115145.D
Acq On : 24 Jun 2019 12:58
Operator : HP/JU
Sample : PB120809BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120809BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

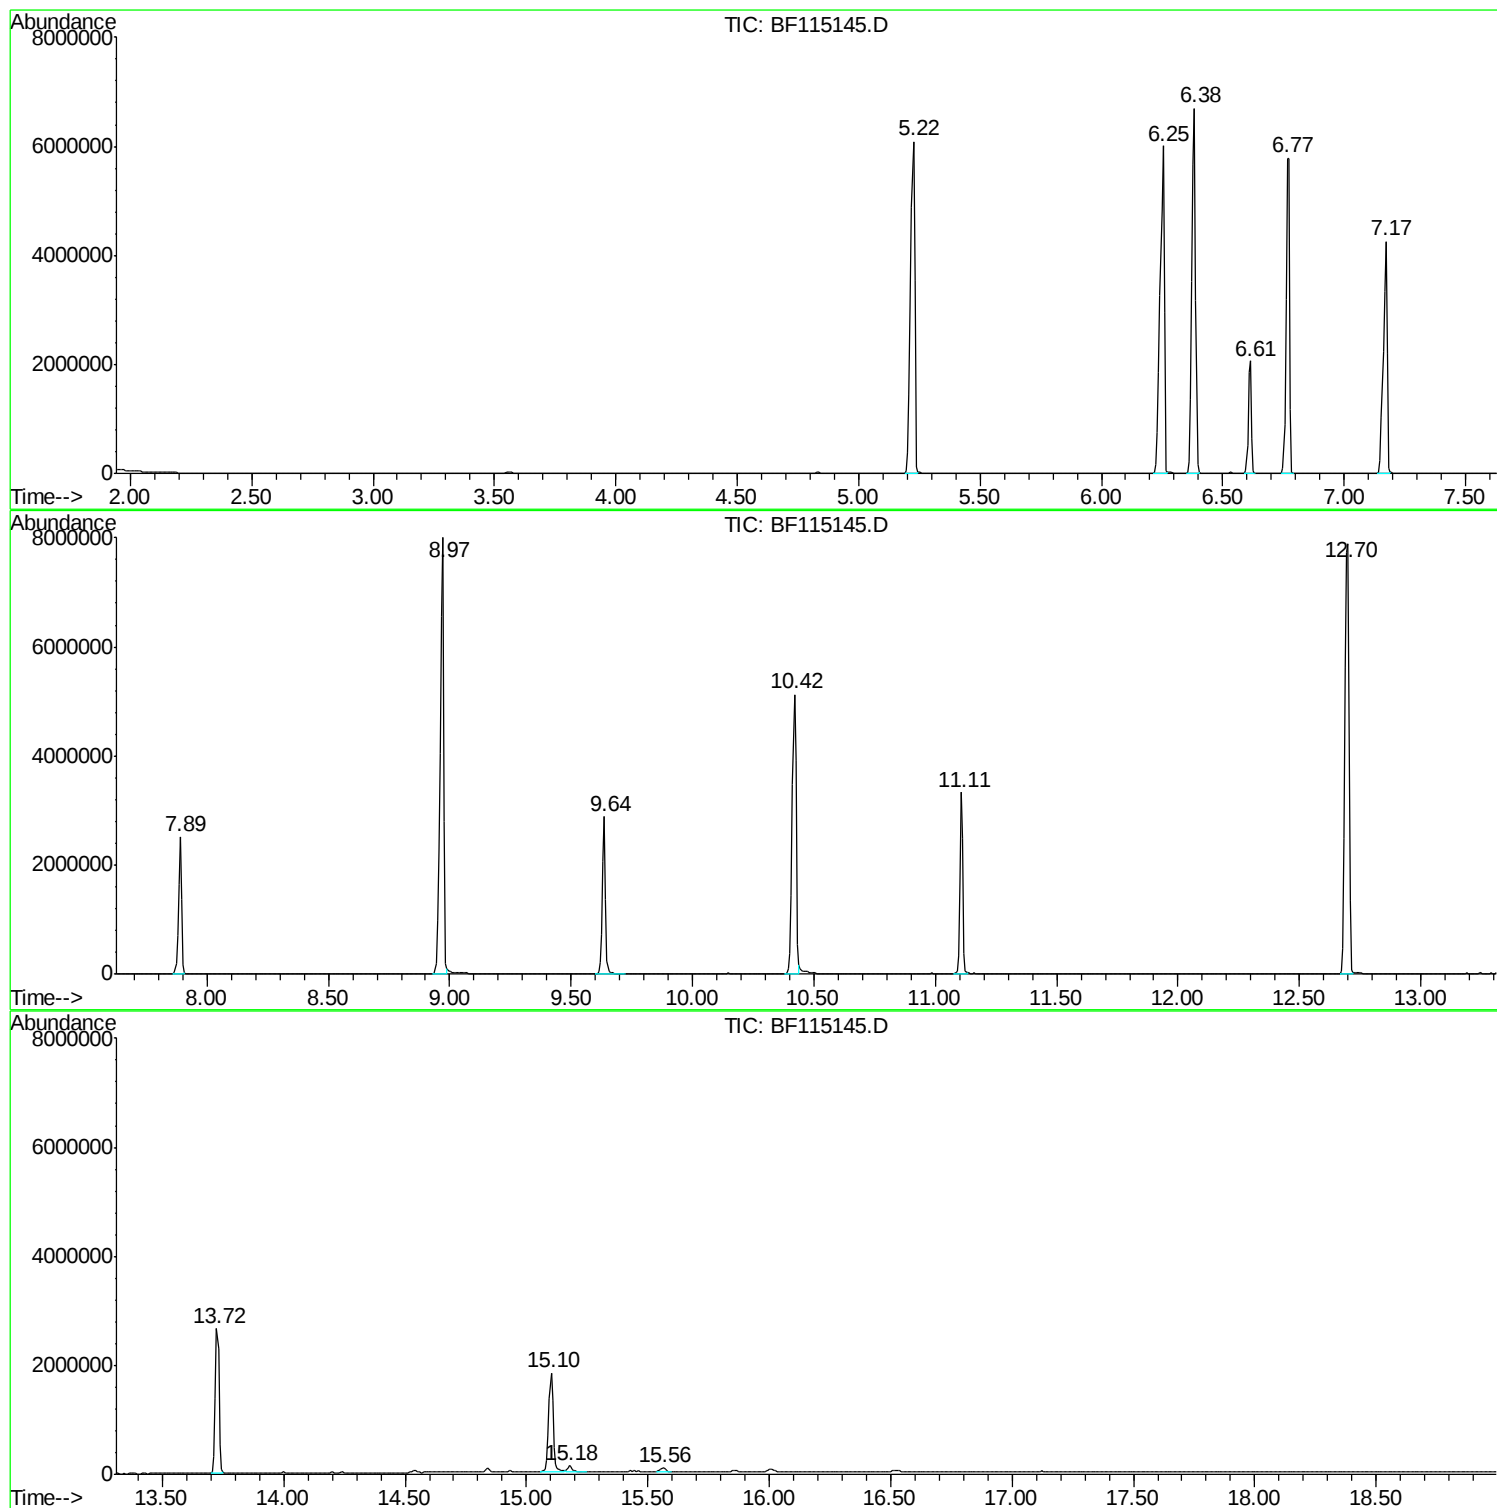

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062419\
Data File : BF115145.D
Acq On : 24 Jun 2019 12:58
Operator : HP/JU
Sample : PB120809BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120809BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	81.10 ng	7343130	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		Xenon	132	Xe	007440-63-3	9
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

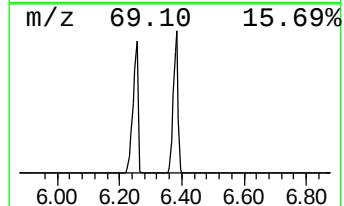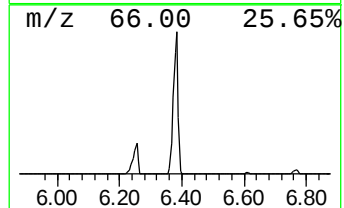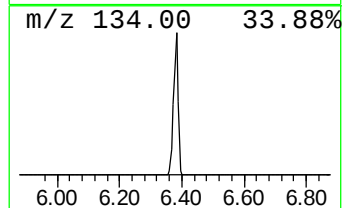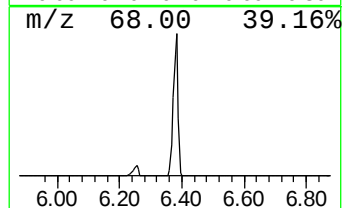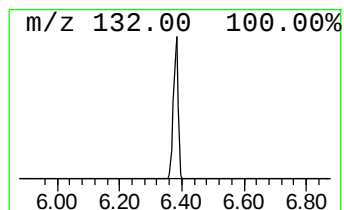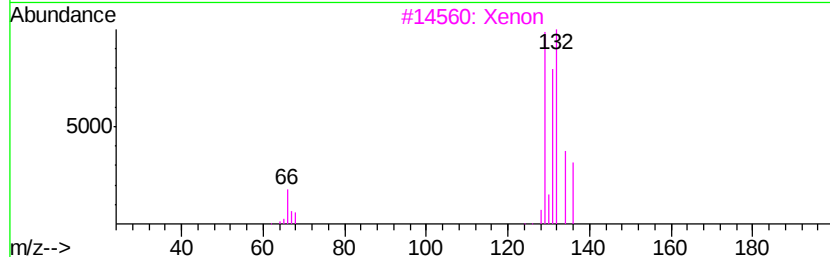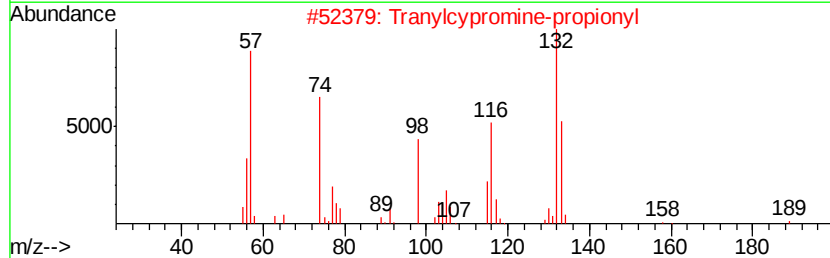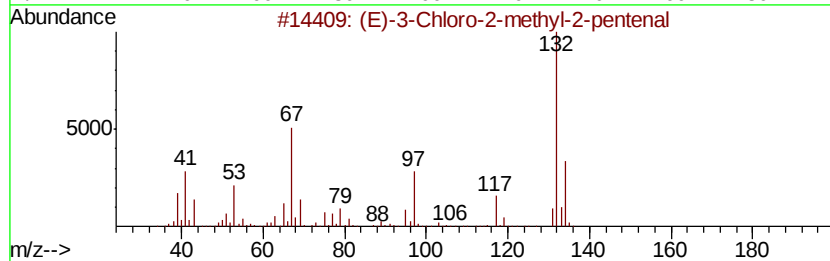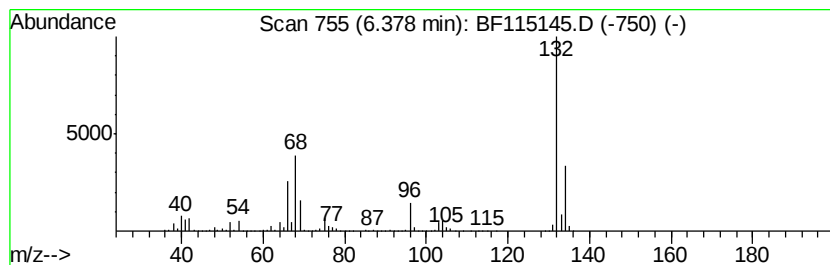

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062419\
Data File : BF115145.D
Acq On : 24 Jun 2019 12:58
Operator : HP/JU
Sample : PB120809BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120809BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.38	6.38	81.1	ng	7343130	1	6.61	1810820	20.0