

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062419\
 Data File : BF115147.D
 Acq On : 24 Jun 2019 13:51
 Operator : HP/JU
 Sample : PB120851BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120851BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.549	263	274	281	rVB	359450	571516	6.34%	0.836%
2	5.225	552	559	562	rBV	5751479	6618715	73.43%	9.680%
3	6.254	727	734	737	rBV	5898589	6733776	74.71%	9.848%
4	6.384	750	756	759	rBV	6617641	7034393	78.05%	10.288%
5	6.613	791	795	798	rBV	2108687	1774912	19.69%	2.596%
6	6.772	817	822	825	rBV	5759421	5747484	63.77%	8.406%
7	7.172	884	890	893	rBV	4159090	4562121	50.62%	6.672%
8	7.889	1007	1012	1015	rBV	2449274	2271248	25.20%	3.322%
9	8.972	1189	1196	1199	rBV	7812075	8461043	93.87%	12.374%
10	9.636	1303	1309	1324	rBV	2945674	2666948	29.59%	3.900%
11	10.419	1435	1442	1445	rBV	4960952	5192841	57.61%	7.594%
12	11.107	1555	1559	1563	rBV	3372916	2896121	32.13%	4.236%
13	12.701	1824	1830	1833	rBV	7643913	9013224	100.00%	13.182%
14	13.724	2000	2004	2008	rBV	2763700	2590110	28.74%	3.788%
15	15.089	2231	2236	2245	rBV	1967573	2242544	24.88%	3.280%


Sum of corrected areas: 68376996

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062419\
Data File : BF115147.D
Acq On : 24 Jun 2019 13:51
Operator : HP/JU
Sample : PB120851BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120851BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

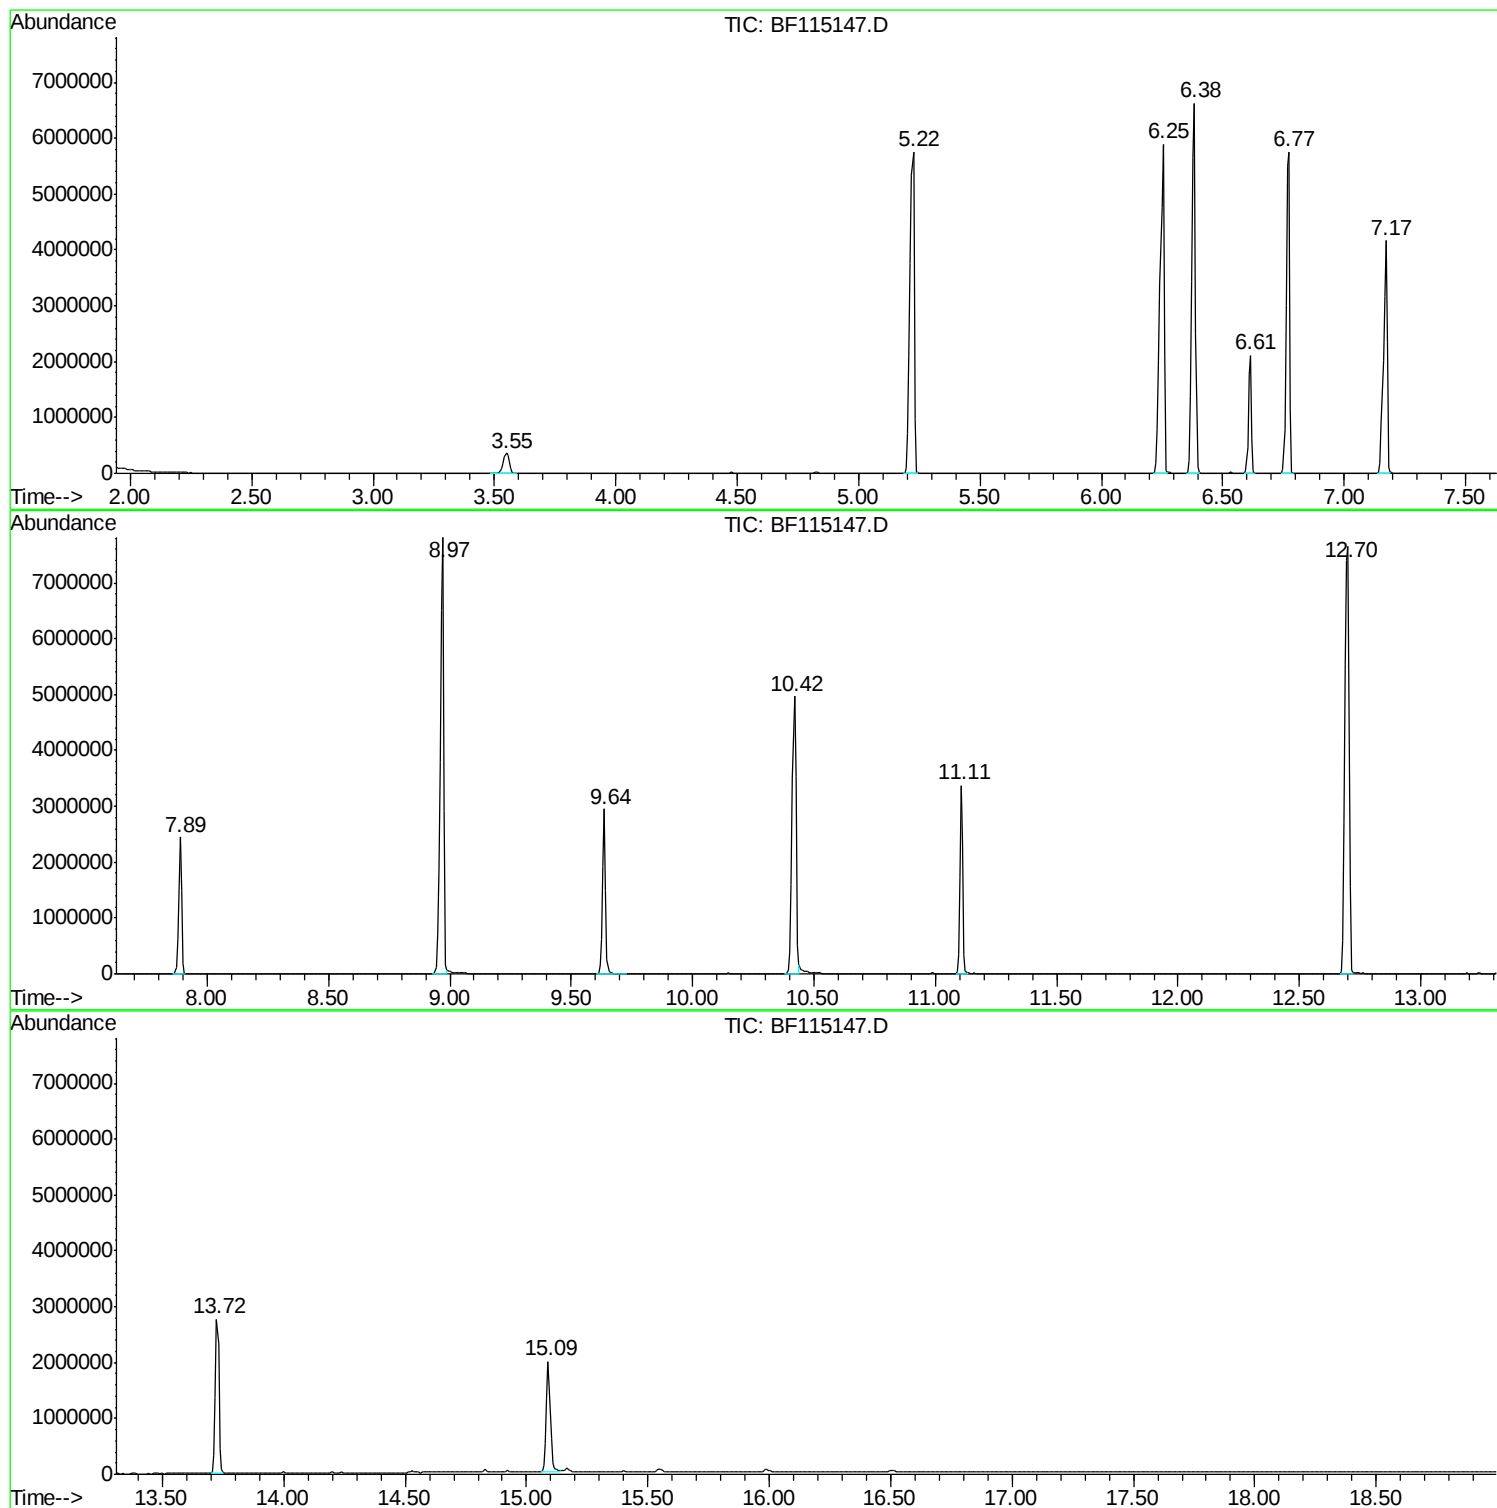

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062419\
Data File : BF115147.D
Acq On : 24 Jun 2019 13:51
Operator : HP/JU
Sample : PB120851BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120851BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	79.26 ng	7034390	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	16
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

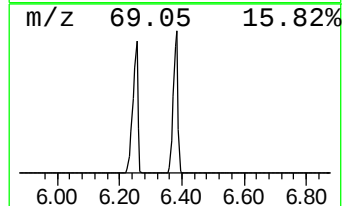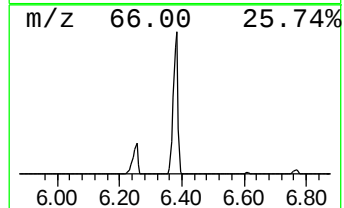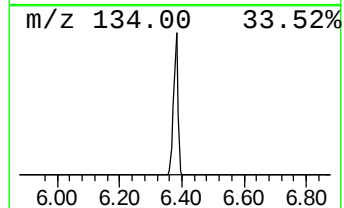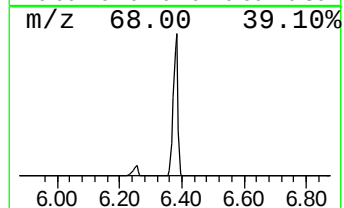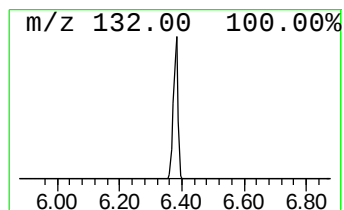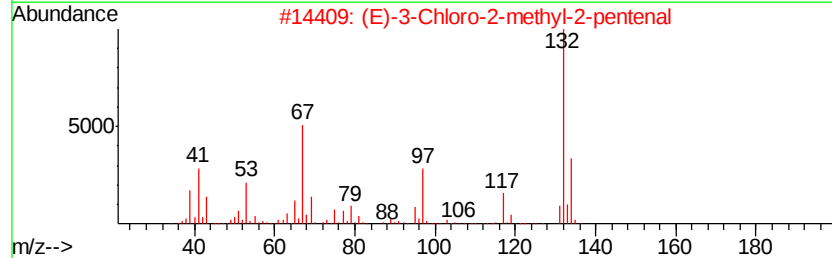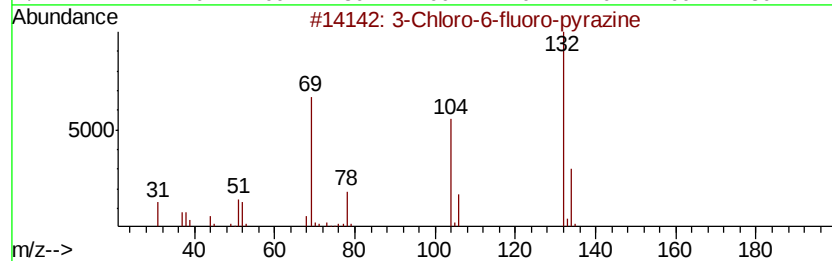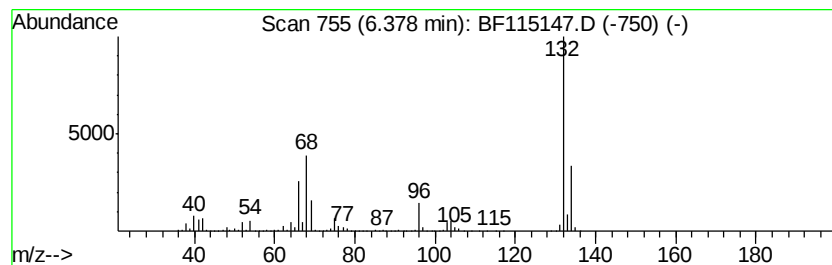

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062419\
Data File : BF115147.D
Acq On : 24 Jun 2019 13:51
Operator : HP/JU
Sample : PB120851BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120851BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.38	6.38	79.3	ng	7034390	1	6.61	1774910	20.0