


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062419\
 Data File : BF115140.D
 Acq On : 24 Jun 2019 10:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 24 04:21:29 2019

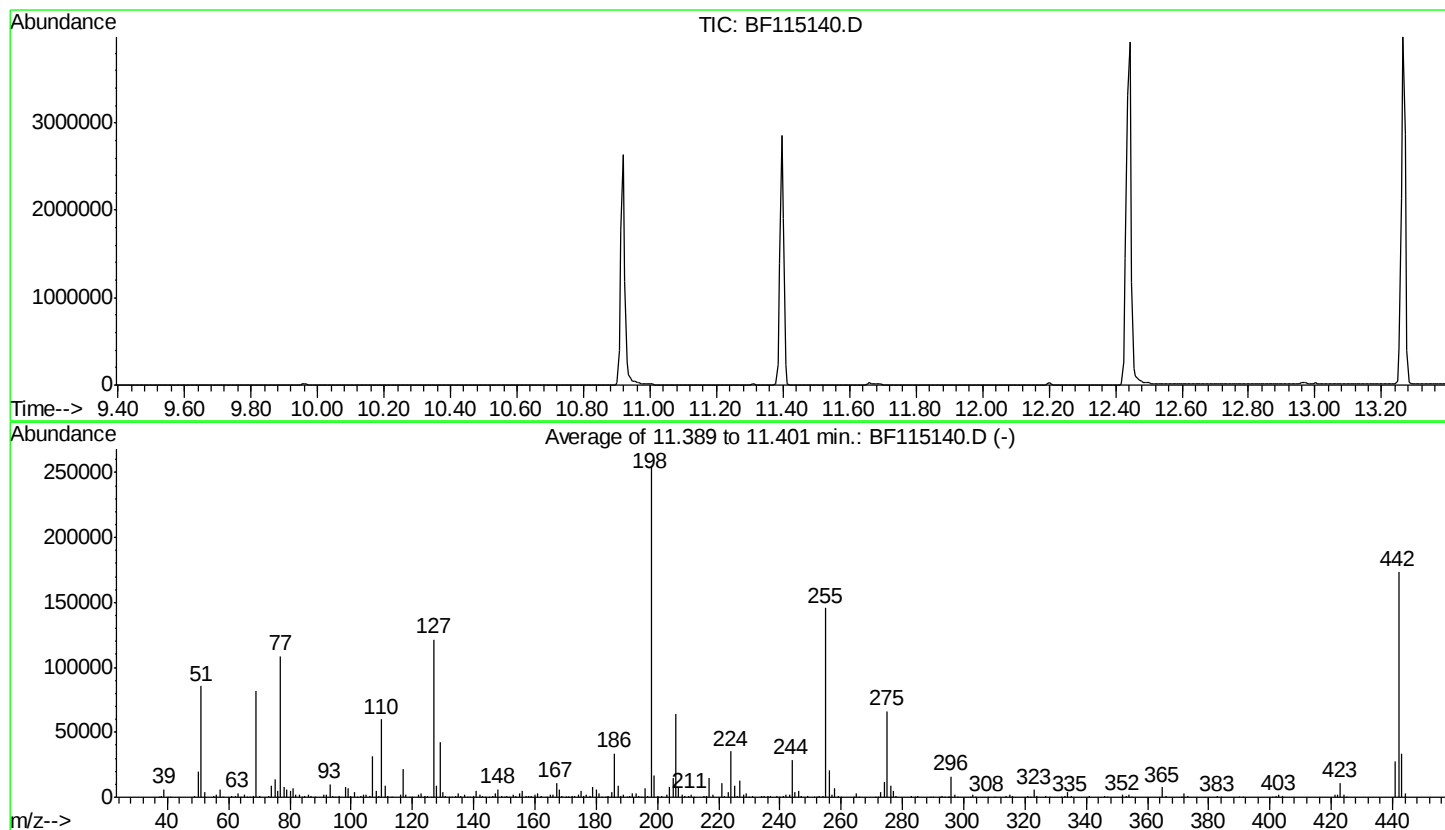

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	85549	PASS
68	69	0.00	2	1.7	1375	PASS
69	198	0.00	100	32.1	81853	PASS
70	69	0.00	2	0.6	530	PASS
127	198	10	80	47.5	121429	PASS
197	198	0.00	2	0.6	1512	PASS
198	198	100	100	100.0	255381	PASS
199	198	5	9	6.4	16460	PASS
275	198	10	60	26.0	66429	PASS
365	198	1	100	2.9	7461	PASS
441	198	0.01	100	10.8	27672	PASS
442	198	50	100	68.1	173824	PASS
443	442	15	24	19.3	33633	PASS