


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062419\
 Data File : BF115152.D
 Acq On : 24 Jun 2019 17:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 24 04:21:29 2019

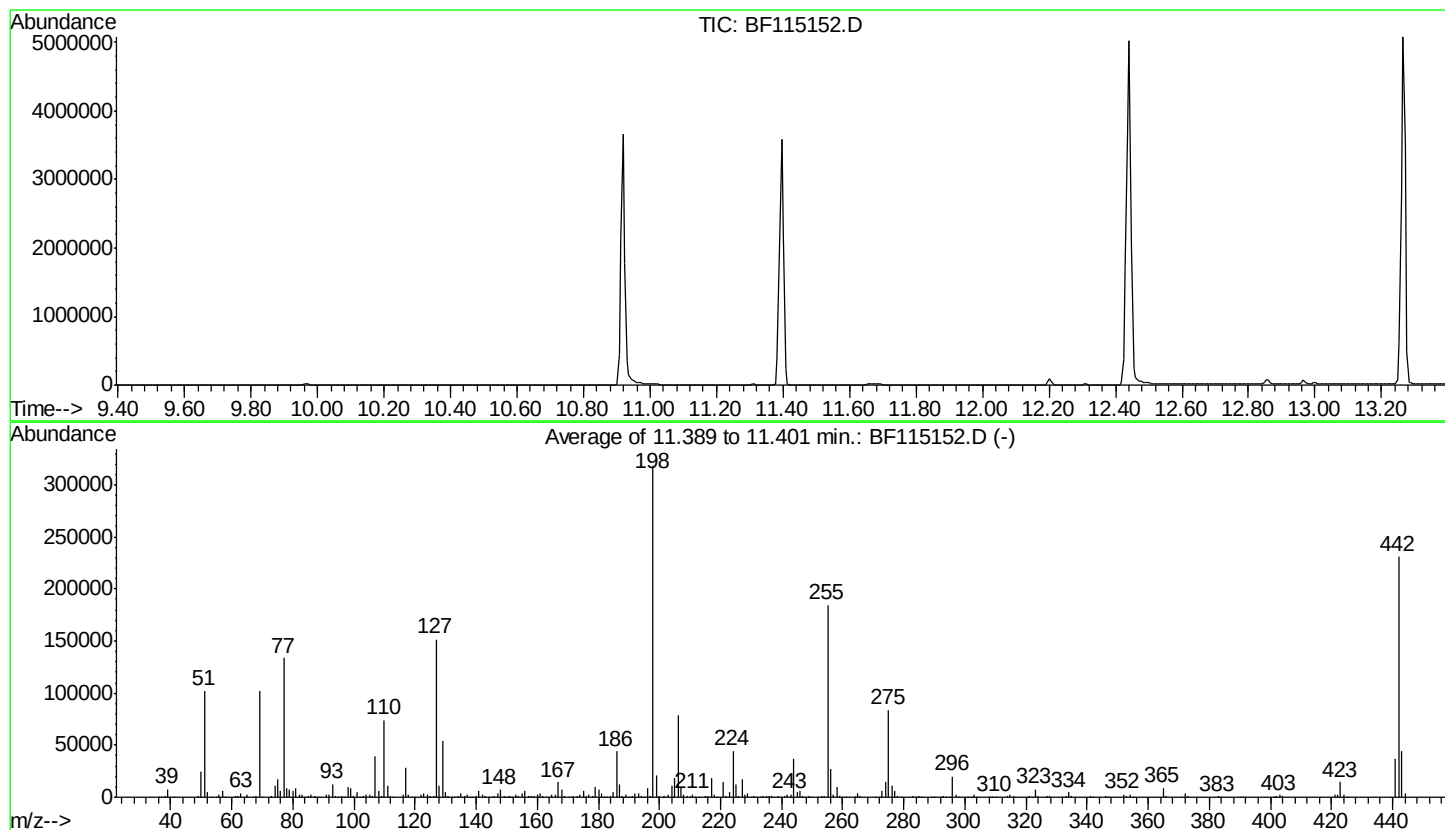

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	102437	PASS
68	69	0.00	2	1.7	1740	PASS
69	198	0.00	100	32.2	102381	PASS
70	69	0.00	2	0.6	591	PASS
127	198	10	80	47.6	151616	PASS
197	198	0.00	2	0.6	1752	PASS
198	198	100	100	100.0	318357	PASS
199	198	5	9	6.7	21306	PASS
275	198	10	60	26.4	84104	PASS
365	198	1	100	2.9	9206	PASS
441	198	0.01	100	11.4	36434	PASS
442	198	50	100	72.5	230962	PASS
443	442	15	24	19.0	43834	PASS