
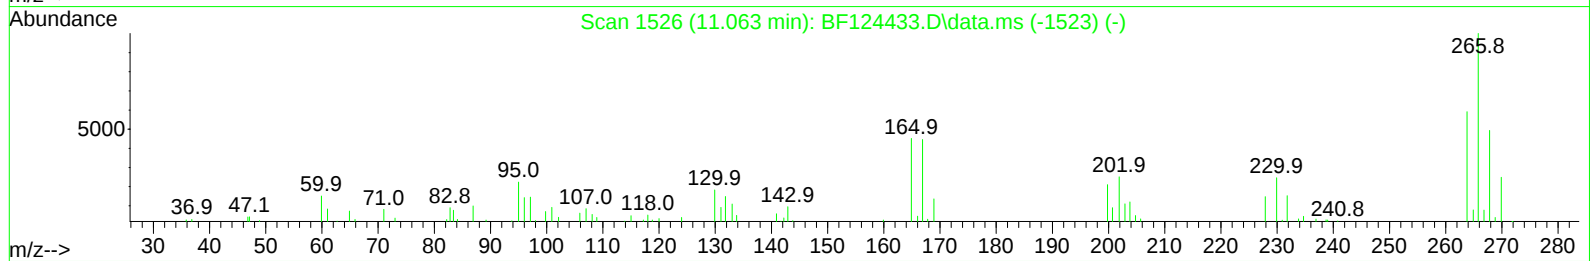
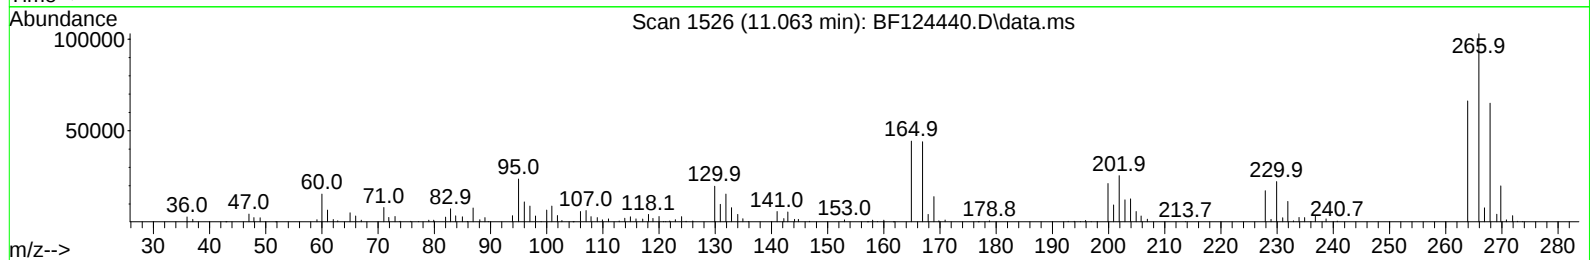


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062421\
Data File : BF124440.D
Acq On : 24 Jun 2021 13:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 13:42:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 18:48:27 2021
Response via : Initial Calibration

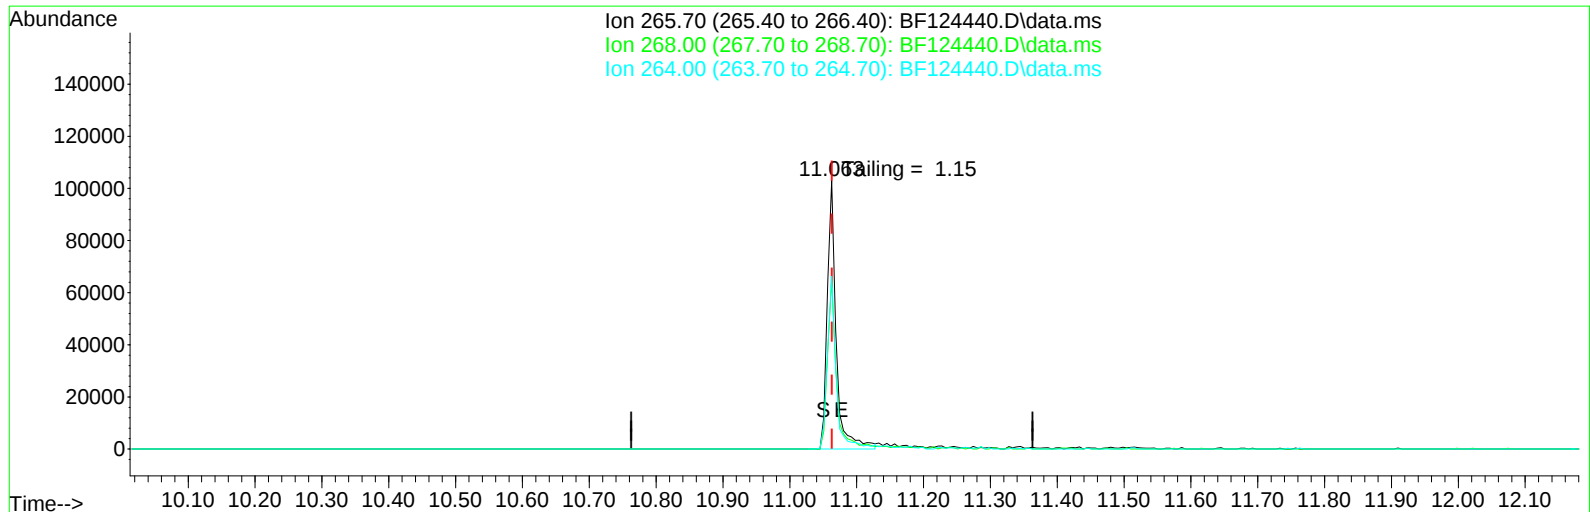

TIC: BF124440.D\data.ms

(70) Pentachlorophenol (C)




11.063min (-0.000) 236640.23 ng

response 100595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.16
264.00	65.70	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062421\
 Data File : BF124440.D
 Acq On : 24 Jun 2021 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 13:42:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 18:48:27 2021
 Response via : Initial Calibration

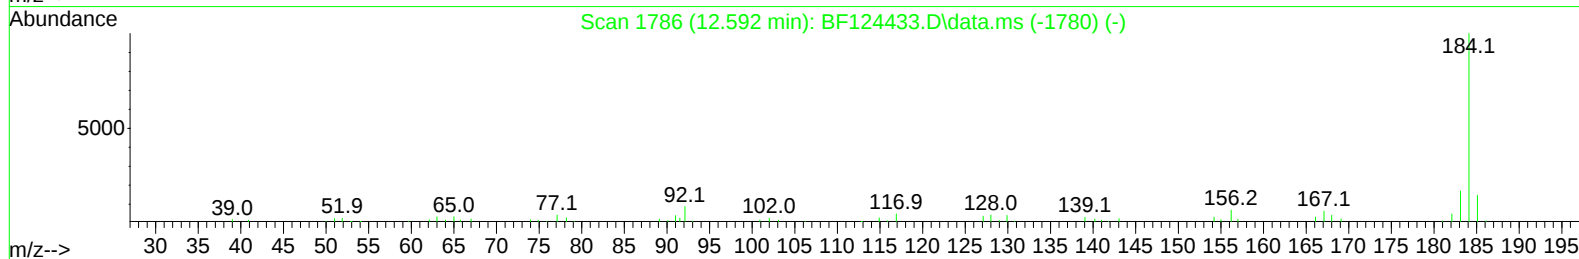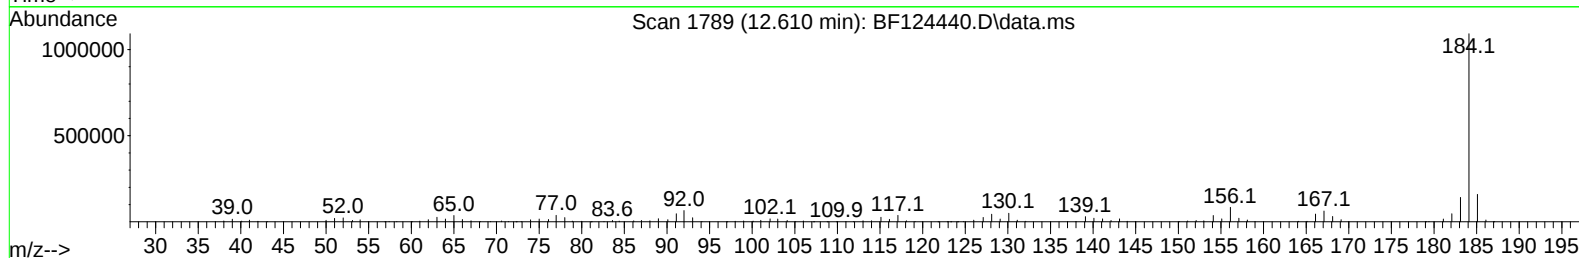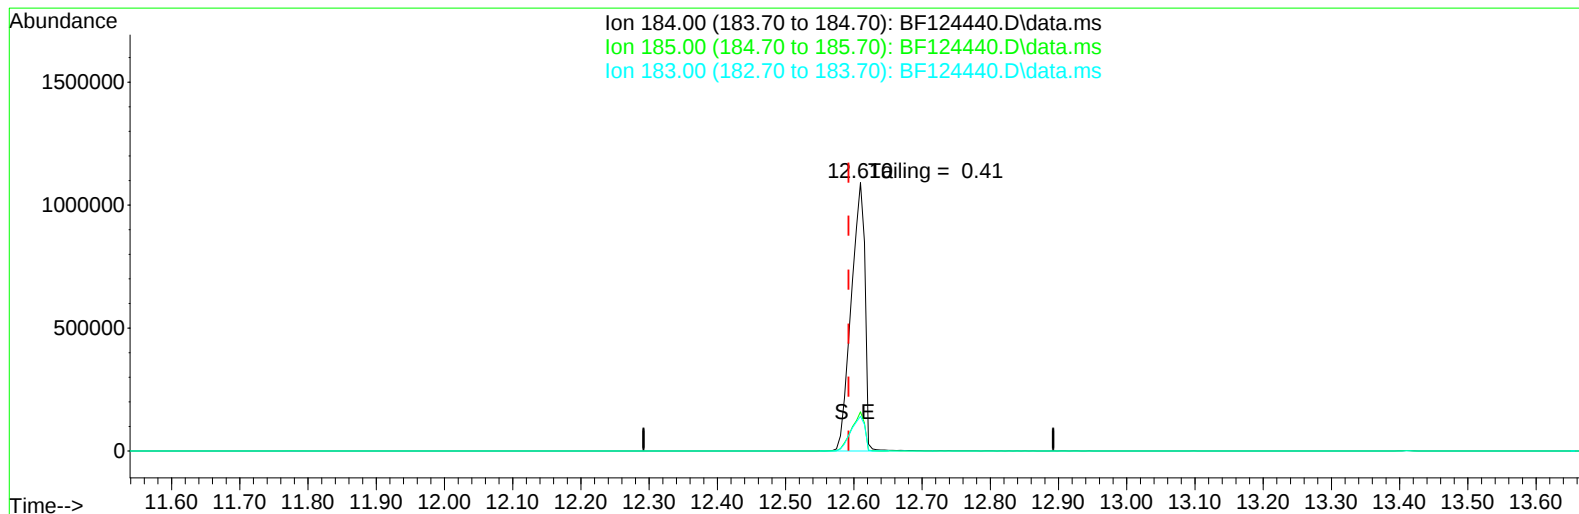

TIC: BF124440.D\data.ms

(77) Benzidine**12.610min (+ 0.018) 471370.95 ng****response 1530386**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.62
183.00	9.80	12.93#
0.00	0.00	0.00