
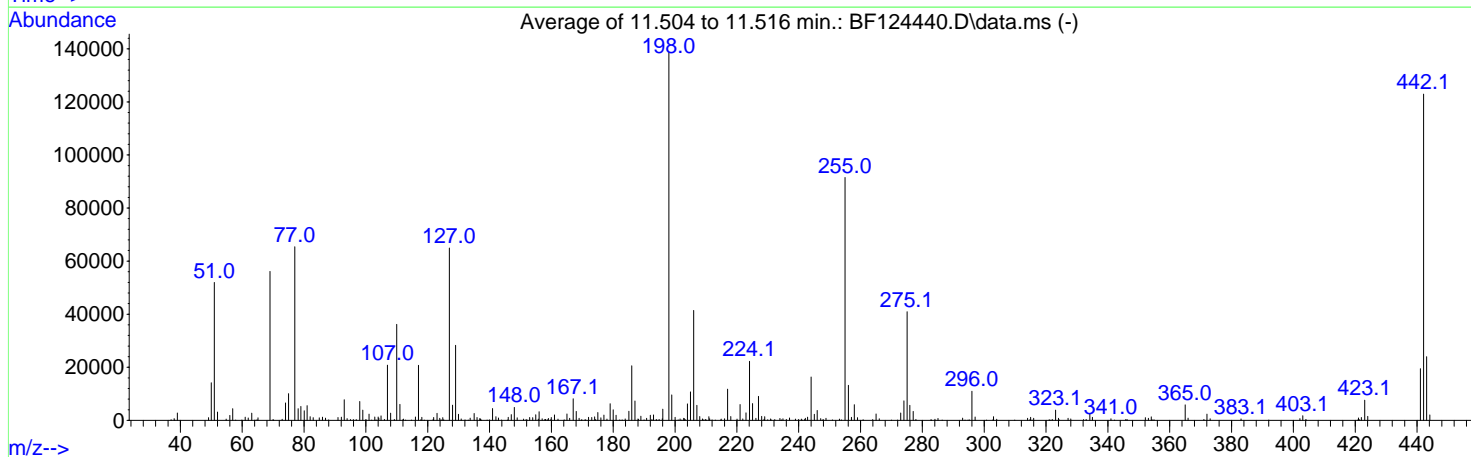


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062421\
 Data File : BF124440.D
 Acq On : 24 Jun 2021 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 23 18:48:27 2021

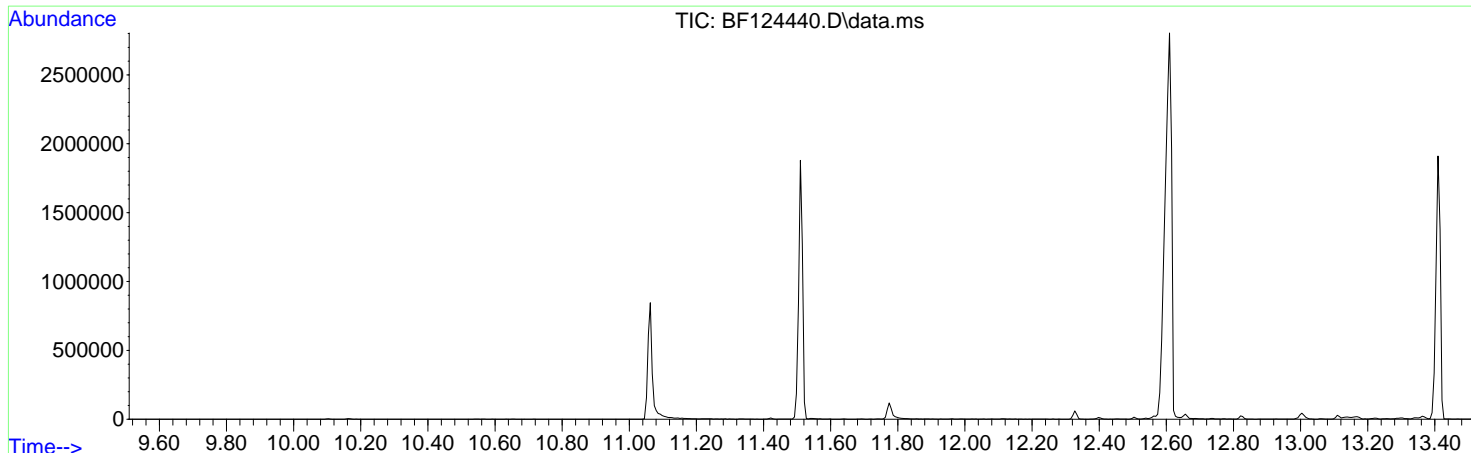




AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	51944	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.5	56115	PASS
70	69	0.00	2	0.6	319	PASS
127	198	10	80	46.8	64907	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	138611	PASS
199	198	5	9	6.9	9587	PASS
275	198	10	60	29.5	40923	PASS
365	198	1	100	4.2	5867	PASS
441	198	0.01	100	14.1	19490	PASS
442	442	50	100	100.0	122939	PASS
443	442	15	24	19.5	24004	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062421\
 Data File : BF124440.D
 Acq On : 24 Jun 2021 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Quant Time: Jun 24 13:42:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 18:48:27 2021
 Response via : Initial Calibration

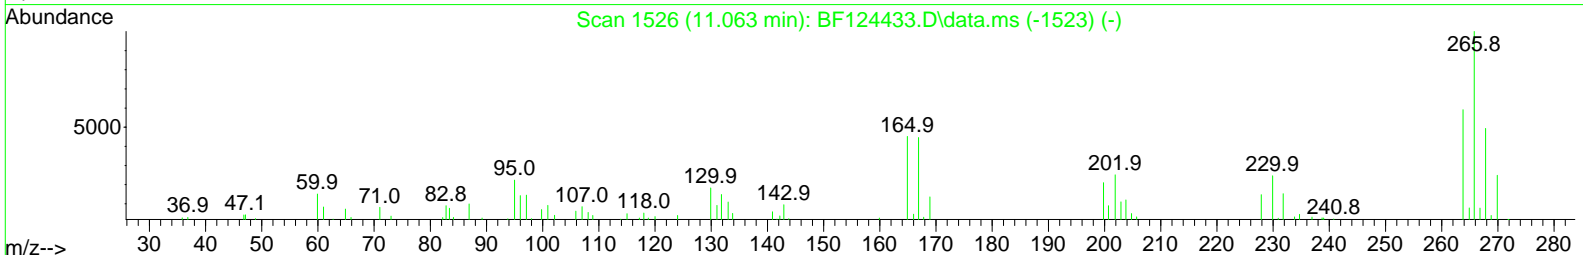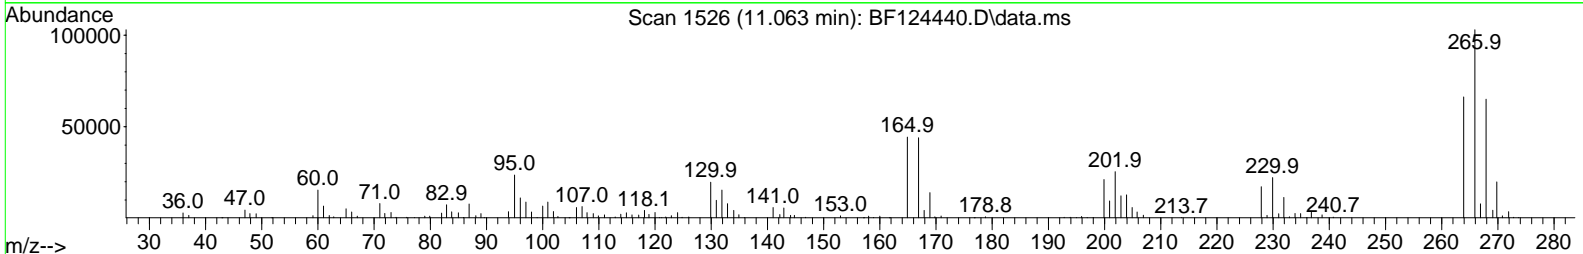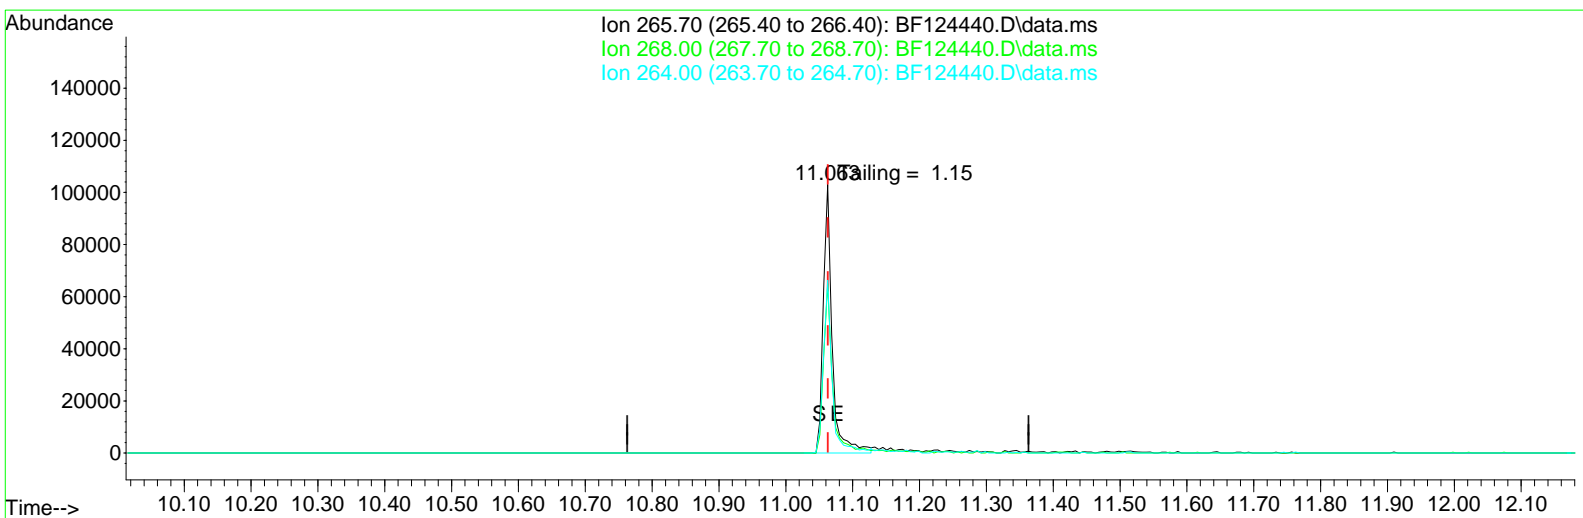

TIC: BF124440.D\data.ms

(70) Pentachlorophenol (C)




11.063min (-0.000) 236640.23 ng

response	100595	
Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.16
264.00	65.70	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062421\
 Data File : BF124440.D
 Acq On : 24 Jun 2021 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 24 13:42:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 18:48:27 2021
 Response via : Initial Calibration

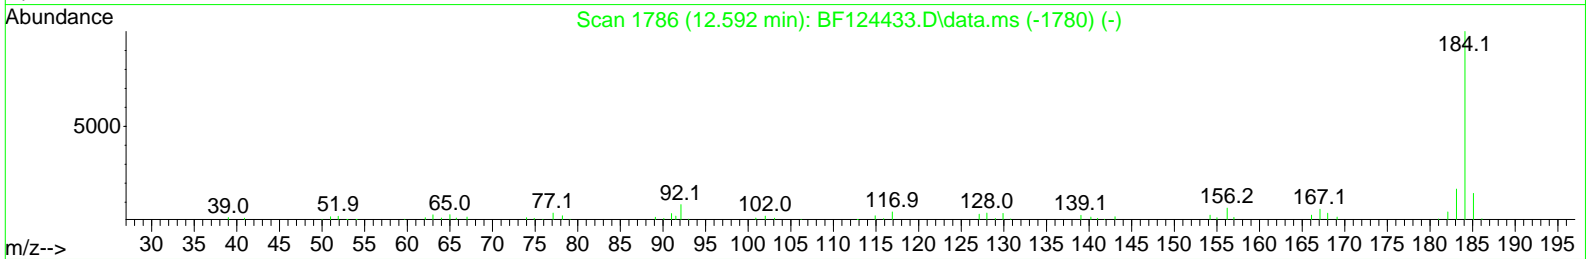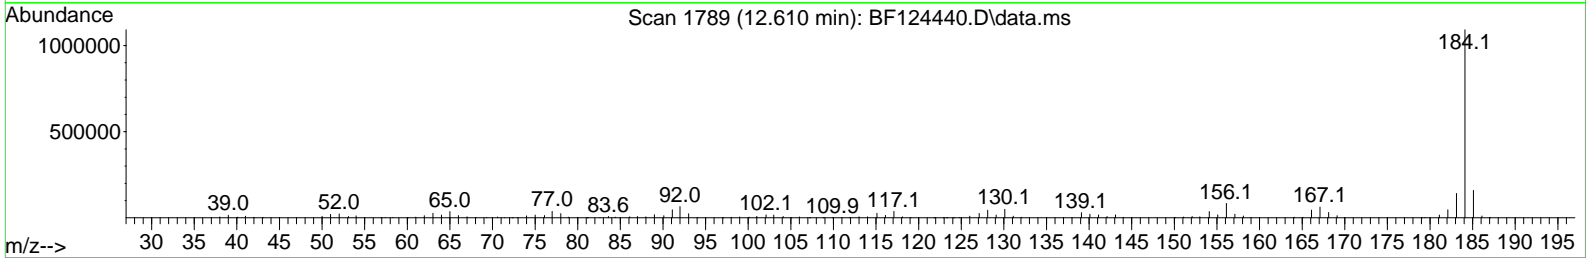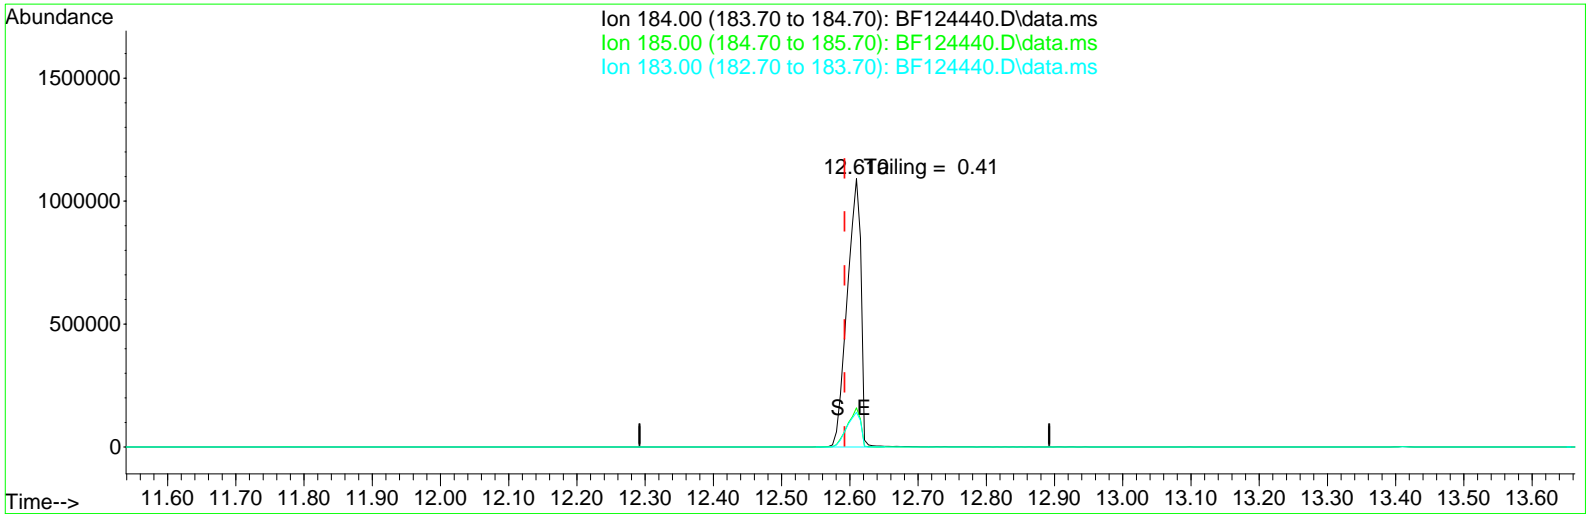

TIC: BF124440.D\data.ms

(77) Benzidine

12.610min (+ 0.018) 471370.95 ng

response 1530386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.62
183.00	9.80	12.93#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/24/2021	BNA_F	<u>BF124440.D</u>
Compound Name	Response	Retention Time
DDT	326275	13.41
DDD	5513	13.11
DDE	455	12.77
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5968	332243	1.80