
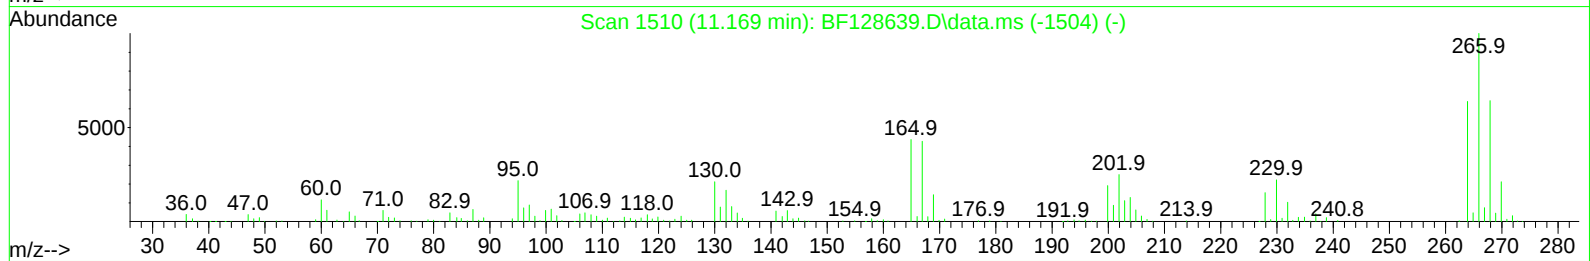
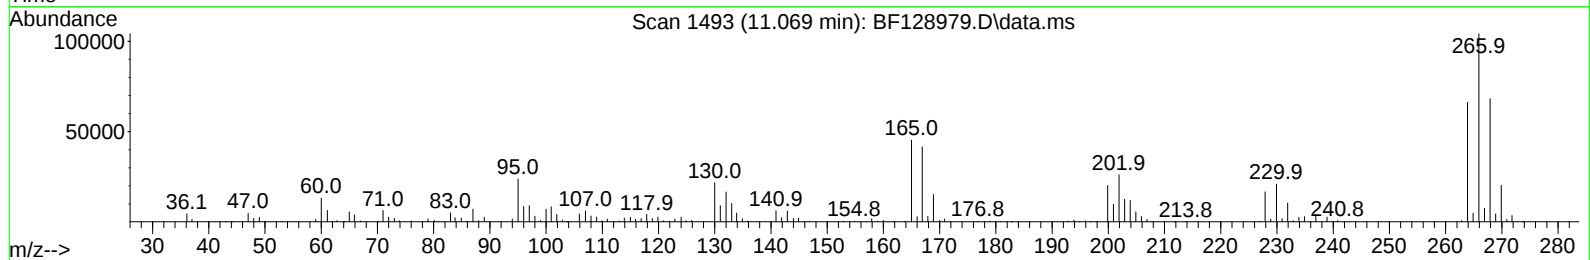


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128979.D
Acq On : 24 Jun 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 05:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:50:48 2022
Response via : Initial Calibration

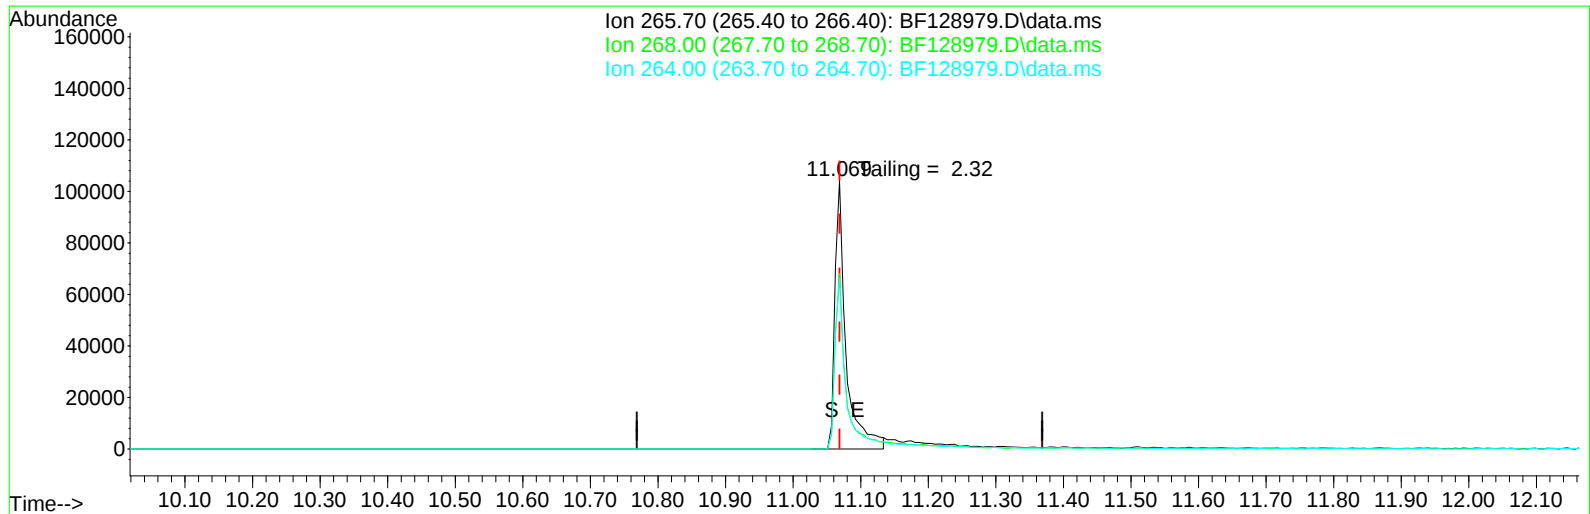

TIC: BF128979.D\data.ms

(70) Pentachlorophenol (C)




11.069min (0.000) 33150.78 ng

response 124812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.49
264.00	61.80	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128979.D
Acq On : 24 Jun 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 05:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:50:48 2022
Response via : Initial Calibration

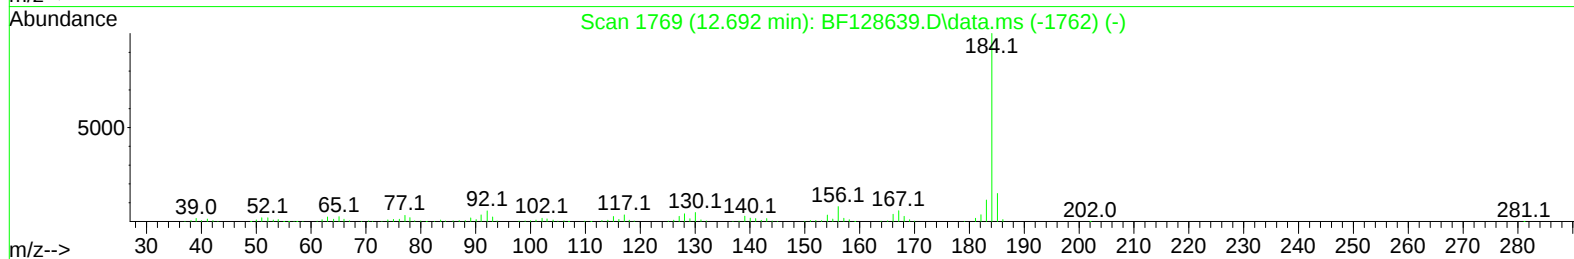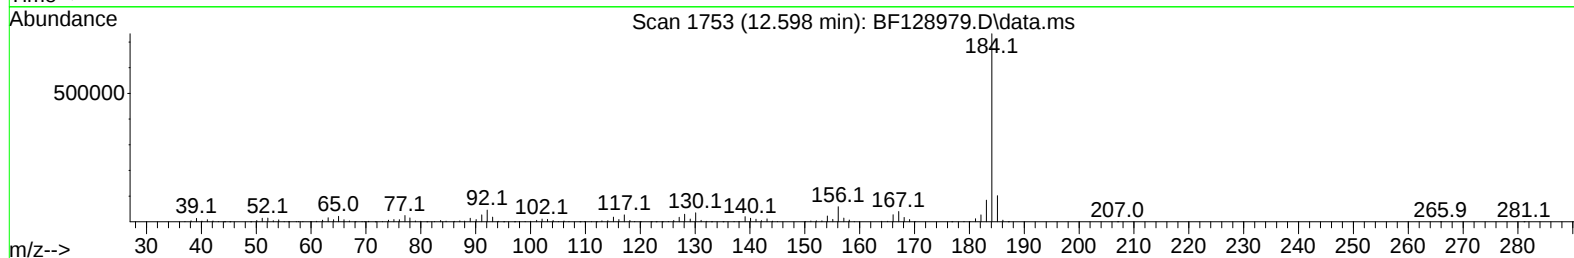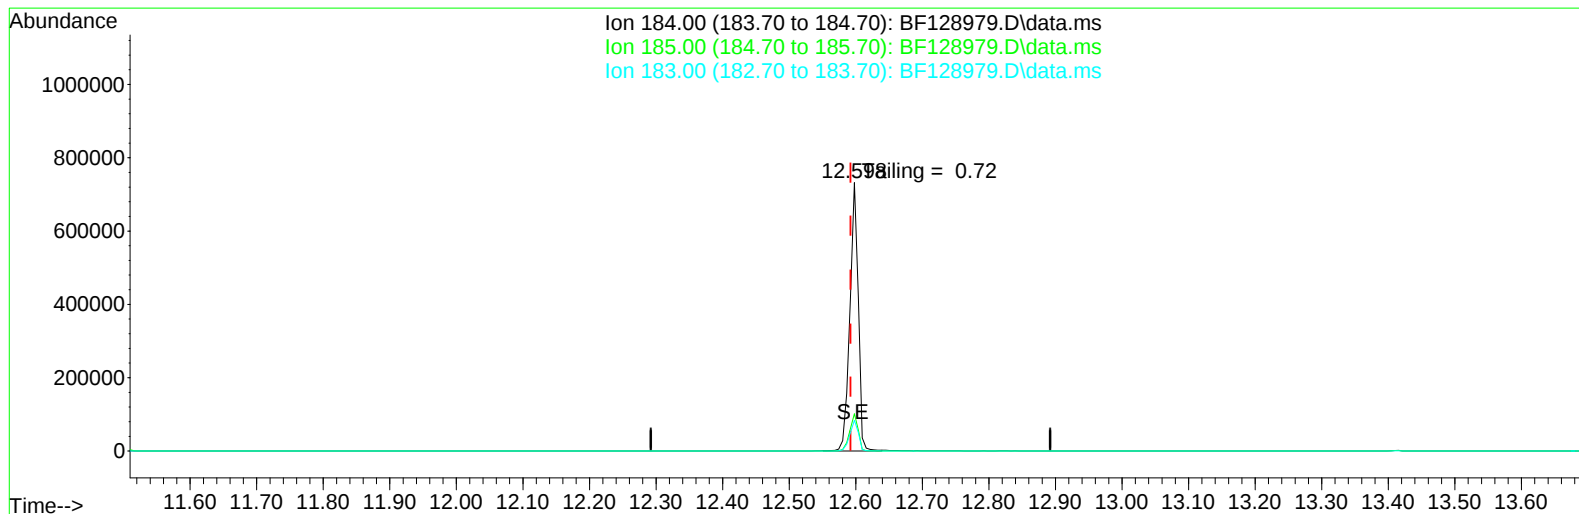

TIC: BF128979.D\data.ms

(77) Benzidine

12.598min (+ 0.006) 0.00 ng

response 649533

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.89
183.00	11.60	11.48
0.00	0.00	0.00