

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
 Data File : BF128981.D
 Acq On : 24 Jun 2022 11:01
 Operator : CG\JU
 Sample : PB145742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145742BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.975	452	457	467	rBV	31436	50724	1.06%	0.175%
2	5.369	520	524	546	rBV	3673077	3773088	79.12%	13.040%
3	6.387	692	697	700	rBV	3514819	3746449	78.56%	12.948%
4	6.722	750	754	761	rBV	971494	797063	16.71%	2.755%
5	7.292	845	851	854	rBV	2285908	2658420	55.74%	9.188%
6	8.004	967	972	976	rBV	1114150	1042440	21.86%	3.603%
7	9.086	1149	1156	1159	rBV	4681535	4745455	99.51%	16.400%
8	9.763	1265	1271	1274	rBV	1346940	1193927	25.04%	4.126%
9	10.557	1400	1406	1427	rBV	2707902	2729223	57.23%	9.432%
10	11.251	1518	1524	1527	rBV	1504676	1230478	25.80%	4.253%
11	12.845	1786	1795	1798	rBV	4880807	4768926	100.00%	16.481%
12	13.898	1970	1974	1977	rBV	1168088	998538	20.94%	3.451%
13	13.986	1983	1989	1996	rBV	138279	167769	3.52%	0.580%
14	15.339	2213	2219	2228	rBV	667528	837533	17.56%	2.895%
15	15.757	2286	2290	2296	rVB2	38366	54309	1.14%	0.188%
16	16.233	2368	2371	2379	rVB2	34230	59137	1.24%	0.204%
17	16.451	2402	2408	2410	rBV2	44862	81557	1.71%	0.282%




Sum of corrected areas: 28935036

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128981.D
Acq On : 24 Jun 2022 11:01
Operator : CG\JU
Sample : PB145742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

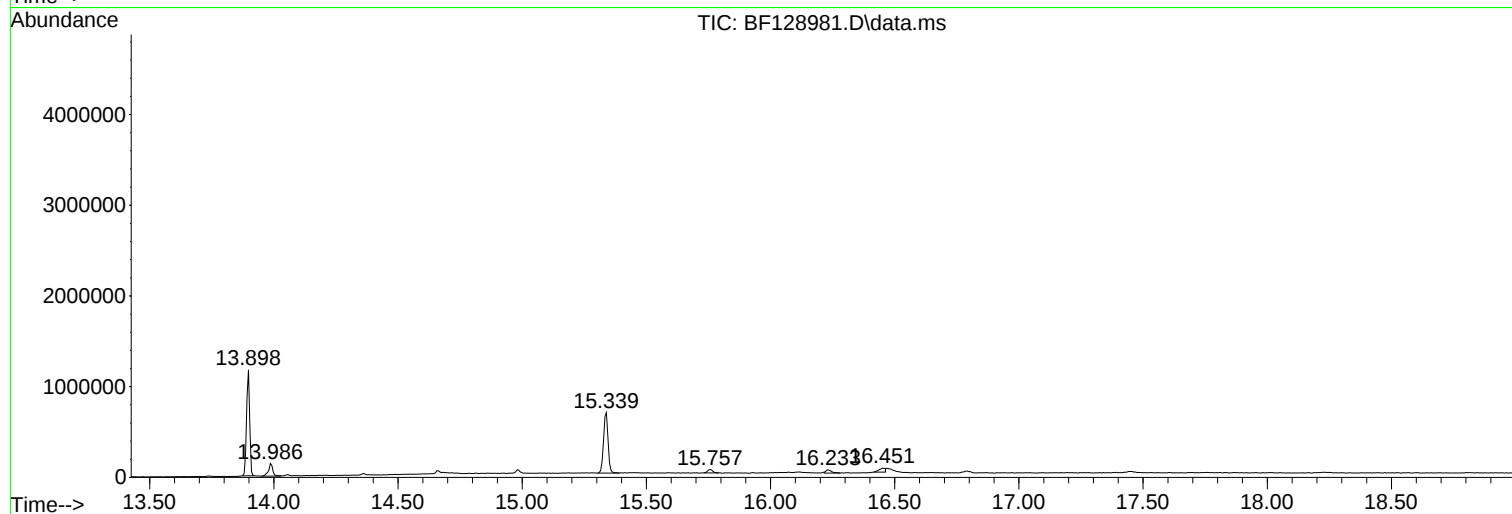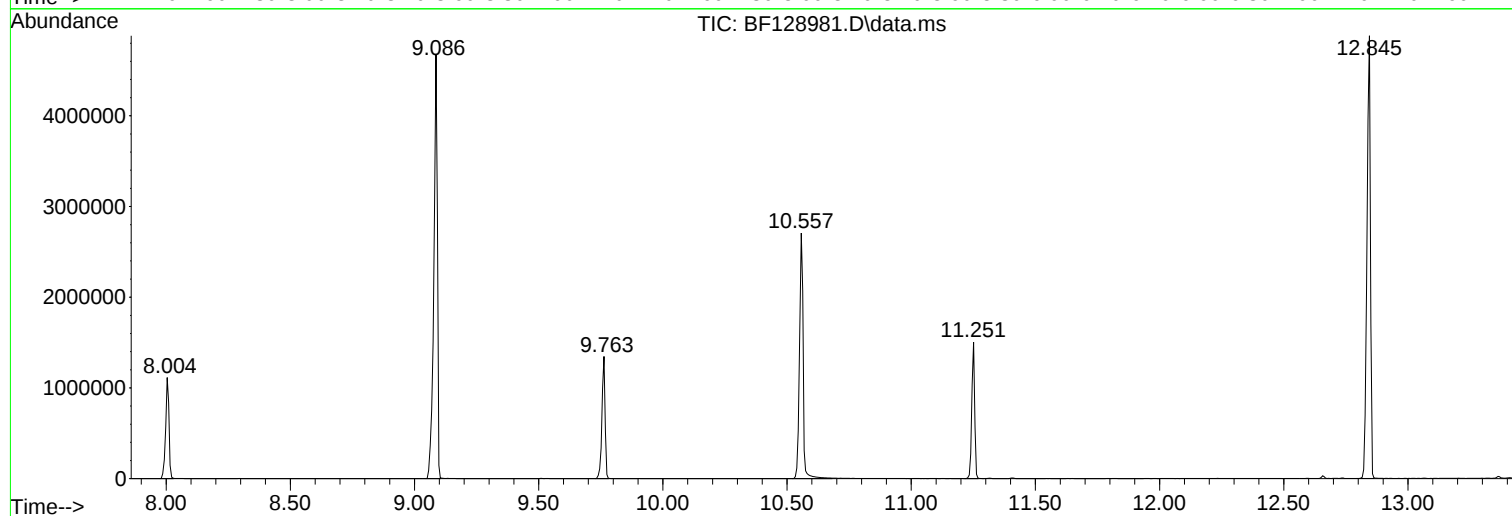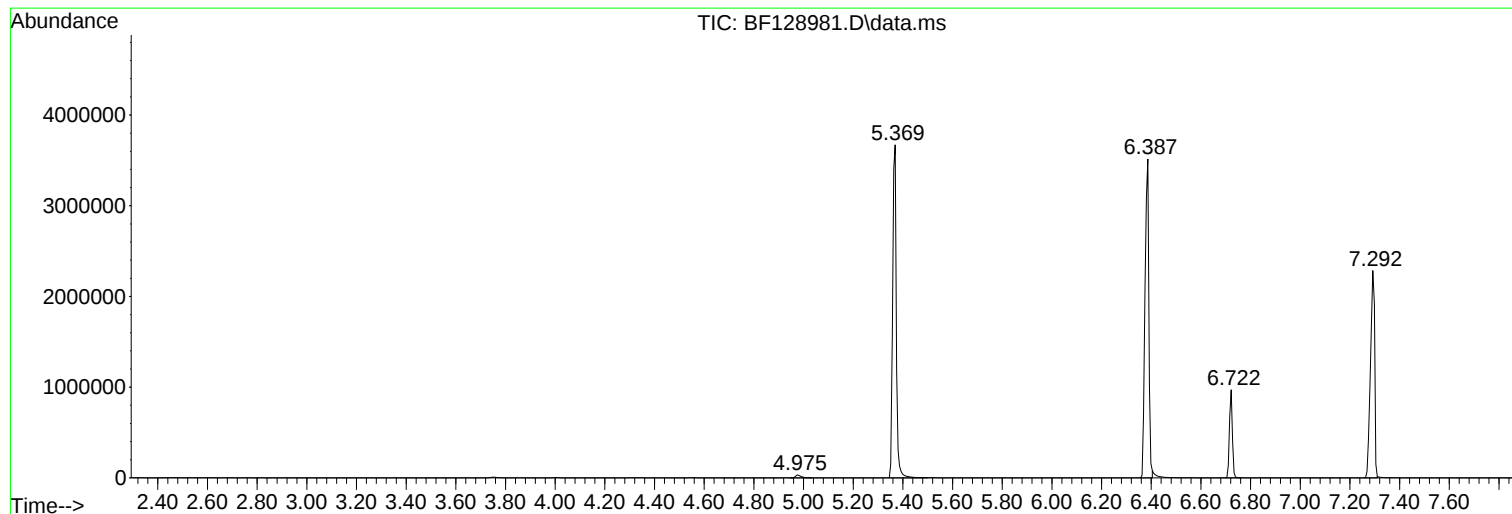

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128981.D
Acq On : 24 Jun 2022 11:01
Operator : CG\JU
Sample : PB145742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145742BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.986	3.36 ng	167769	Chrysene-d12	13.898

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	46
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	38
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	37

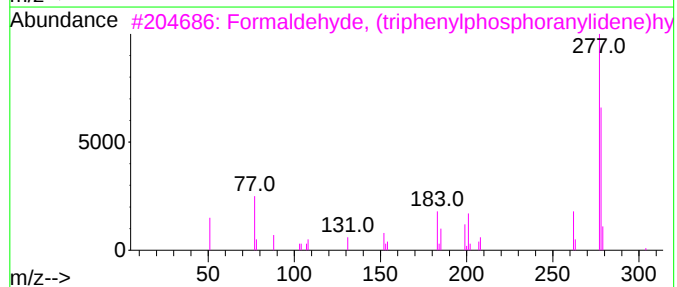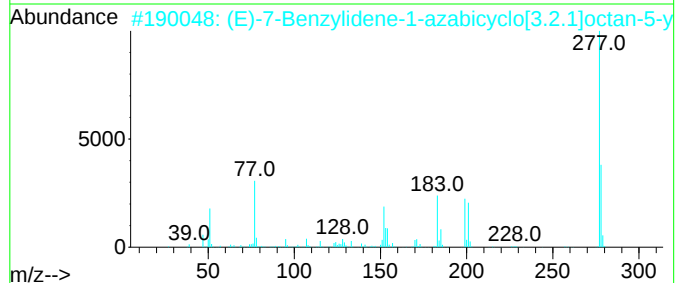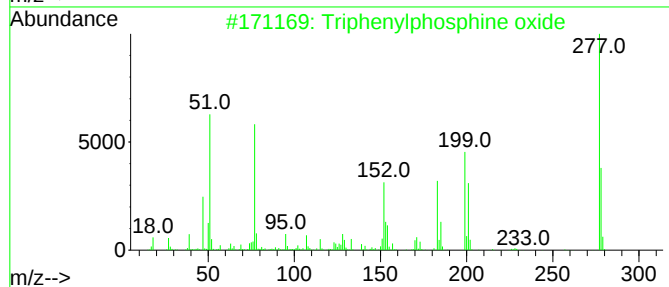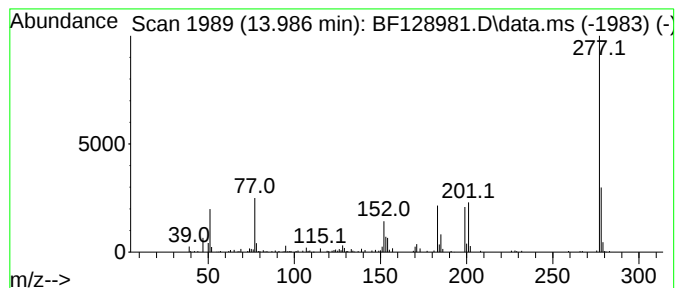

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128981.D
Acq On : 24 Jun 2022 11:01
Operator : CG\JU
Sample : PB145742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.986	3.4	ng	167769	5	13.898	998538	20.0