
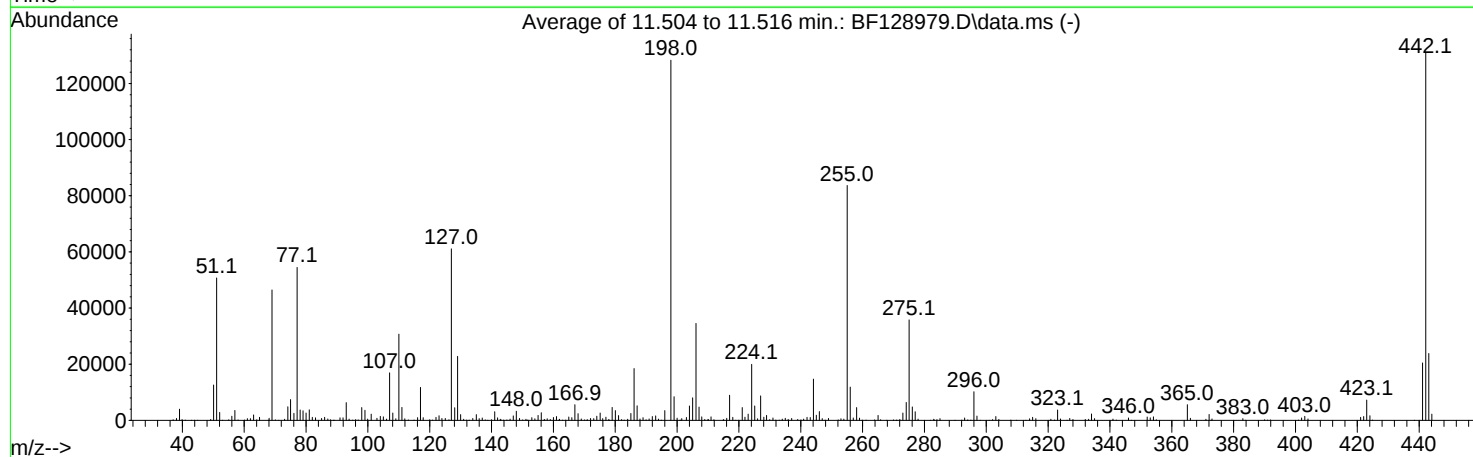


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
 Data File : BF128979.D
 Acq On : 24 Jun 2022 09:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 00:50:48 2022

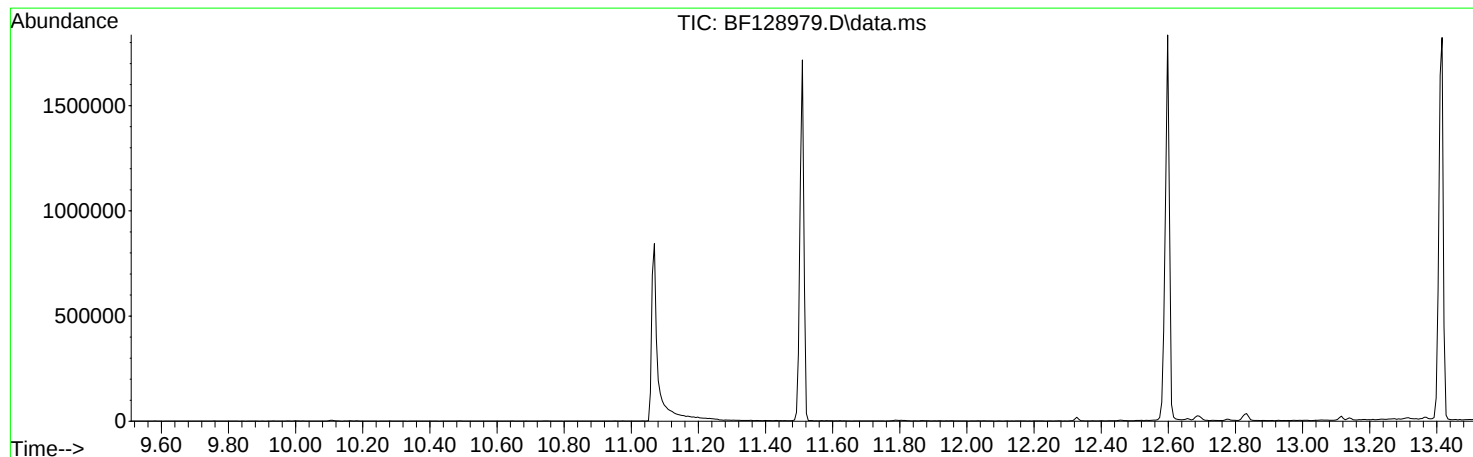




AutoFind: Scans 1567, 1568, 1569; Background Corrected with Scan 1561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	50747	PASS
68	69	0.00	2	1.6	747	PASS
69	198	0.00	100	36.2	46452	PASS
70	69	0.00	2	0.4	180	PASS
127	198	10	80	47.6	61093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128280	PASS
199	198	5	9	6.6	8431	PASS
275	198	10	60	27.9	35789	PASS
365	198	1	100	4.3	5576	PASS
441	198	0.01	100	15.9	20458	PASS
442	442	50	100	100.0	131037	PASS
443	442	15	24	18.2	23835	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128979.D
Acq On : 24 Jun 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 05:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:50:48 2022
Response via : Initial Calibration

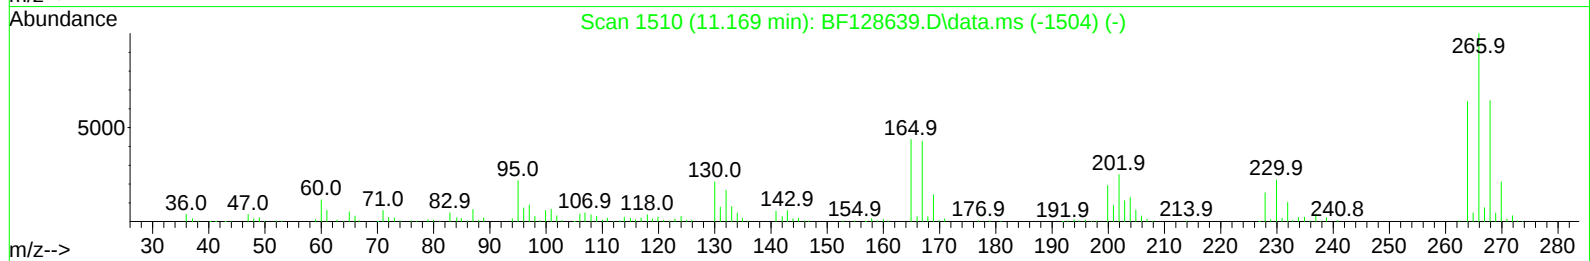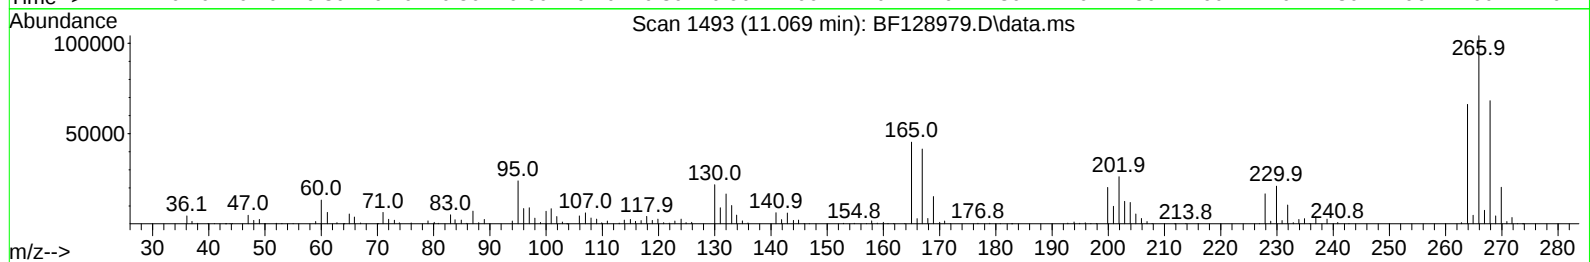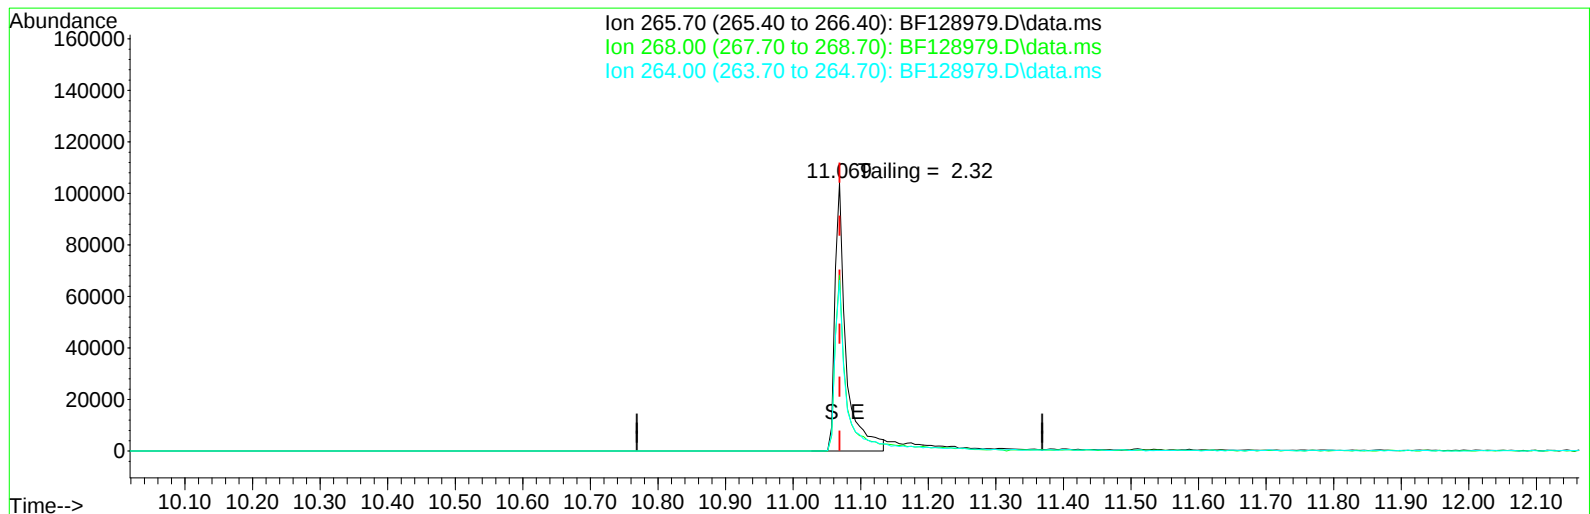

TIC: BF128979.D\data.ms

(70) Pentachlorophenol (C)

11.069min (0.000) 33150.78 ng




response 124812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.49
264.00	61.80	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062422\
Data File : BF128979.D
Acq On : 24 Jun 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 05:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:50:48 2022
Response via : Initial Calibration

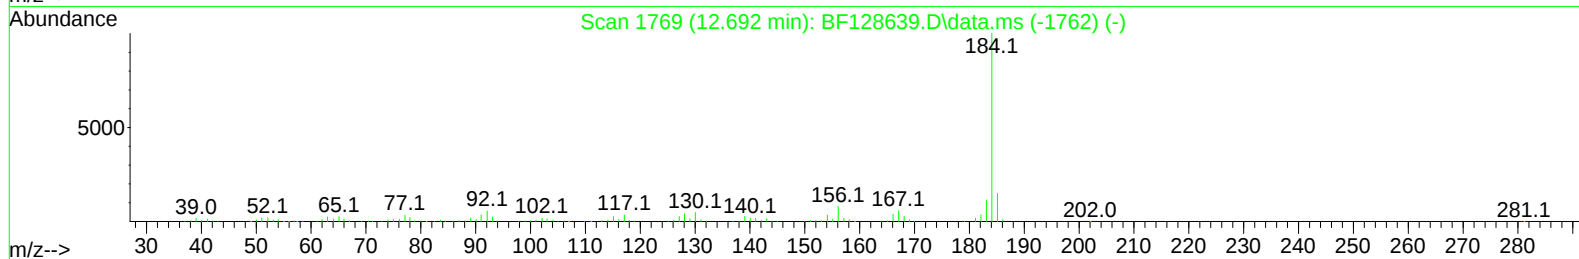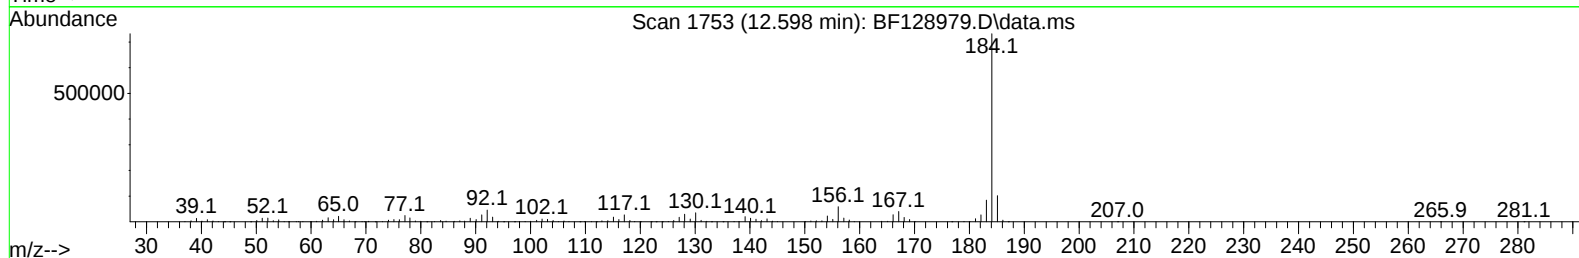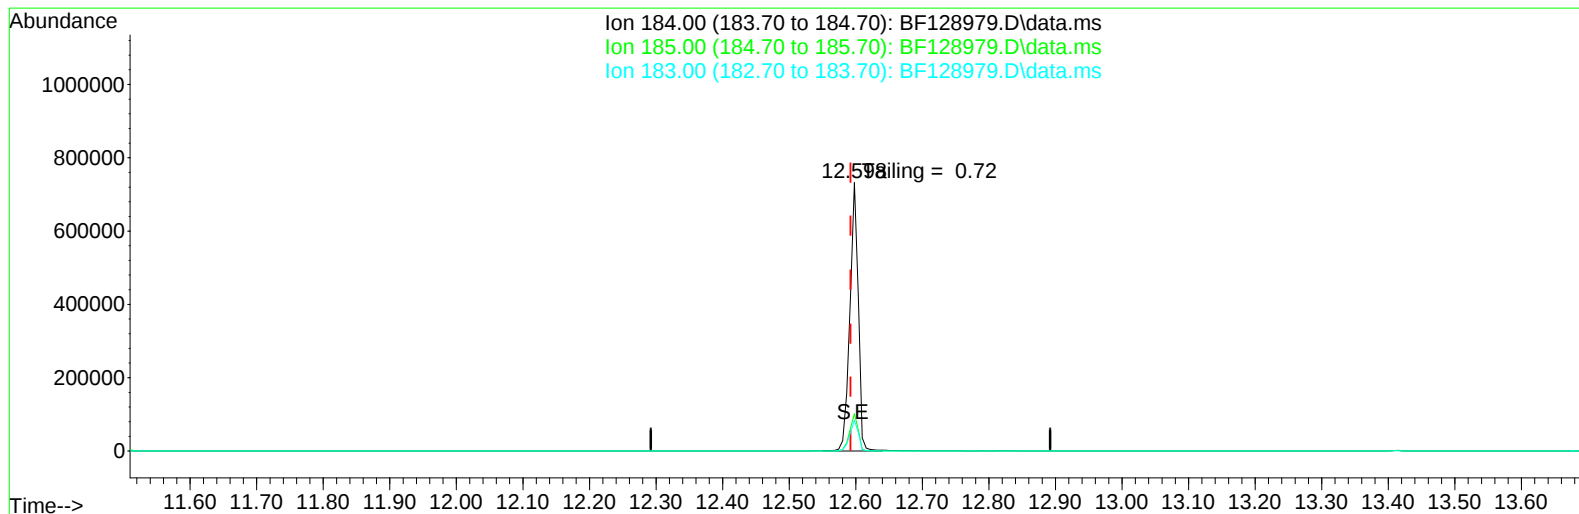

TIC: BF128979.D\data.ms

(77) Benzidine

12.598min (+ 0.006) 0.00 ng

response 649533

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.89
183.00	11.60	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/24/2022	BNA_F	<u>BF128979.D</u>
Compound Name	Response	Retention Time
DDT	322317	13.41
DDD	3720	13.11
DDE	1462	12.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5182	327499	1.58

Instrument :
BNA_F
ClientSampleId :
DFTPP