
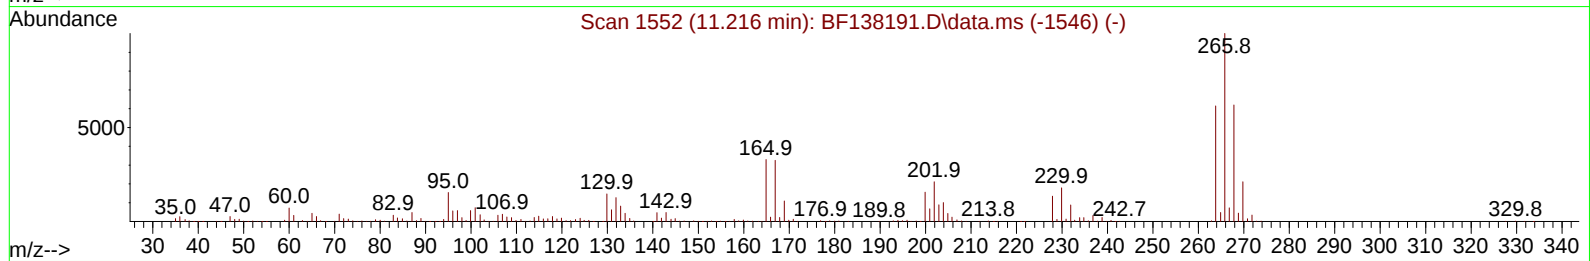
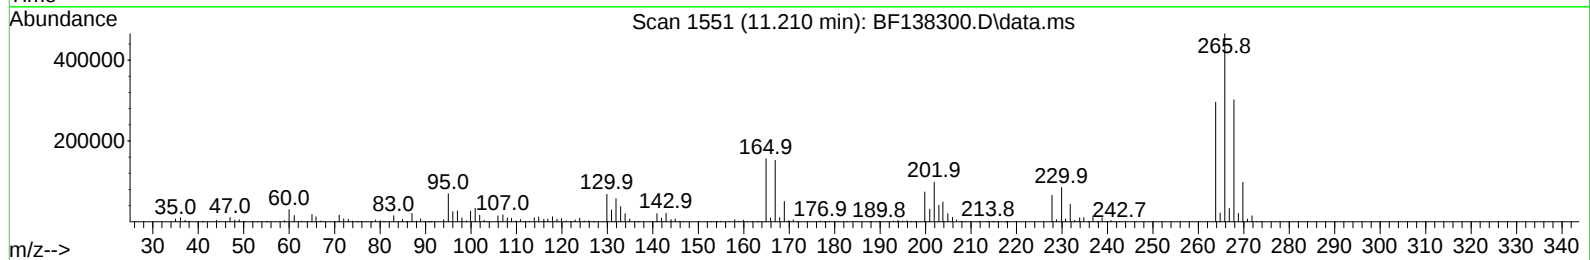


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062424\
Data File : BF138300.D
Acq On : 24 Jun 2024 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 12:08:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

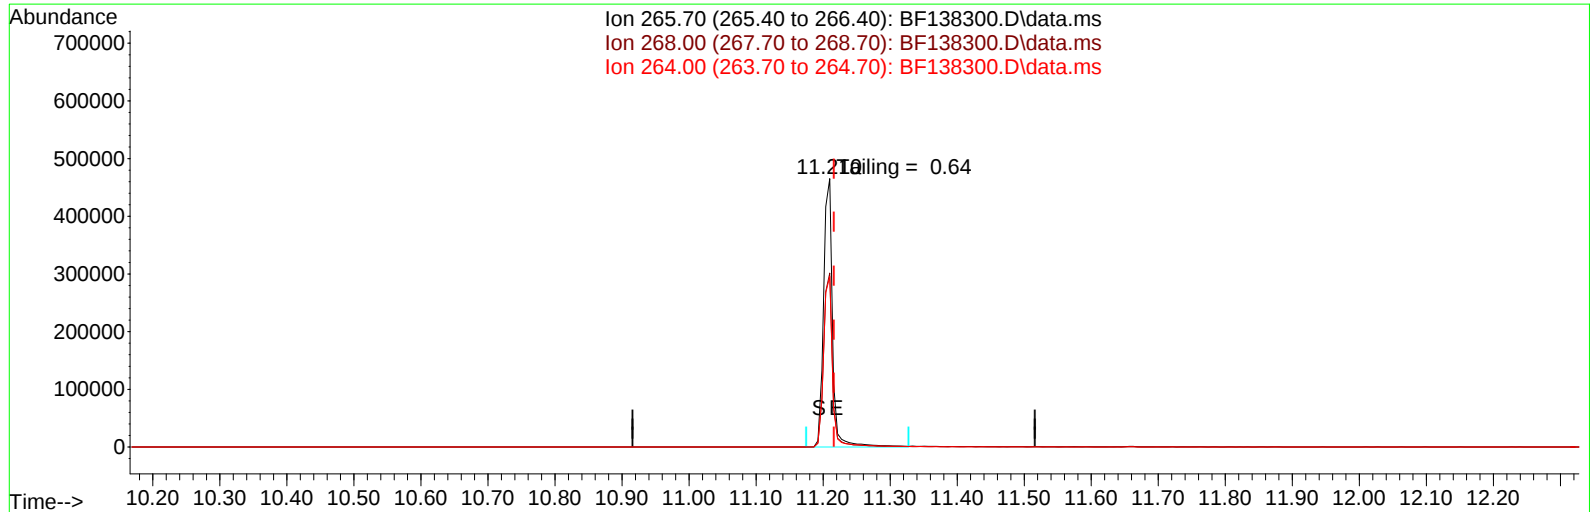

TIC: BF138300.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 147231.33 ng

response 435852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.83
264.00	61.50	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062424\
Data File : BF138300.D
Acq On : 24 Jun 2024 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 12:08:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

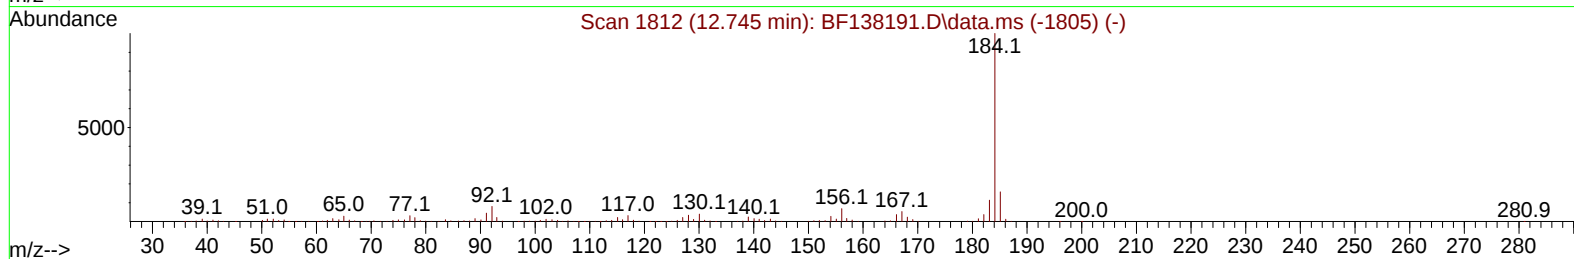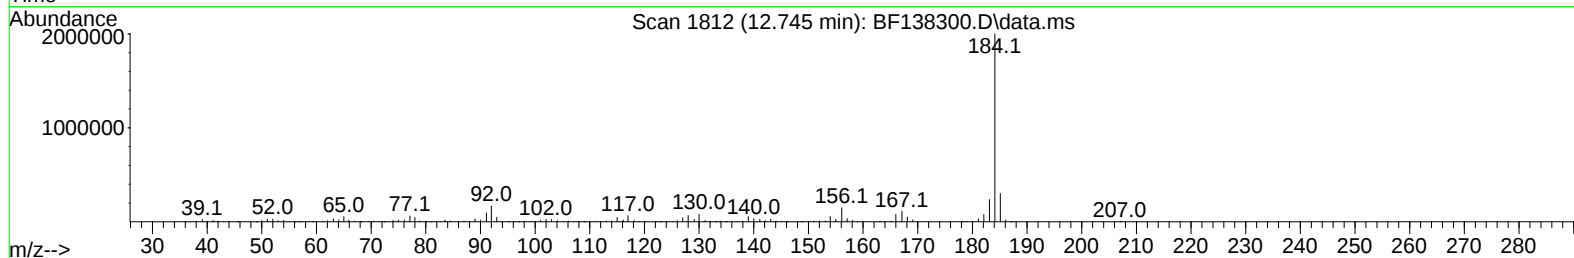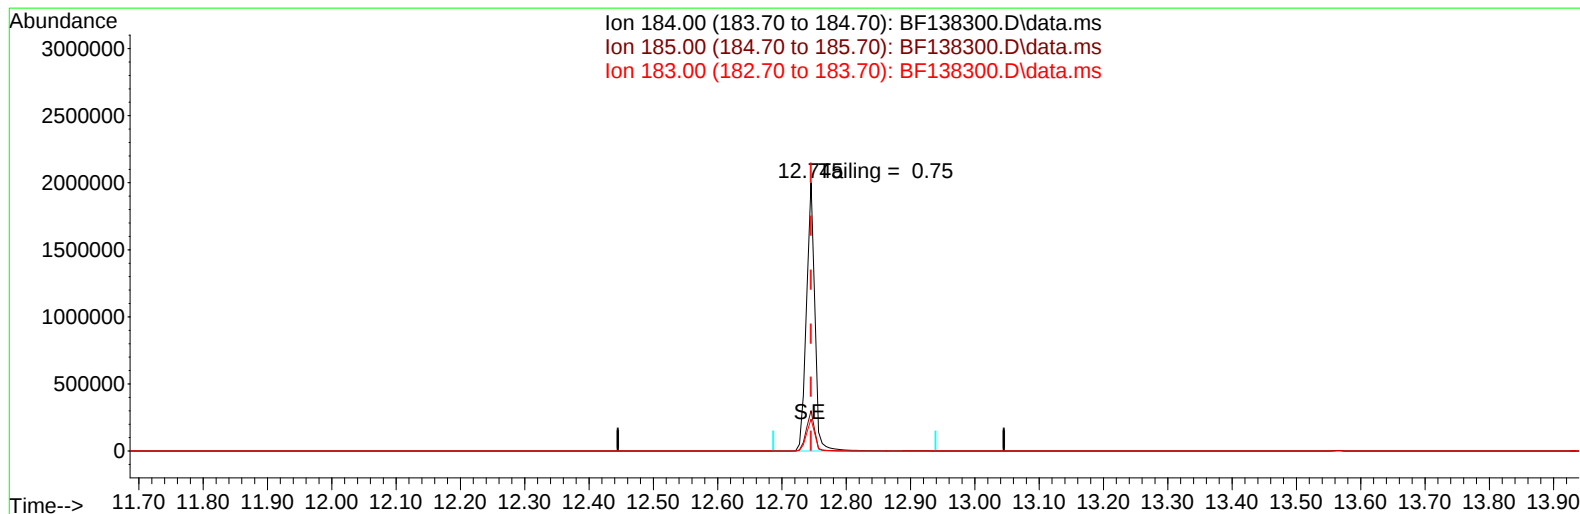

TIC: BF138300.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 2290595.18 ng

response 1828131

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.02
183.00	11.30	11.88
0.00	0.00	0.00