


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062424\
Data File : BF138300.D
Acq On : 24 Jun 2024 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

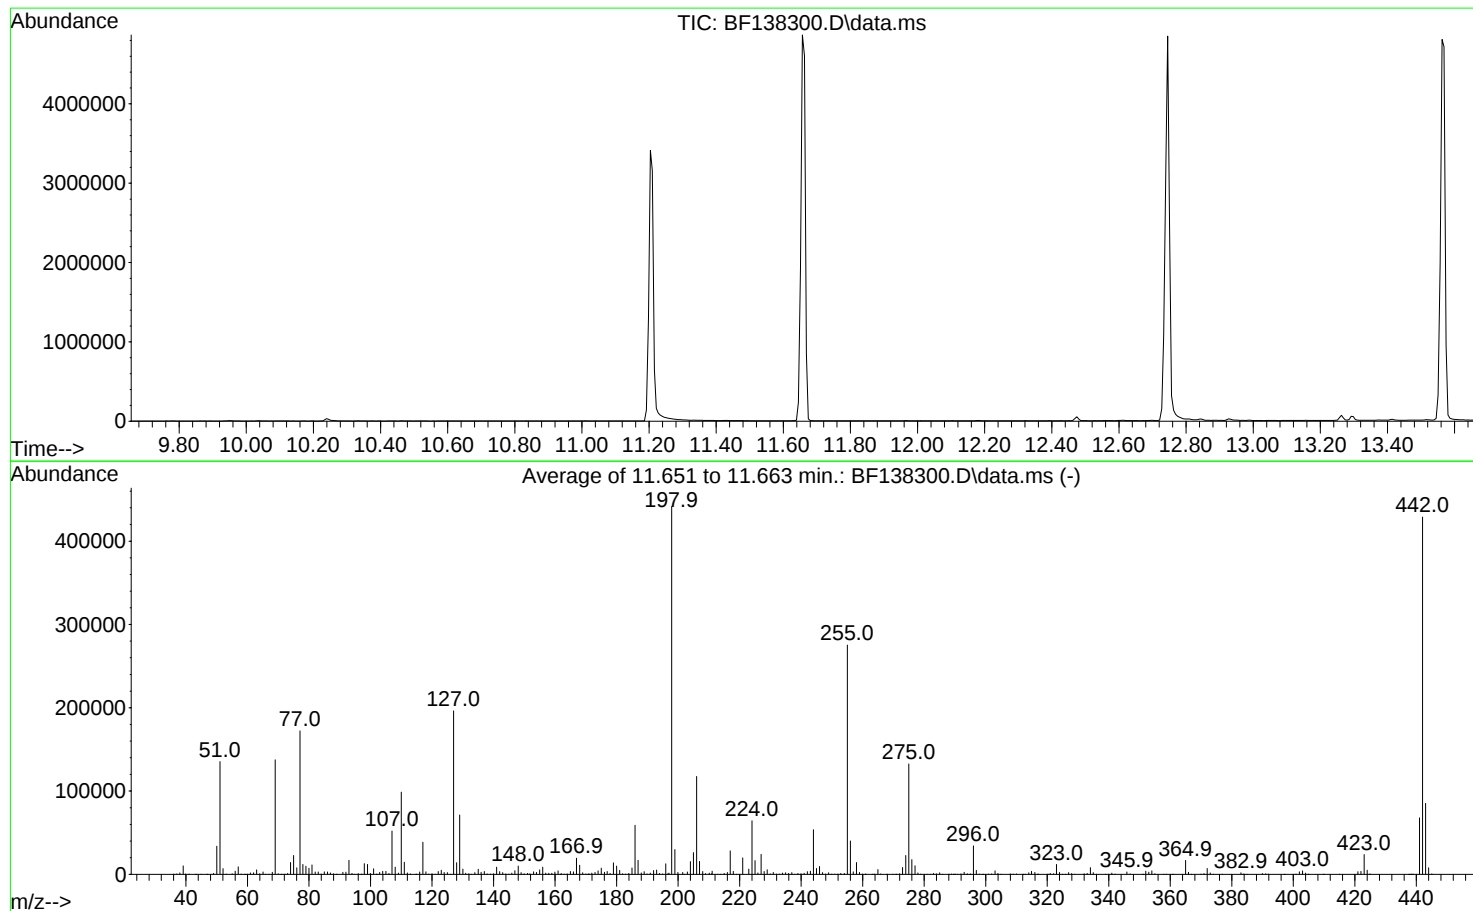




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	135448	PASS
68	69	0.00	2	1.8	2529	PASS
69	198	0.00	100	31.2	137563	PASS
70	69	0.00	2	0.6	827	PASS
127	198	10	80	44.5	196331	PASS
197	198	0.00	2	0.3	1518	PASS
198	198	100	100	100.0	441600	PASS
199	198	5	9	6.8	29885	PASS
275	198	10	60	30.0	132624	PASS
365	198	1	100	3.8	16642	PASS
441	198	0.01	100	15.4	67805	PASS
442	442	50	100	100.0	428872	PASS
443	442	15	24	19.9	85352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062424\
Data File : BF138300.D
Acq On : 24 Jun 2024 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 24 12:08:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

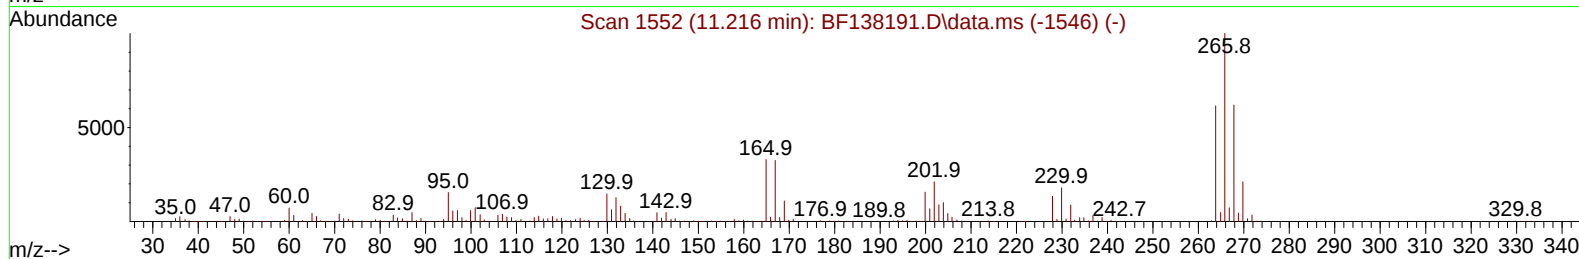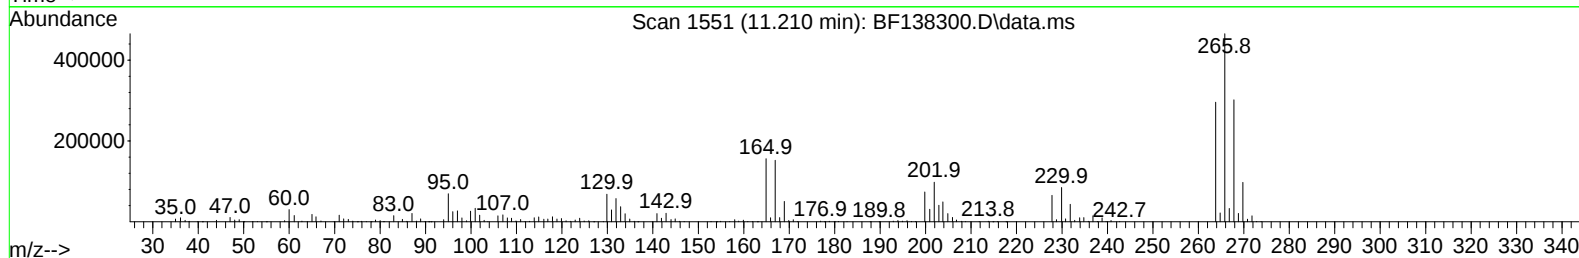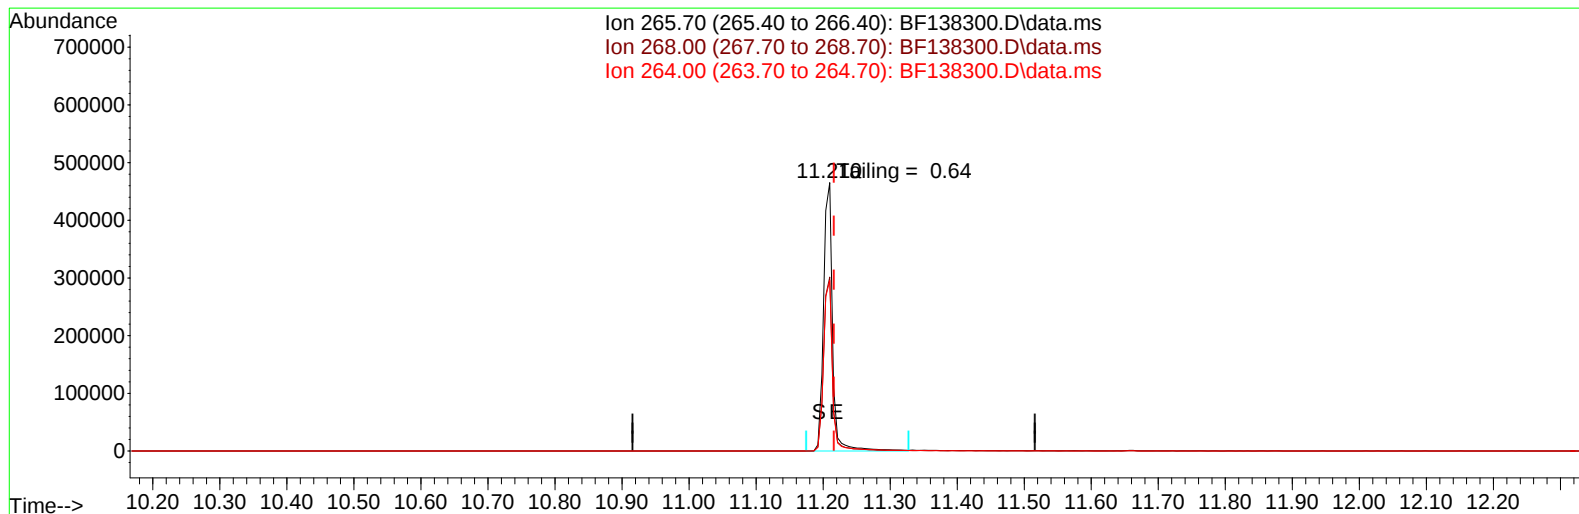

TIC: BF138300.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 147231.33 ng




response 435852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.83
264.00	61.50	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062424\
Data File : BF138300.D
Acq On : 24 Jun 2024 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 24 12:08:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

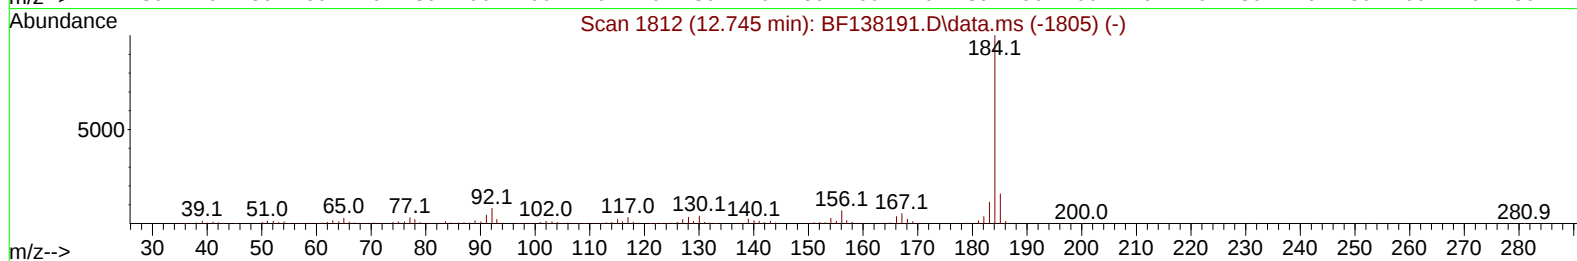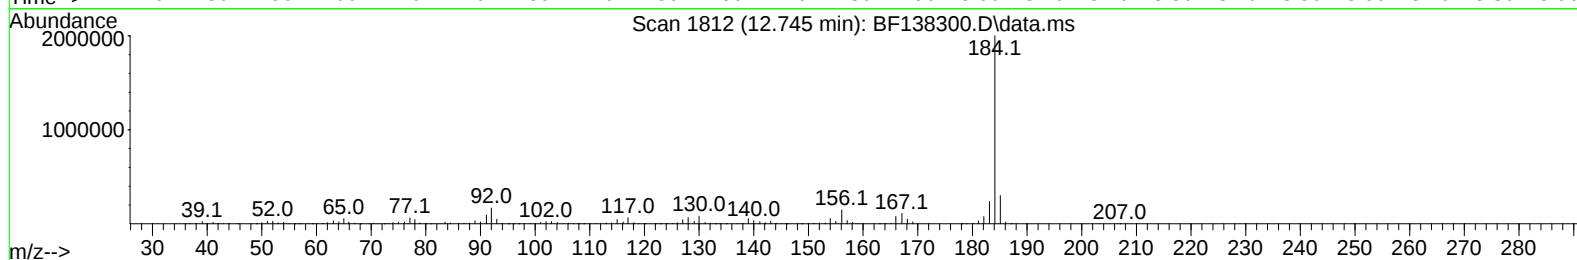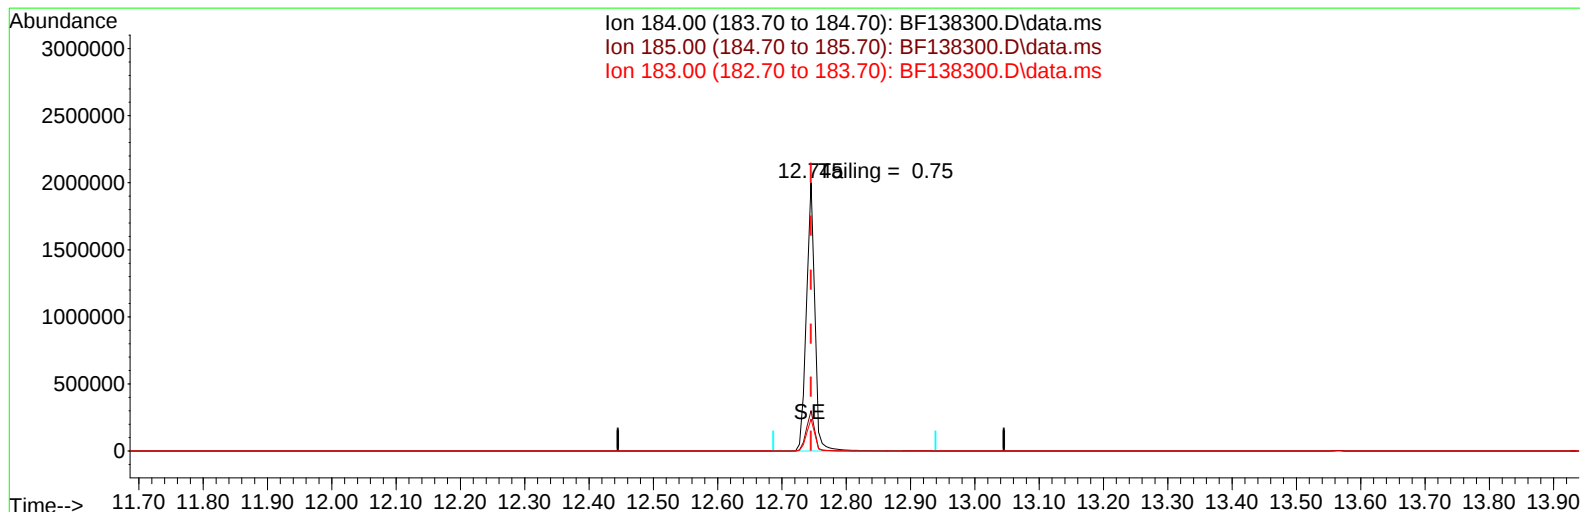

TIC: BF138300.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 2290595.18 ng

response 1828131

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.02
183.00	11.30	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/24/2024	BNA_F	<u>BF138300.D</u>
Compound Name	Response	Retention Time
DDT	935544	13.569
DDD	18988	13.263
DDE	4653	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23641	959185	2.46

Instrument :
BNA_F
ClientSampleId :
DFTPP