


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062425\
Data File : BF142810.D
Acq On : 24 Jun 2025 09:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

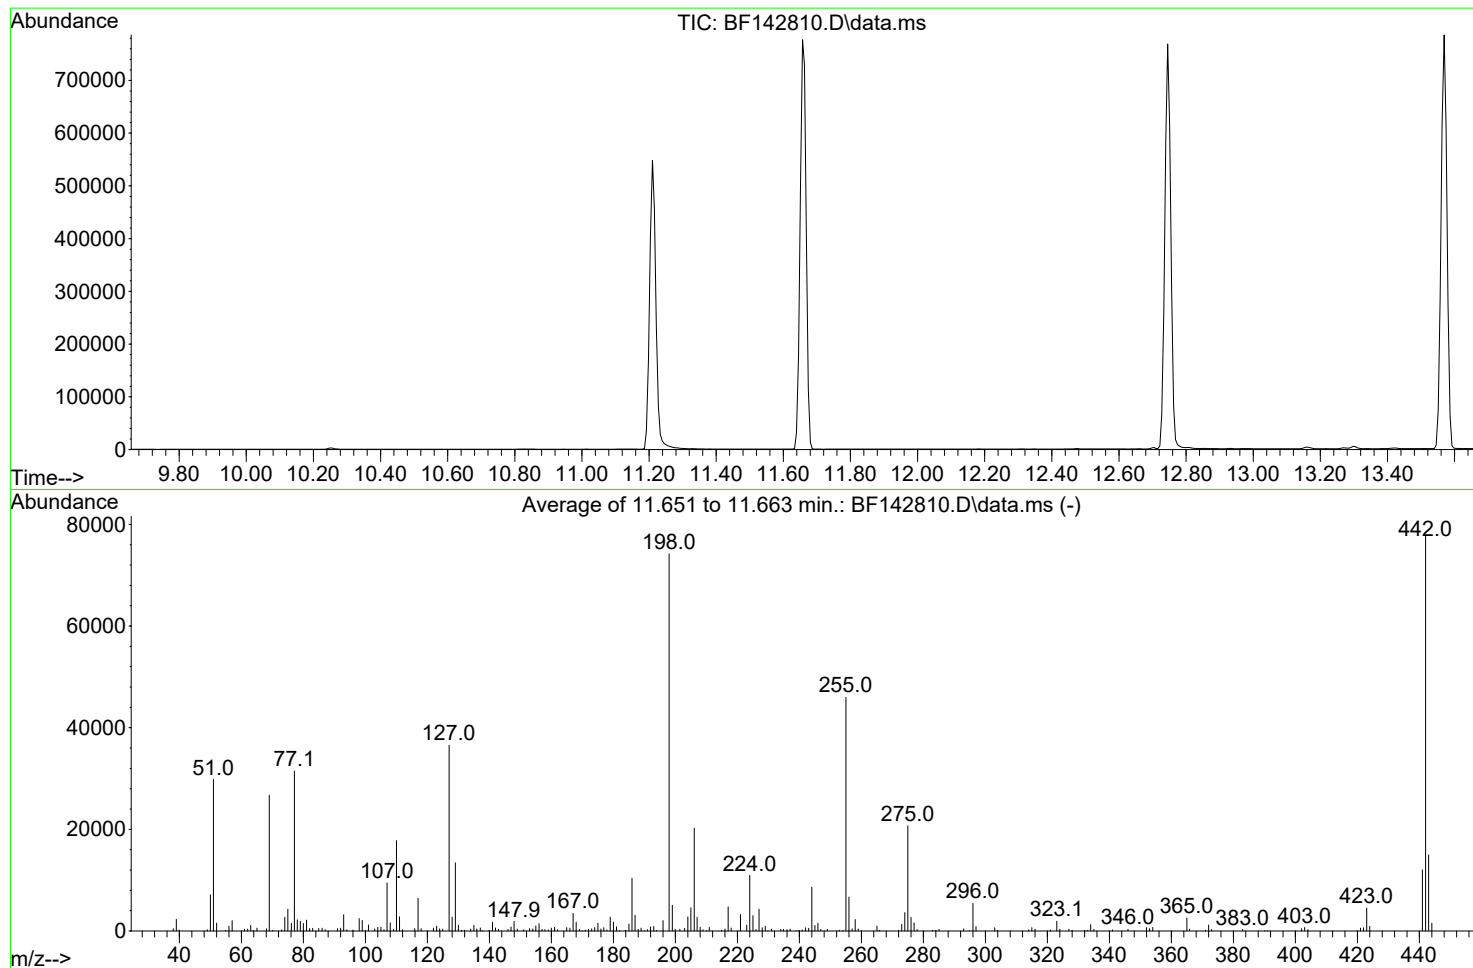

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	459	PASS
69	69	100	100	100.0	26725	PASS
70	69	0.00	2	0.4	109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74195	PASS
199	198	5	9	6.8	5079	PASS
365	198	1	100	3.5	2567	PASS
441	443	0.01	150	80.4	12014	PASS
442	442	100	100	100.0	77685	PASS
443	442	15	24	19.2	14940	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/24/2025	BNA_F	<u>BF142810.D</u>
Compound Name	Response	Retention Time
DDT	200766	13.569
DDD	2580	13.298
DDE	274	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2854	203620	1.40

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062425\
Data File : BF142810.D
Acq On : 24 Jun 2025 09:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 24 12:45:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

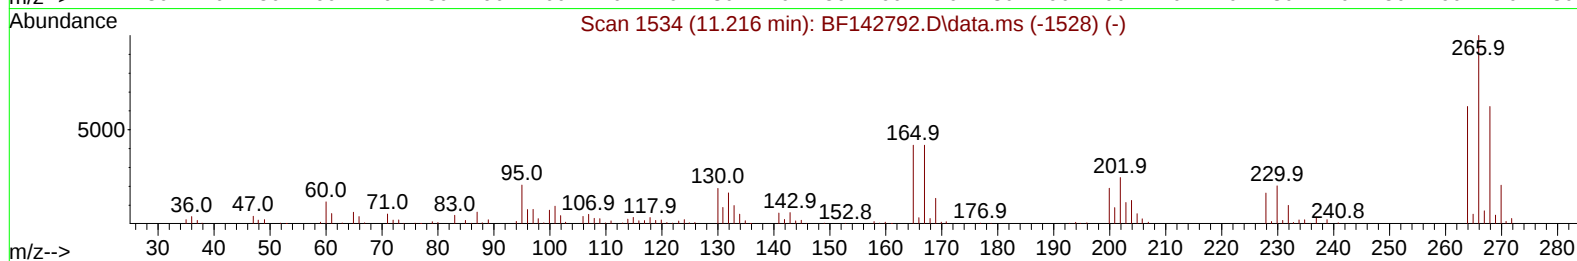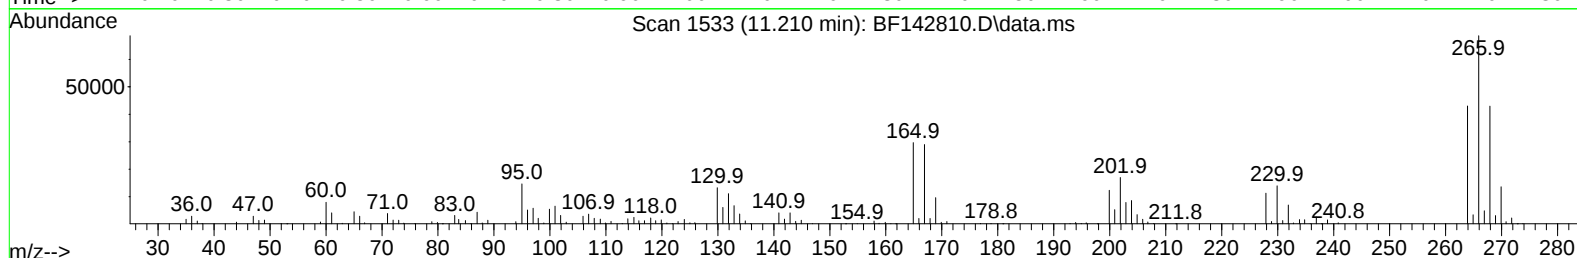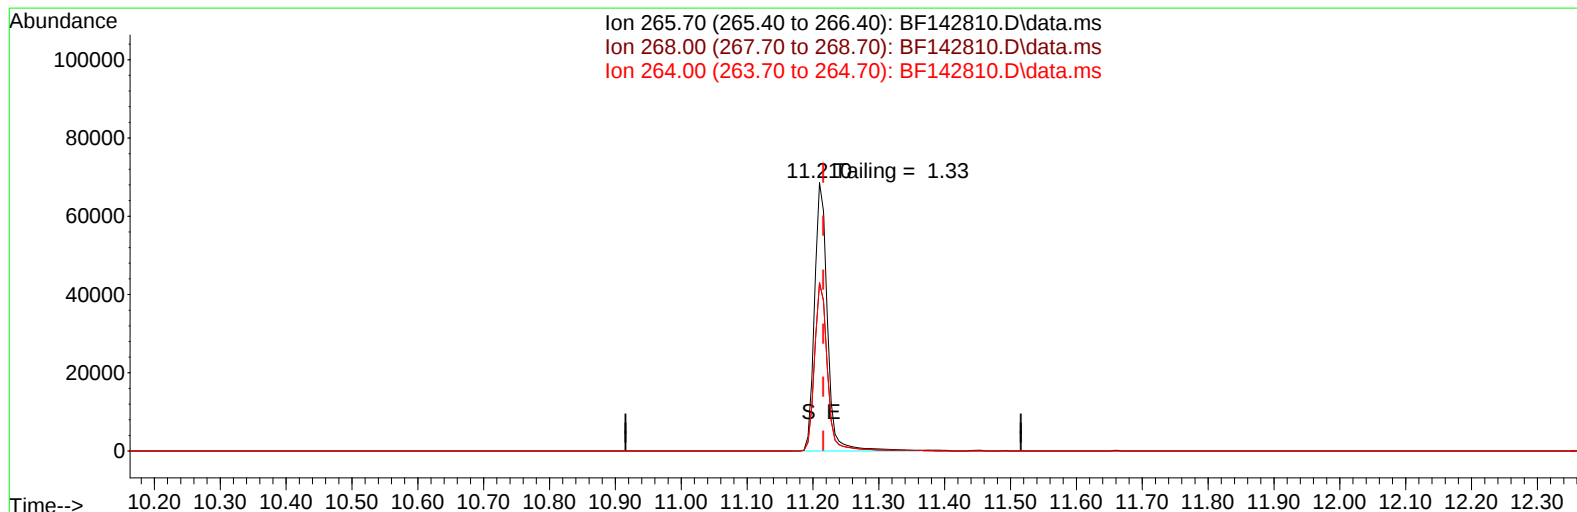

TIC: BF142810.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 37936.00 ng




response 93471

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.64
264.00	62.40	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062425\
Data File : BF142810.D
Acq On : 24 Jun 2025 09:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 24 12:45:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

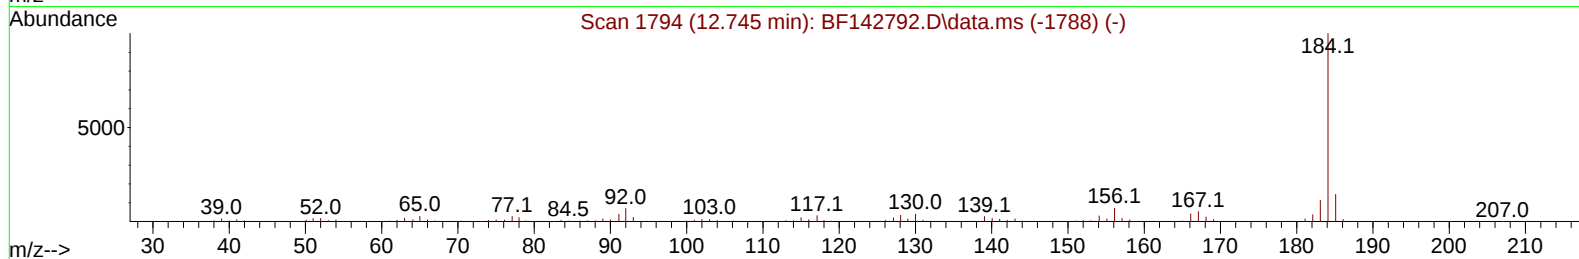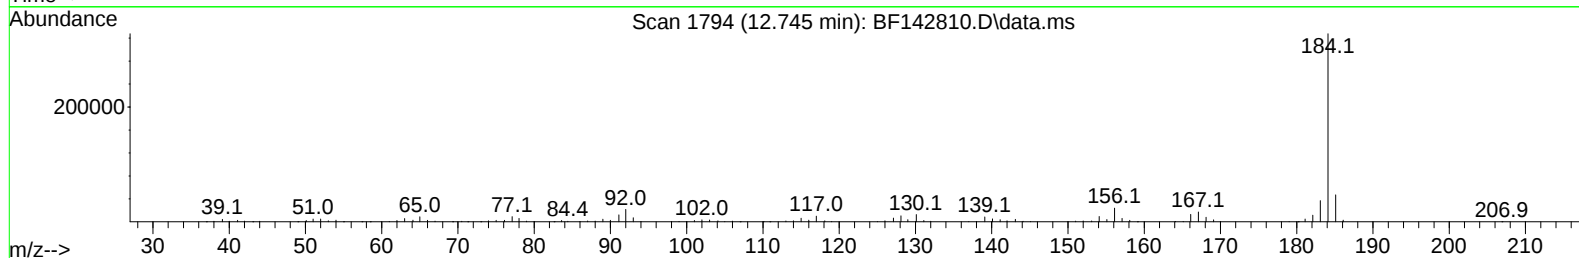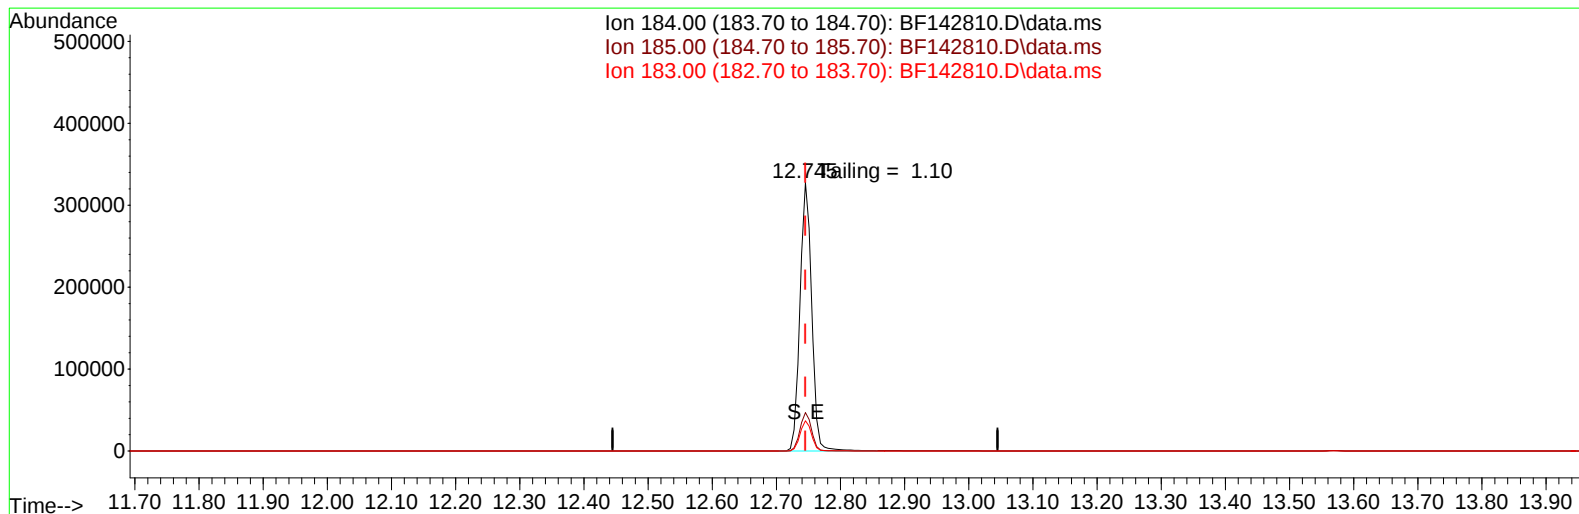

TIC: BF142810.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 419228

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.33
183.00	11.20	11.26
0.00	0.00	0.00