

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080172.D
Acq On : 25 Jun 2015 18:11
Operator : TP/IZ
Sample : PB84215BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84215BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	210	212	218	rBV	110363	127748	9.23%	1.452%
2	5.899	244	246	249	rBV	807583	831223	60.09%	9.451%
3	6.893	331	333	336	rBV	822619	813932	58.84%	9.254%
4	7.064	345	348	350	rBV	816043	888319	64.22%	10.100%
5	7.293	366	368	371	rVB	222043	189970	13.73%	2.160%
6	7.453	380	382	385	rBV	891826	715368	51.71%	8.134%
7	7.853	415	417	419	rBV	640078	552814	39.96%	6.285%
8	8.585	479	481	484	rVB	312142	259973	18.79%	2.956%
9	9.659	573	575	578	rBV	1174522	1056419	76.37%	12.011%
10	10.356	634	636	639	rVB	348328	297504	21.51%	3.383%
11	11.145	703	705	708	rBV2	505199	658578	47.61%	7.488%
12	11.865	765	768	770	rBV	379163	327511	23.68%	3.724%
13	13.557	913	916	918	rBV	1423775	1383340	100.00%	15.729%
14	14.837	1025	1028	1030	rBV	262844	350226	25.32%	3.982%
15	16.711	1189	1192	1198	rBV	206625	342170	24.74%	3.890%


Sum of corrected areas: 8795095

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080172.D
Acq On : 25 Jun 2015 18:11
Operator : TP/IZ
Sample : PB84215BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
PB84215BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

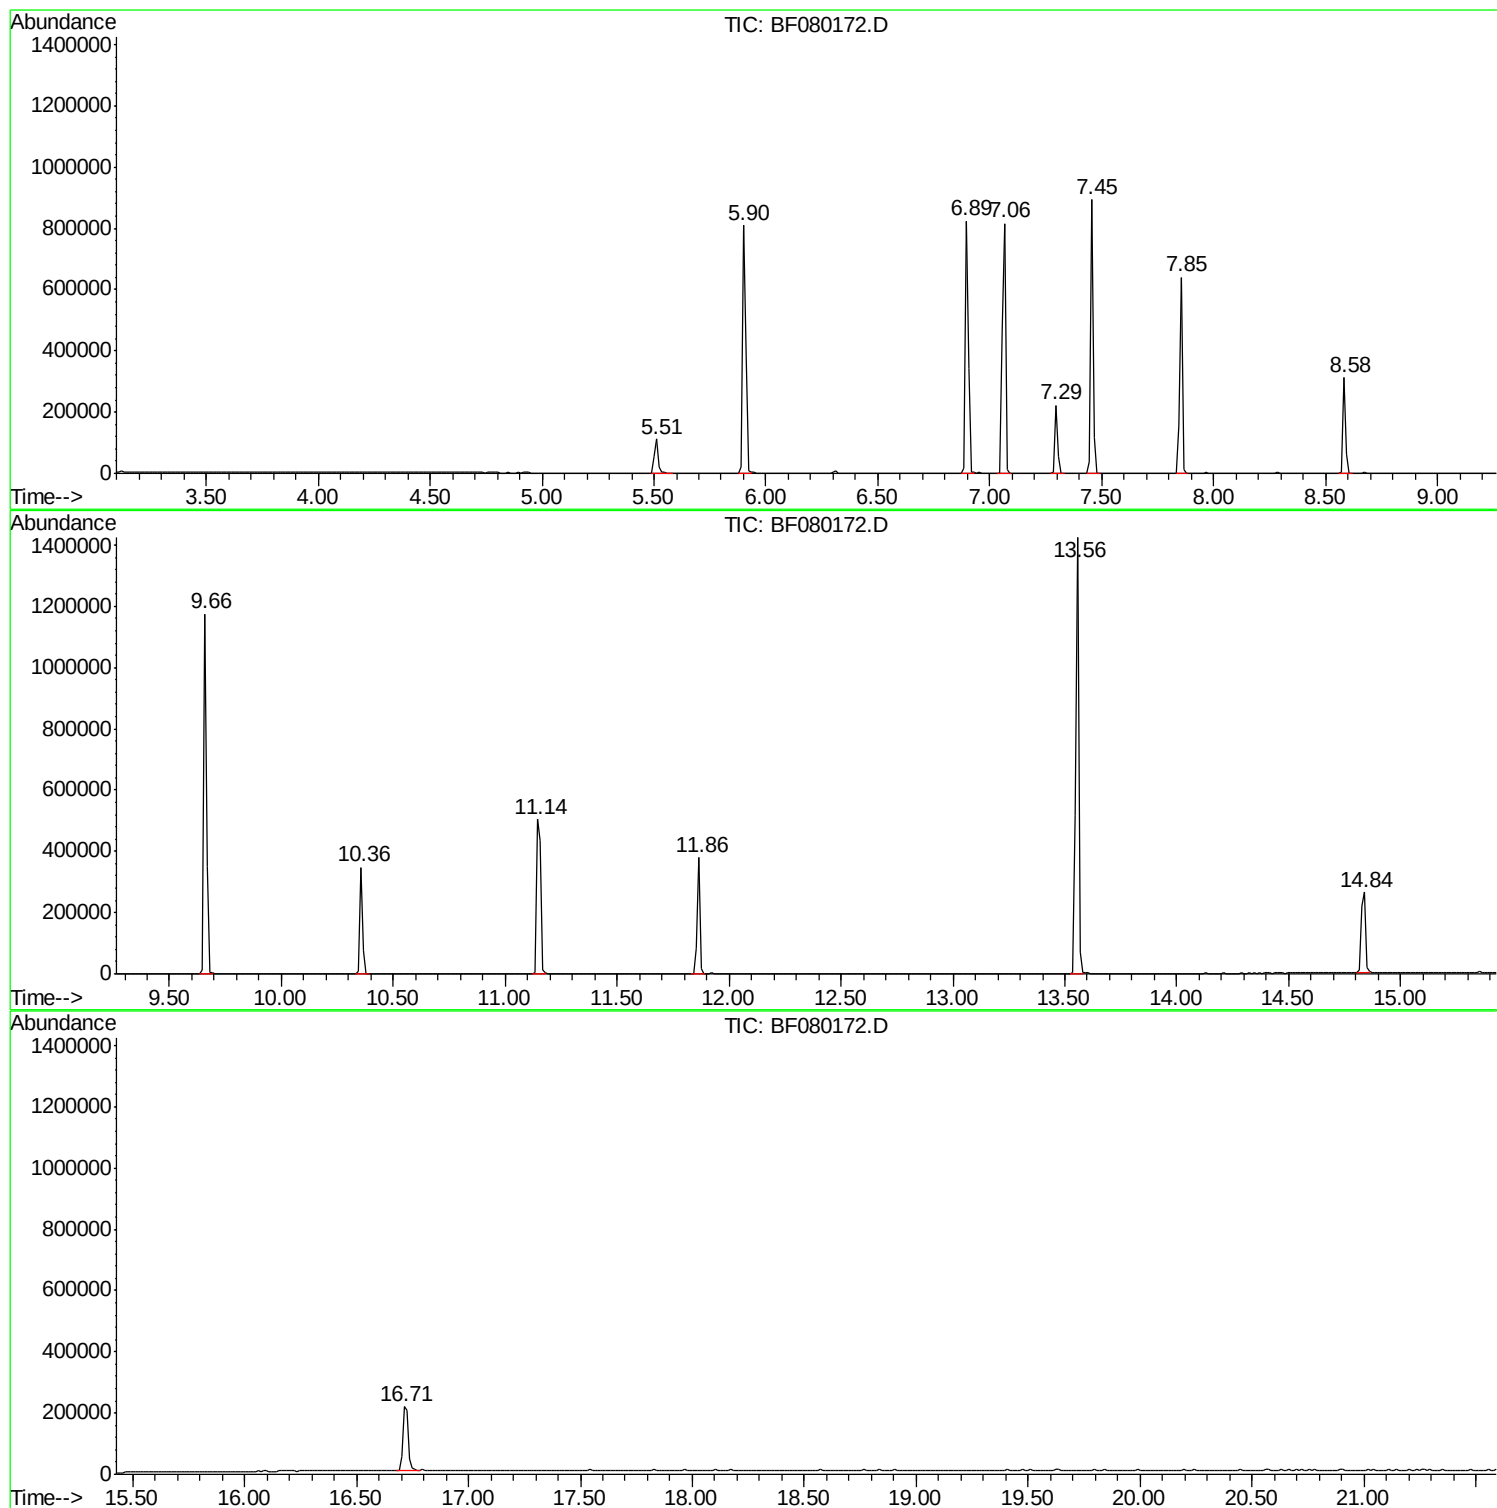

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080172.D
Acq On : 25 Jun 2015 18:11
Operator : TP/IZ
Sample : PB84215BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84215BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.51	13.45 ng	127748	1,4-Dichlorobenzene-d4	7.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
3		5-Oxohexanenitrile	111	C6H9NO	010412-98-3	9
4		1,3-Dioxolane-2-methanol, 2,4-di...	132	C6H12O3	053951-43-2	9
5		4-Hydroxy-3-hexanone	116	C6H12O2	004984-85-4	9

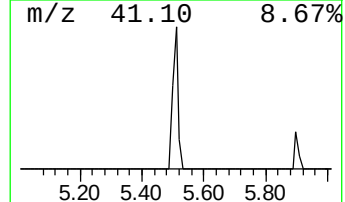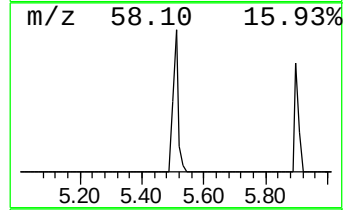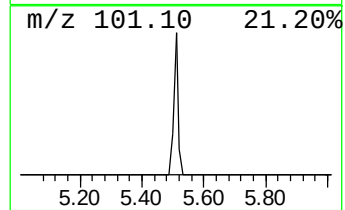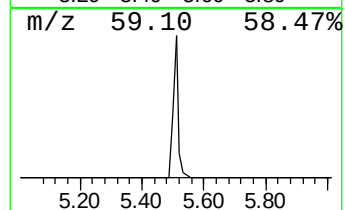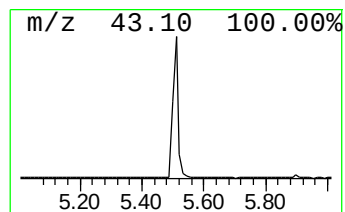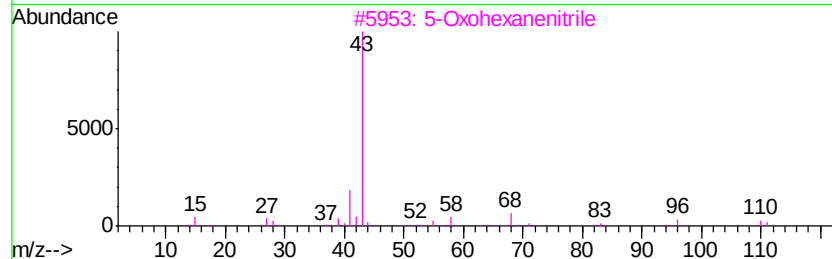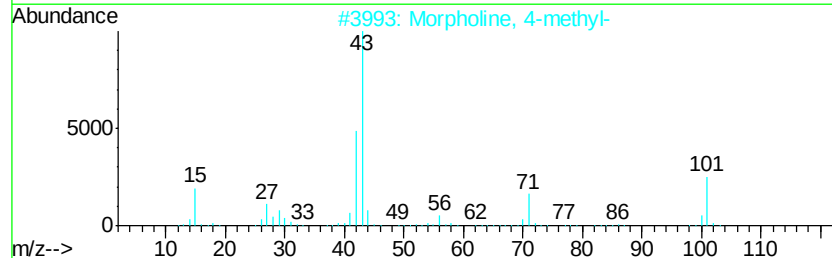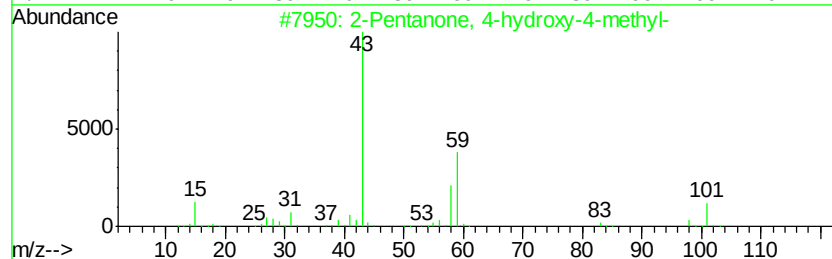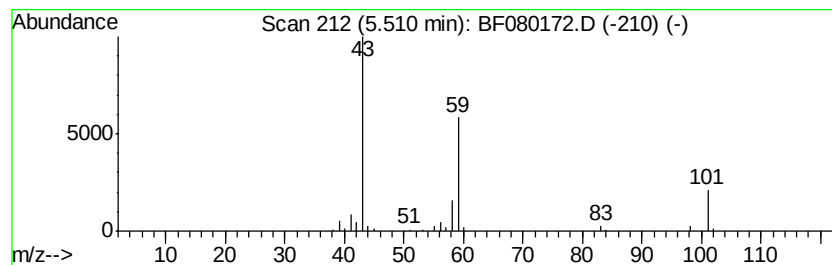

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080172.D
Acq On : 25 Jun 2015 18:11
Operator : TP/IZ
Sample : PB84215BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84215BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.06 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.06	93.52 ng	888319	1,4-Dichlorobenzene-d4	7.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

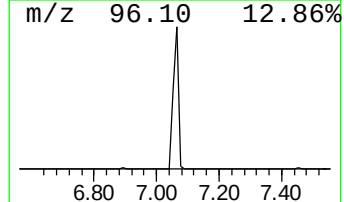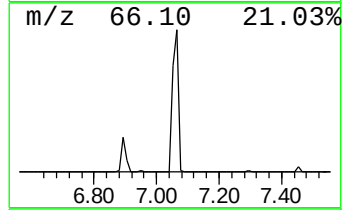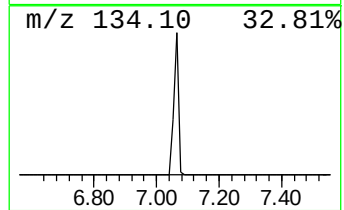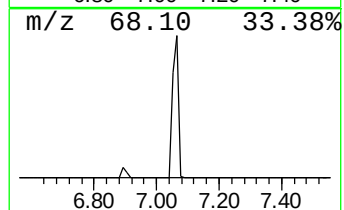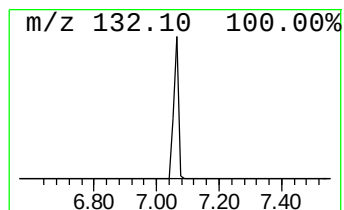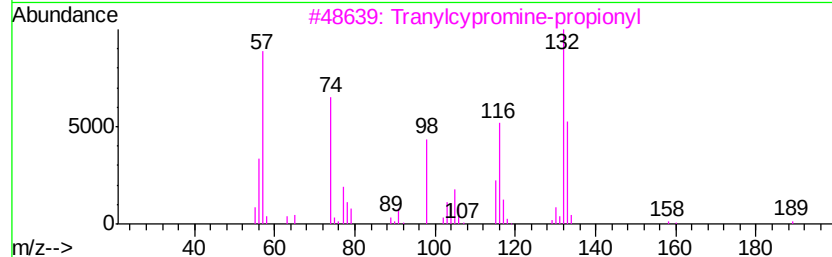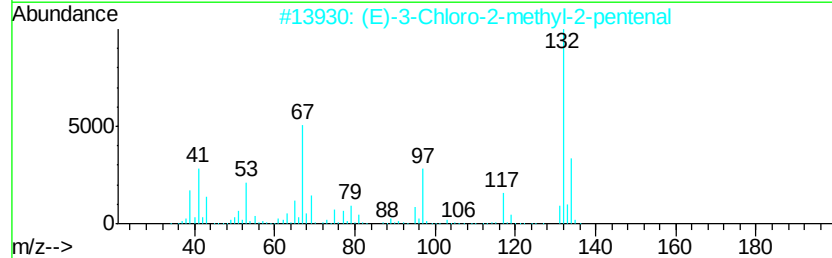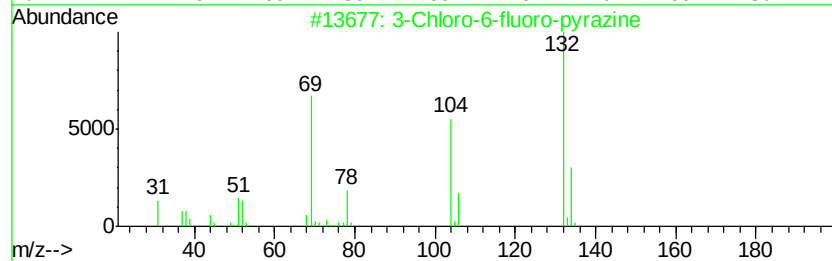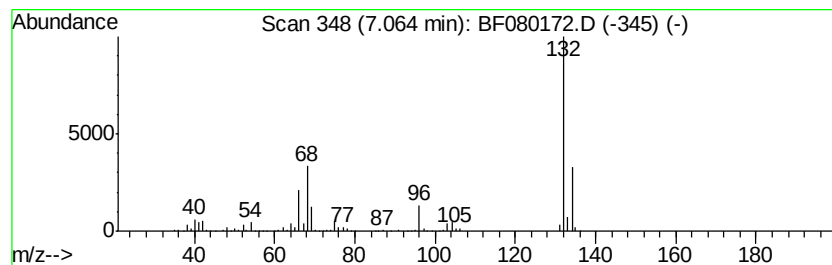

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080172.D
Acq On : 25 Jun 2015 18:11
Operator : TP/IZ
Sample : PB84215BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84215BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.51	13.4	ng	127748	1	7.29	189970	20.0
unknown7.06	7.06	93.5	ng	888319	1	7.29	189970	20.0