

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
 Data File : BF080183.D
 Acq On : 26 Jun 2015 00:55
 Operator : TP/IZ
 Sample : G2699-01RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LAR9819RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	209	211	214	rBV	248722	303050	21.46%	2.596%
2	5.898	244	246	249	rBV	1007789	925093	65.52%	7.925%
3	6.299	279	281	284	rBV	21457	24826	1.76%	0.213%
4	6.527	300	301	305	rBV	15198	17275	1.22%	0.148%
5	6.893	331	333	336	rBV	781596	916068	64.88%	7.848%
6	7.064	345	348	350	rBV	947314	998721	70.73%	8.556%
7	7.293	366	368	370	rVB	199905	171894	12.17%	1.473%
8	7.453	380	382	384	rVB	970139	775319	54.91%	6.642%
9	7.853	415	417	419	rBV	749616	624120	44.20%	5.347%
10	8.344	458	460	462	rVB	17914	15852	1.12%	0.136%
11	8.584	479	481	485	rVB	285155	261005	18.49%	2.236%
12	8.916	508	510	511	rBV	130938	99113	7.02%	0.849%
13	8.939	511	512	516	rVB	21533	17553	1.24%	0.150%
14	9.007	516	518	519	rBV	19453	21046	1.49%	0.180%
15	9.042	519	521	523	rVB	71909	74990	5.31%	0.642%
16	9.247	536	539	542	rVB	38397	43729	3.10%	0.375%
17	9.305	542	544	545	rBV	27566	27231	1.93%	0.233%
18	9.339	545	547	549	rBV	19308	23564	1.67%	0.202%
19	9.442	552	556	557	rBV	31974	50840	3.60%	0.436%
20	9.533	561	564	569	rVB2	12310	26630	1.89%	0.228%
21	9.659	573	575	577	rVB	1229718	1149698	81.43%	9.849%
22	10.047	607	609	612	rBV	114799	95953	6.80%	0.822%
23	10.356	633	636	638	rBV2	342250	313902	22.23%	2.689%
24	11.156	703	706	708	rBV2	629581	828418	58.67%	7.097%
25	11.248	711	714	717	rBV2	11372	14144	1.00%	0.121%
26	11.373	724	725	729	rVB	15798	15357	1.09%	0.132%
27	11.865	765	768	769	rBV	313478	319414	22.62%	2.736%
28	11.888	769	770	772	rVB	47928	34839	2.47%	0.298%
29	12.059	783	785	790	rBV	8404	17402	1.23%	0.149%
30	13.133	877	879	880	rBV	76129	95853	6.79%	0.821%
31	13.305	892	894	896	rBV2	13925	20573	1.46%	0.176%
32	13.385	896	901	903	rBV	82205	118882	8.42%	1.018%
33	13.522	911	913	916	rBV	1183377	1411931	100.00%	12.095%
34	13.739	928	932	936	rBV2	13213	27526	1.95%	0.236%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080183.D
Acq On : 26 Jun 2015 00:55
Operator : TP/IZ
Sample : G2699-01RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAR9819RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.562	1000	1004	1012	rBV2	85469	165037	11.69%	1.414%
36	14.734	1017	1019	1020	rBV	14418	21958	1.56%	0.188%
37	14.768	1020	1022	1024	rBV2	339864	423298	29.98%	3.626%
38	14.905	1032	1034	1037	rVB	17641	20451	1.45%	0.175%
39	15.374	1072	1075	1078	rBV2	44275	83783	5.93%	0.718%
40	15.568	1090	1092	1095	rBV2	12309	16260	1.15%	0.139%
41	16.082	1134	1137	1142	rBV	80626	179586	12.72%	1.538%
42	16.220	1147	1149	1153	rVB	17072	24318	1.72%	0.208%
43	16.460	1167	1170	1174	rVB	54945	81006	5.74%	0.694%
44	16.540	1174	1177	1181	rVV	66228	113491	8.04%	0.972%
45	16.620	1181	1184	1186	rVV	221121	359453	25.46%	3.079%
46	16.654	1186	1187	1195	rVV	33310	47548	3.37%	0.407%
47	17.282	1240	1242	1247	rVB5	8515	26246	1.86%	0.225%
48	17.511	1260	1262	1270	rVB7	7714	26768	1.90%	0.229%
49	18.071	1308	1311	1315	rVB3	7232	19106	1.35%	0.164%
50	18.437	1339	1343	1348	rVB2	37851	89075	6.31%	0.763%
51	18.985	1387	1391	1398	rBV	32271	77370	5.48%	0.663%
52	19.283	1414	1417	1421	rVB	6652	16691	1.18%	0.143%


Sum of corrected areas: 11673256

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080183.D
Acq On : 26 Jun 2015 00:55
Operator : TP/IZ
Sample : G2699-01RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAR9819RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

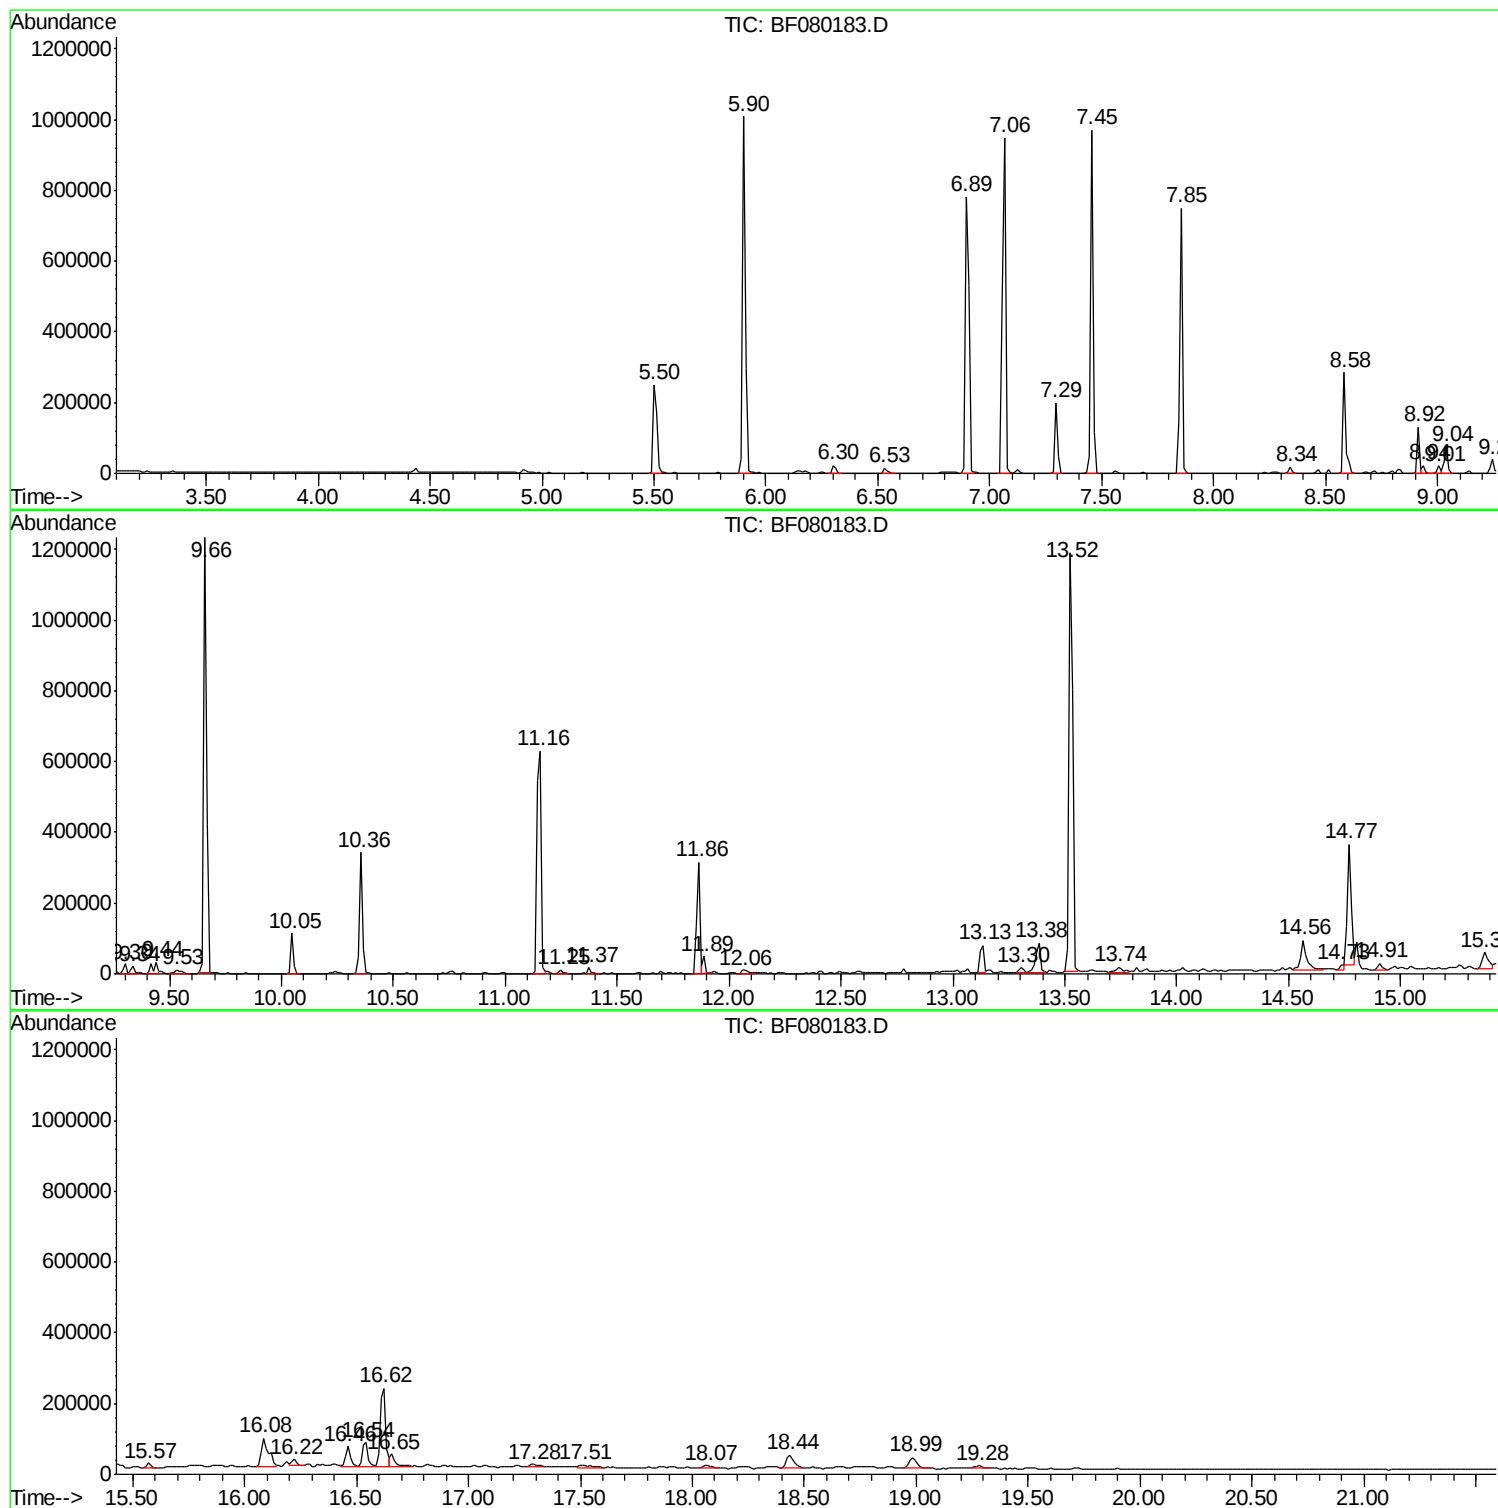

DbaaaPathh::ZZ\NRPBMM1BNAFNDAAAB000255\
 DbaaaFile::BB000083DD
 Aeqq00n ::206Jun2005 000555
 Opeaaor ::TPPIZ
 Sample ::G0009900RE
 Misc ::
 AASSVaal ::223 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 LAR9819RE

QqaabMebbdd::ZZ\NRPBMM1BNAFMEH00S8200BB006775MM
 QqaabTitle ::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICCLibbaay ::CC\DAABASSEN0\$002LL
 TICIntegratíonPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
