


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062515\
Data File : BF080158.D
Acq On : 25 Jun 2015 10:48
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 23 00:53:56 2015

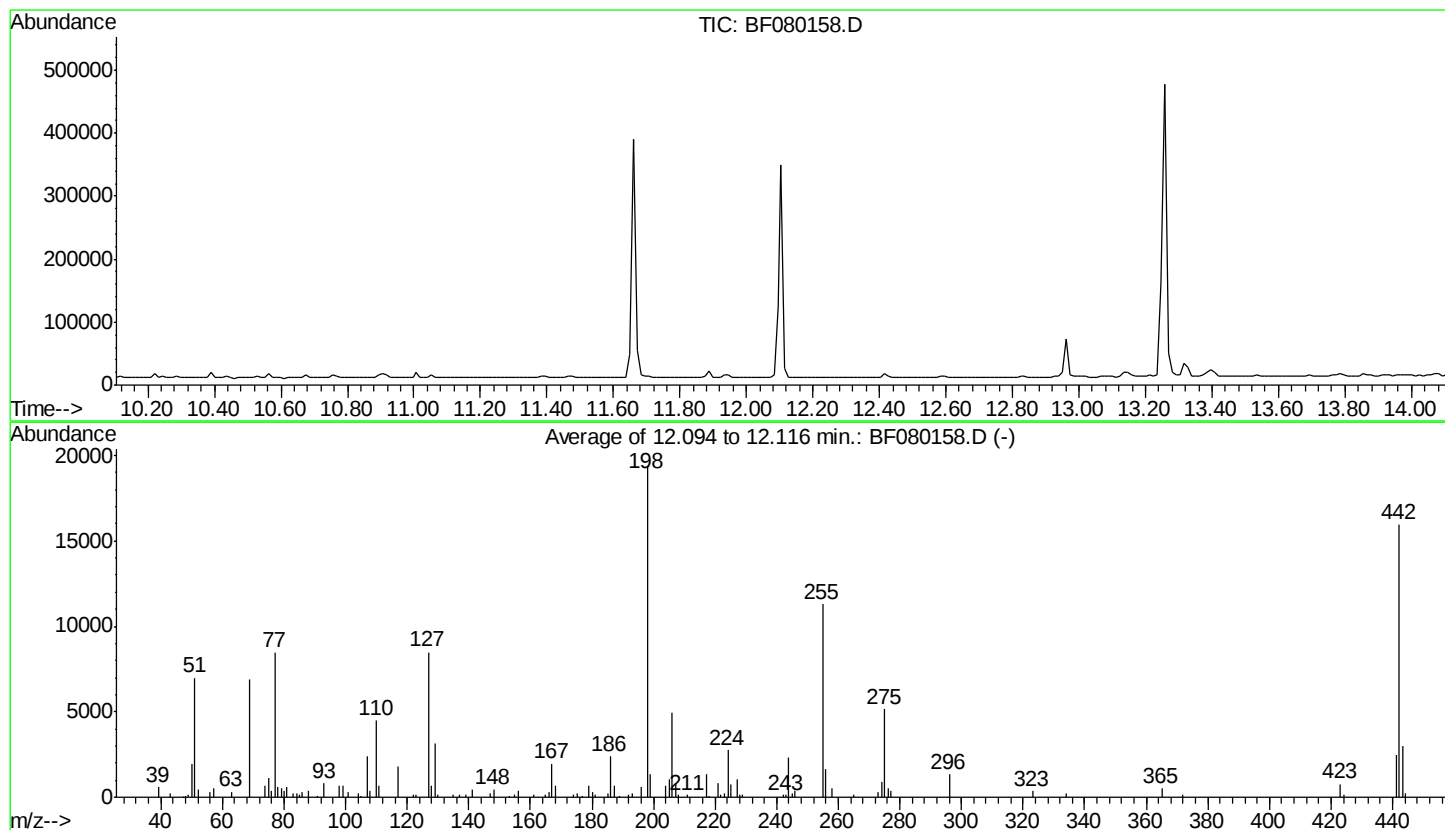

AutoFind: Scans 788, 789, 790; Background Corrected with Scan 785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	7001	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.7	6930	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.8	8493	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19405	PASS
199	198	5	9	7.1	1372	PASS
275	198	10	60	26.6	5159	PASS
365	198	1	100	2.6	501	PASS
441	442	0.01	24	15.6	2494	PASS
442	198	50	100	82.2	15946	PASS
443	442	15	24	18.9	3020	PASS