

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062516\
 Data File : BF088374.D
 Acq On : 25 Jun 2016 13:51
 Operator : UM/SJ
 Sample : H3602-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 Q8-B4(0-2)C

Quant Time: Jun 26 02:37:18 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 14:55:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.56	152	80805	20.00	ng	-0.05
21) Naphthalene-d8	7.85	136	316355	20.00	ng	-0.05
38) Acenaphthene-d10	9.60	164	131463	20.00	ng	-0.05
63) Phenanthrene-d10	11.08	188	146689	20.00	ng	-0.03
75) Chrysene-d12	13.71	240	123194	20.00	ng	-0.03
86) Perylene-d12	15.05	264	143085	20.00	ng	-0.06

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.15	112	691482	146.29	ng	-0.02
7) Phenol-d6	6.24	99	882144	154.00	ng	-0.02
23) Nitrobenzene-d5	7.14	82	556035	102.64	ng	-0.03
41) 2,4,6-Tribromophenol	10.40	330	137831	99.29	ng	-0.03
44) 2-Fluorobiphenyl	8.92	172	688275	82.05	ng	-0.05
78) Terphenyl-d14	12.66	244	469074	86.64	ng	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
31) Naphthalene	7.87	128	38156	2.44	ng	100
37) 2-Methylnaphthalene	8.56	142	31702	3.07	ng	# 93
45) 1,1'-Biphenyl	9.03	154	520919	54.04	ng	98
48) Acenaphthylene	9.46	152	96593	7.14	ng	# 89
49) Dimethylphthalate	9.35	163	125293	13.16	ng	98
51) Acenaphthene	9.67	154	2765396	327.60	ng	98
54) Dibenzofuran	9.83	168	2502377	215.25	ng	# 83
57) Fluorene	10.17	166	2339238	328.15	ng	97
70) Phenanthrene	11.15	178	5541056	719.86	ng	98
71) Anthracene	11.19	178	1856724m	239.13	ng	
72) Carbazole	11.32	167	756640	104.14	ng	100
74) Fluoranthene	12.32	202	3983790	490.42	ng	99
77) Pvrene	12.54	202	3125884m	341.93	ng	
80) Benzo(a)anthracene	13.70	228	984746m	140.27	ng	
82) Chrysene	13.74	228	710896m	107.64	ng	
85) Indeno(1,2,3-cd)pyrene	16.30	276	71791	11.70	ng	# 100
87) Benzo(b)fluoranthene	14.70	252	502295m	50.37	ng	
88) Benzo(k)fluoranthene	14.71	252	172632m	22.95	ng	
89) Benzo(a)pvrene	15.01	252	274847m	34.06	ng	
90) Dibenzo(a,h)anthracene	16.30	278	18889	2.52	ng	# 66
91) Benzo(q,h,i)perylene	16.66	276	55889	7.25	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062516\
Data File : BF088374.D
Acq On : 25 Jun 2016 13:51
Operator : UM/SJ
Sample : H3602-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Q8-B4(0-2)C

Quant Time: Jun 26 02:37:18 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration









#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.56 min Scan# 435
Delta R.T. -0.05 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51

Instrument :
BNA_F
ClientSampleId :
Q8-B4(0-2)C




Tot Ion:152 Resp: 80805
Ion Ratio Lower Upper
152 100
150 159.1 123.8 185.6
115 62.5 39.6 59.4#



#5

2-Fluorophenol
Concen: 146.29 ng
RT: 5.15 min Scan# 312
Delta R.T. -0.02 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51

Tgt Ion:112 Resp: 691482
Ion Ratio Lower Upper
112 100
64 51.6 42.2 63.2
63 27.2 21.8 32.8





#7

Phenol-d6

Concen: 154.00 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.02 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C




Tot Ion: 99 Resp: 882144

Ion Ratio Lower Upper

99 100

42 11.5 12.2 18.2#

71 29.9 23.4 35.0



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.85 min Scan# 548

Delta R.T. -0.05 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Tgt Ion: 136 Resp: 316355




Ion Ratio Lower Upper


136 100

137 10.7 9.1 13.7

54 5.3 6.6 10.0#

68 4.6 5.1 7.7#



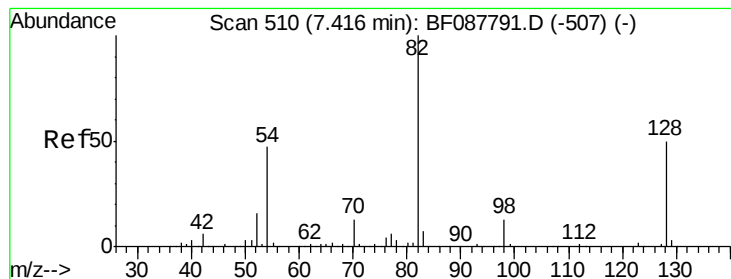

#23

Nitrobenzene-d5

Concen: 102.64 ng

RT: 7.14 min Scan# 486

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion: 82 Resp: 556035

Ion Ratio Lower Upper




82 100

128 49.0 35.9 53.9

54 43.5 40.9 61.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0



#31

Naphthalene

Concen: 2.44 ng

RT: 7.87 min Scan# 550

Delta R.T. -0.05 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:128 Resp: 38156

Ion Ratio Lower Upper



128 100


129 11.9 9.4 14.2

127 13.6 10.9 16.3



Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E









#37
2-Methylnaphthalene
Concen: 3.07 ng
RT: 8.56 min Scan# 610
Delta R.T. -0.05 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51




Instrument :
BNA_F
ClientSampleId :
Q8-B4(0-2)C

Tot Ion:142 Resp: 31702
Ion Ratio Lower Upper
142 100
141 91.8 71.0 106.6
115 38.4 22.6 33.8#



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.60 min Scan# 701
Delta R.T. -0.05 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51

Tgt Ion:164 Resp: 131463
Ion Ratio Lower Upper
164 100
162 104.0 85.4 128.2
160 45.1 39.5 59.3








#41
 2,4,6-Tribromophenol
 Concen: 99.29 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.03 min
 Lab File: BF088374.D
 Acq: 25 Jun 2016 13:51

Instrument :
 BNA_F
 ClientSampleId :
 Q8-B4(0-2)C

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	0.0	0.0#
141	39.4	0.0	0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E





#44
 2-Fluorobiphenyl
 Concen: 82.05 ng
 RT: 8.92 min Scan# 642
 Delta R.T. -0.05 min
 Lab File: BF088374.D
 Acq: 25 Jun 2016 13:51

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	28.6	43.0
170	24.1	19.2	28.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E





#45

1,1'-Biphenyl

Concen: 54.04 ng

RT: 9.03 min Scan# 651

Delta R.T. -0.05 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:154 Resp: 520919

Ion Ratio Lower Upper

154 100

153 40.6 20.6 60.6




76 11.6 0.0 35.1



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BF0



#48

Acenaphthylene

Concen: 7.14 ng

RT: 9.46 min Scan# 689

Delta R.T. -0.05 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:152 Resp: 96593

Ion Ratio Lower Upper

152 100

151 21.4 16.2 24.4



153 23.9 11.0 16.6#




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E









#49
Dimethylphthalate
Concen: 13.16 ng
RT: 9.35 min Scan# 679
Delta R.T. -0.03 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51




Instrument :
BNA_F
ClientSampleId :
Q8-B4(0-2)C


Tot Ion:163 Resp: 125293
Ion Ratio Lower Upper
163 100
194 4.1 2.8 4.2
164 9.8 8.3 12.5



#51
Acenaphthene
Concen: 327.60 ng
RT: 9.67 min Scan# 707
Delta R.T. -0.01 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51

Tgt Ion:154 Resp: 2765396
Ion Ratio Lower Upper
154 100
153 113.5 89.5 134.3
152 54.9 42.7 64.1





#54

Dibenzenofuran

Concen: 215.25 ng

RT: 9.83 min Scan# 721

Delta R.T. -0.02 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:168 Resp: 2502377

Ion Ratio Lower Upper

168 100

139 46.0 26.4 39.6#




169 14.3 10.4 15.6



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E



#57

Fluorene

Concen: 328.15 ng

RT: 10.17 min Scan# 751

Delta R.T. -0.02 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:166 Resp: 2339238

Ion Ratio Lower Upper

166 100

165 99.7 77.8 116.8



167 16.1 11.2 16.8




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E





#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.08 min Scan# 831

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:188 Resp: 146689

Ion Ratio Lower Upper

188 100

94 10.9 9.0 13.6




80 10.9 10.0 15.0



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



#70

Phenanthrene

Concen: 719.86 ng

RT: 11.15 min Scan# 837

Delta R.T. 0.01 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:178 Resp: 5541056

Ion Ratio Lower Upper

178 100

176 20.6 15.8 23.6



179 16.7 13.0 19.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#71

Anthracene

Concen: 239.13 ng/mL

RT: 11.19 min Scan# 840

Delta R.T. -0.01 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:178 Resp: 1856724

Ion Ratio Lower Upper

178 100

176 20.2 15.6 23.4




179 17.1 12.8 19.2



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



#72

Carbazole

Concen: 104.14 ng/mL

RT: 11.32 min Scan# 852

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:167 Resp: 756640

Ion Ratio Lower Upper

167 100

166 22.2 17.8 26.6



139 13.8 11.2 16.8




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E





#74

Fluoranthene

Concen: 490.42 ng

RT: 12.32 min Scan# 939

Delta R.T. 0.00 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:202 Resp: 3983790

Ion Ratio Lower Upper

202 100

101 12.6 0.0 33.1




203 18.8 0.0 38.1



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.71 min Scan# 1061

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:240 Resp: 123194

Ion Ratio Lower Upper

240 100

120 9.7 6.8 10.2



236 24.9 20.2 30.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E





#77

Pvrene

Concen: 341.93 ng/mL

RT: 12.54 min Scan# 958

Delta R.T. -0.01 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:202 Resp: 3125884

Ion Ratio Lower Upper

202 100

200 22.7 17.4 26.2




203 26.7 14.5 21.7#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



#78

Terphenyl-d14

Concen: 86.64 ng/mL

RT: 12.66 min Scan# 969

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:244 Resp: 469074

Ion Ratio Lower Upper

244 100

212 6.8 6.0 9.0



122 8.5 11.2 16.8#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E





#80

Benzo(a)anthracene

Concen: 140.27 ng m

RT: 13.70 min Scan# 1060

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:228 Resp: 984746

Ion Ratio Lower Upper

228 100

226 28.0 22.3 33.5




229 21.0 16.0 24.0



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#82

Chrysene

Concen: 107.64 ng m

RT: 13.74 min Scan# 1063

Delta R.T. -0.03 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:228 Resp: 710896

Ion Ratio Lower Upper

228 100

226 31.5 25.4 38.2



229 22.5 16.3 24.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E









#85
Indeno(1,2,3-cd)pyrene
Concen: 11.70 ng
RT: 16.30 min Scan# 1287
Delta R.T. -0.07 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51




Instrument :
BNA_F
ClientSampleId :
Q8-B4(0-2)C


Tot Ion:276 Resp: 71791
Ion Ratio Lower Upper
276 100
138 25.6 0.0 0.0#
277 24.2 0.0 0.0#



#86
Perylene-d12
Concen: 20.00 ng
RT: 15.05 min Scan# 1178
Delta R.T. -0.06 min
Lab File: BF088374.D
Acq: 25 Jun 2016 13:51

Tgt Ion:264 Resp: 143085
Ion Ratio Lower Upper
264 100
260 23.3 19.2 28.8
265 23.1 16.9 25.3





#87

Benzo(b)fluoranthene

Concen: 50.37 ng m

RT: 14.70 min Scan# 1147

Delta R.T. -0.05 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:252 Resp: 502295

Ion Ratio Lower Upper

252 100

253 22.8 17.4 26.2




125 13.2 7.1 10.7#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#88

Benzo(k)fluoranthene

Concen: 22.95 ng m

RT: 14.71 min Scan# 1148

Delta R.T. -0.06 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:252 Resp: 172632

Ion Ratio Lower Upper

252 100

253 23.2 18.0 27.0



125 14.1 11.2 16.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E





#89

Benzo(a)pyrene

Concen: 34.06 ng/mL

RT: 15.01 min Scan# 1174

Delta R.T. -0.05 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51

Instrument :

BNA_F

ClientSampleId :

Q8-B4(0-2)C


Tot Ion:252 Resp: 274847

Ion Ratio Lower Upper

252 100

253 22.7 17.9 26.9




125 12.3 12.5 18.7#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#90

Dibenzo(a,h)anthracene

Concen: 2.52 ng/mL

RT: 16.30 min Scan# 1287

Delta R.T. -0.07 min

Lab File: BF088374.D

Acq: 25 Jun 2016 13:51


Tgt Ion:278 Resp: 18889

Ion Ratio Lower Upper

278 100

139 34.8 15.7 23.5#



279 41.2 19.4 29.2#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E






#91
 Benzo(a,h,i)perylene
 Concen: 7.25 ng
 RT: 16.66 min Scan# 1319
 Delta R.T. -0.08 min
 Lab File: BF088374.D
 Acq: 25 Jun 2016 13:51

Instrument :
 BNA_F
 ClientSampleId :
 Q8-B4(0-2)C

Tot Ion	Ratio	Lower	Upper
276	100		
277	26.2	18.9	28.3
138	28.2	21.4	32.2



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

