

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062516\
 Data File : BF088404.D
 Acq On : 26 Jun 2016 6:31
 Operator : UM/SJ
 Sample : H3599-02DL 10X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PM-STA-1402(0-4)DL

Quant Time: Jun 26 08:25:36 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 14:55:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.56	152	93801	20.00	ng	-0.05
21) Naphthalene-d8	7.85	136	382808	20.00	ng	-0.05
38) Acenaphthene-d10	9.59	164	159936	20.00	ng	-0.06
63) Phenanthrene-d10	11.06	188	261007	20.00	ng	-0.06
75) Chrysene-d12	13.69	240	199209	20.00	ng	-0.06
86) Perylene-d12	15.05	264	163799	20.00	ng	-0.06

System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	35973	6.56	ng	-0.02
7) Phenol-d6	6.24	99	52516	7.90	ng	-0.02
23) Nitrobenzene-d5	7.14	82	30220	4.61	ng	-0.03
41) 2,4,6-Tribromophenol	10.39	330	8153	4.83	ng	-0.05
44) 2-Fluorobiphenyl	8.92	172	70340	1.47	ng	-0.05
78) Terphenyl-d14	12.64	244	45733	5.22	ng	-0.06


Target Compounds						Qvalue
48) Acenaphthylene	9.45	152	87855	5.34	ng	99
70) Phenanthrene	11.08	178	75564	5.52	ng	99
71) Anthracene	11.14	178	66769	4.83	ng	97
74) Fluoranthene	12.27	202	297284	20.57	ng	96
77) Pyrene	12.50	202	275365	18.63	ng	98
80) Benzo(a)anthracene	13.68	228	188092	16.57	ng	93
82) Chrysene	13.71	228	153743m	14.40	ng	
85) Indeno(1,2,3-cd)pyrene	16.29	276	88366	8.91	ng	# 100
87) Benzo(b)fluoranthene	14.69	252	226685m	19.86	ng	
88) Benzo(k)fluoranthene	14.70	252	118183m	13.72	ng	
89) Benzo(a)pyrene	14.99	252	132706	14.37	ng	97
90) Dibenzo(a,h)anthracene	16.29	278	22476m	2.62	ng	
91) Benzo(a,h,i)perylene	16.65	276	70396	7.98	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062516\
Data File : BF088404.D
Acq On : 26 Jun 2016 6:31
Operator : UM/SJ
Sample : H3599-02DL 10X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PM-STA-1402(0-4)DL

Quant Time: Jun 26 08:25:36 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

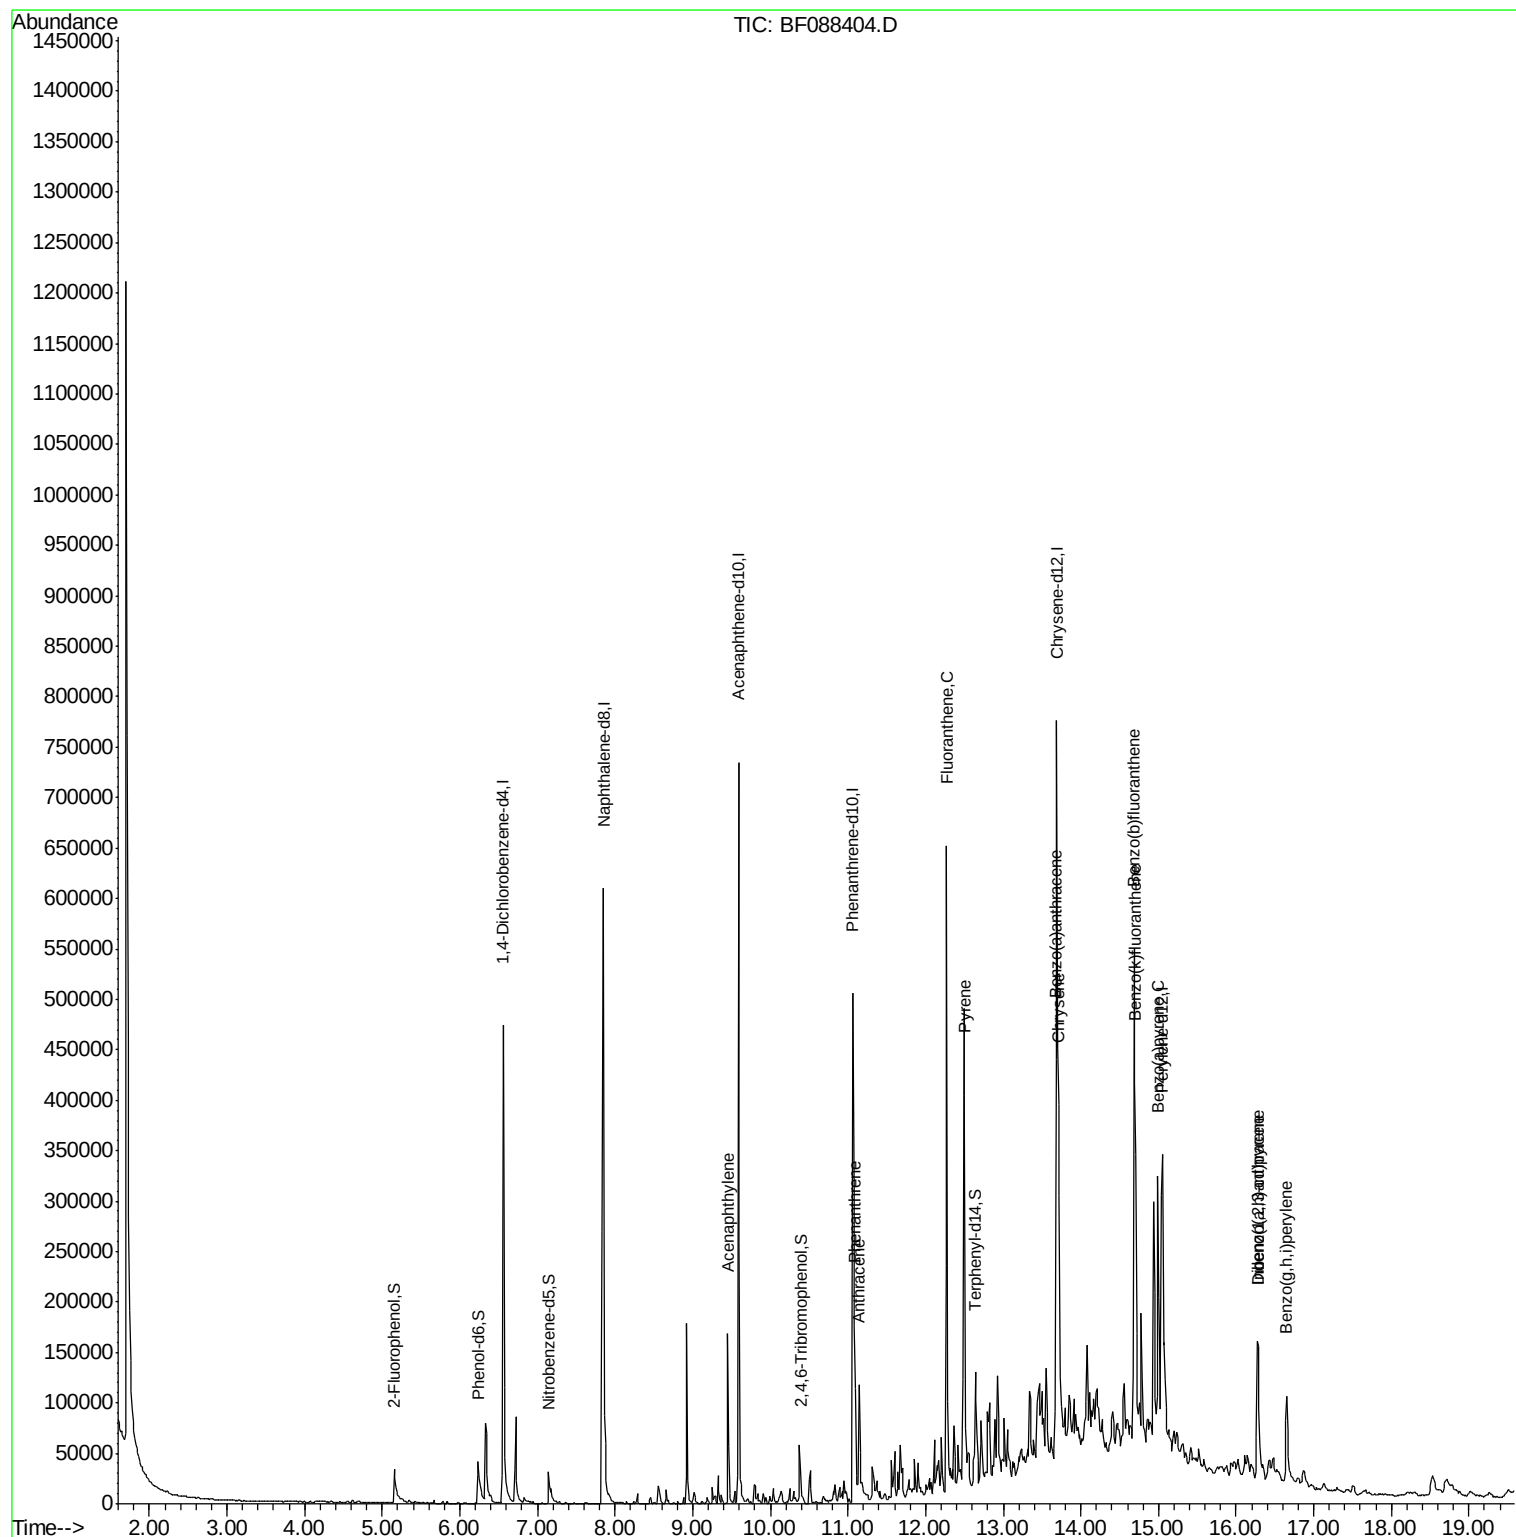

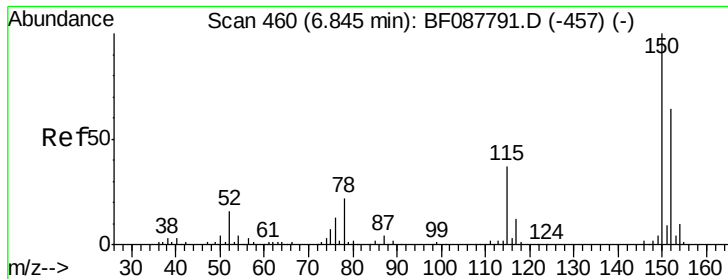

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.56 min Scan# 435

Delta R.T. -0.05 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion:152 Resp: 93801

Ion Ratio Lower Upper

152 100

150 155.3 123.8 185.6




115 59.4 39.6 59.4

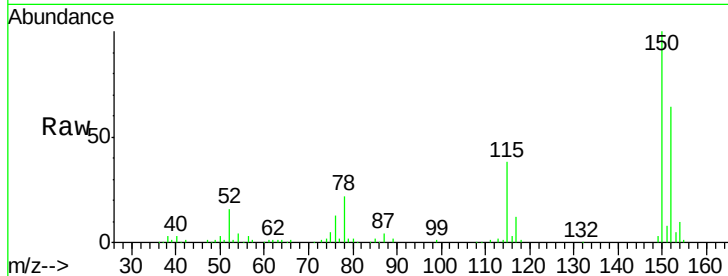

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

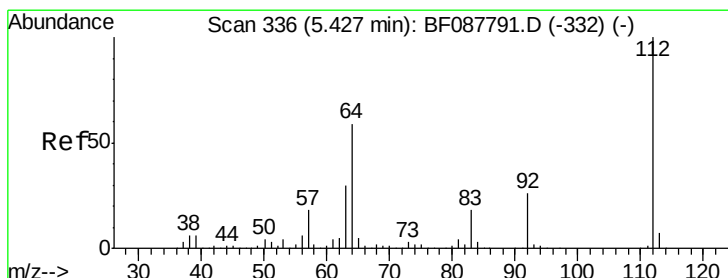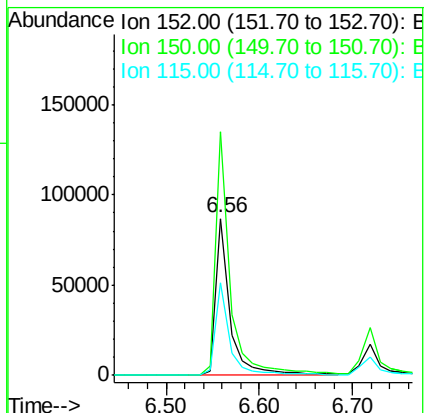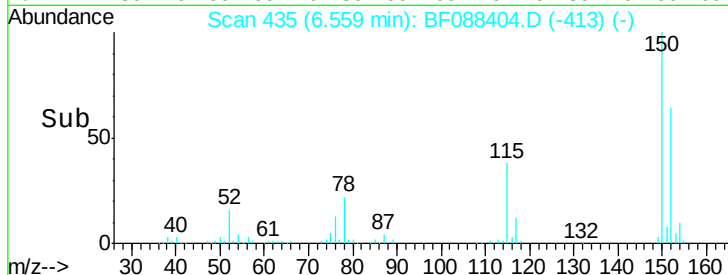

#5

2-Fluorophenol

Concen: 6.56 ng

RT: 5.15 min Scan# 312

Delta R.T. -0.02 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31


Tgt Ion:112 Resp: 35973

Ion Ratio Lower Upper

112 100

64 54.8 42.2 63.2



63 28.6 21.8 32.8

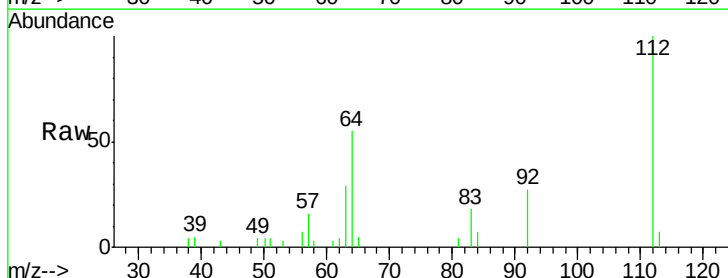


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

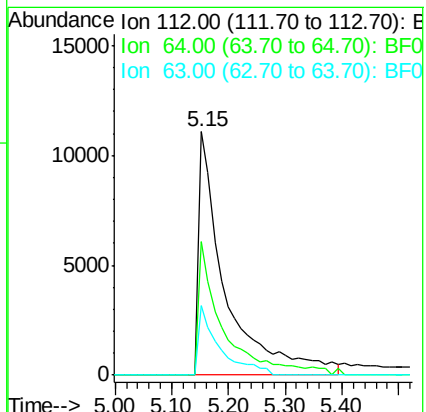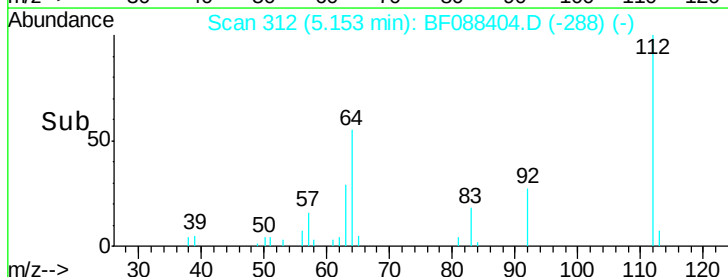

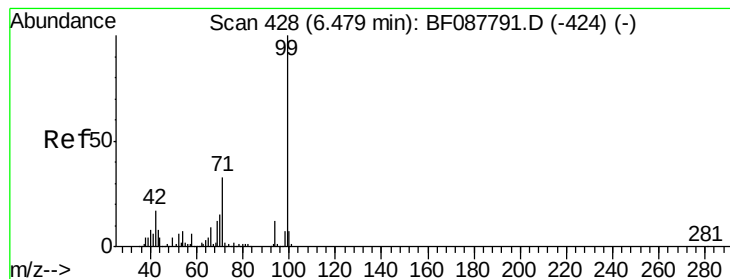

#7

Phenol-d6

Concen: 7.90 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.02 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion: 99 Resp: 52516

Ion Ratio Lower Upper

99 100

42 14.2 12.2 18.2




71 29.7 23.4 35.0

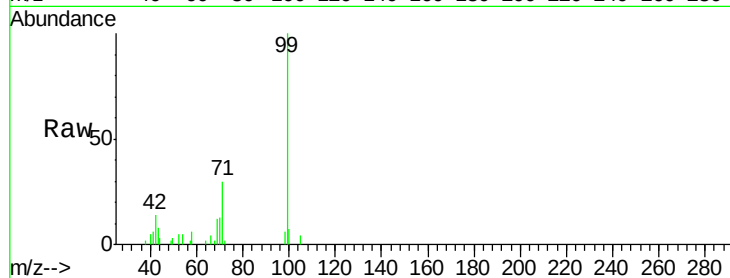

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

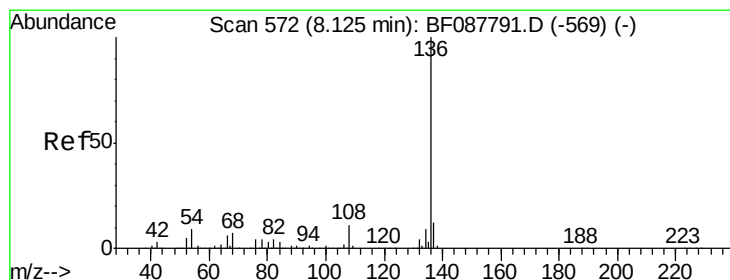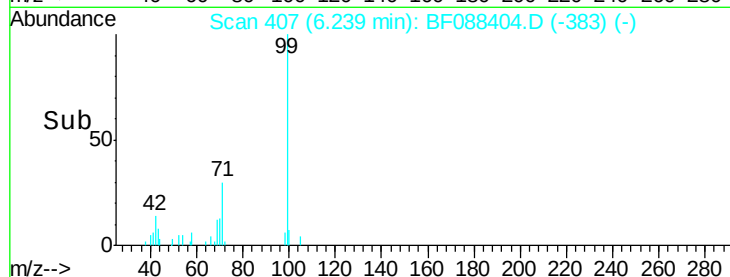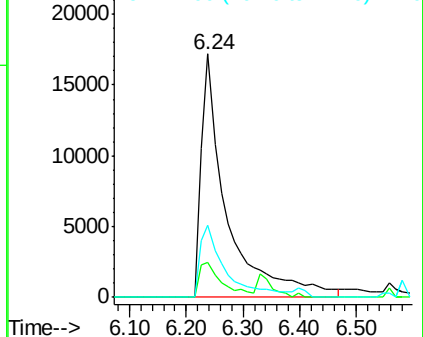

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.85 min Scan# 548

Delta R.T. -0.05 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Tgt Ion: 136 Resp: 382808


Ion Ratio Lower Upper

136 100

137 10.4 9.1 13.7

54 5.1 6.6 10.0#

68 4.5 5.1 7.7#


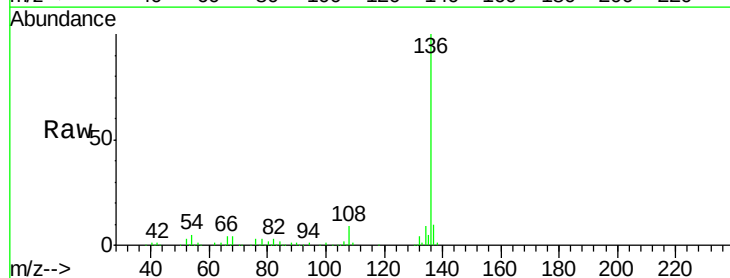



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



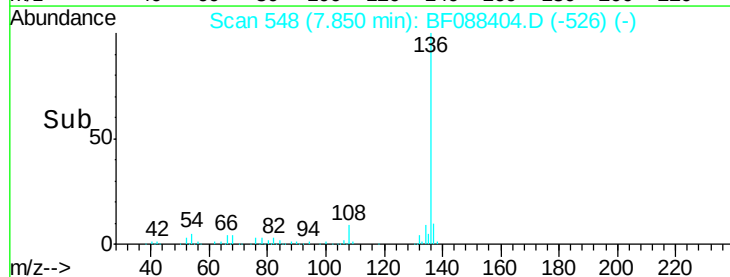
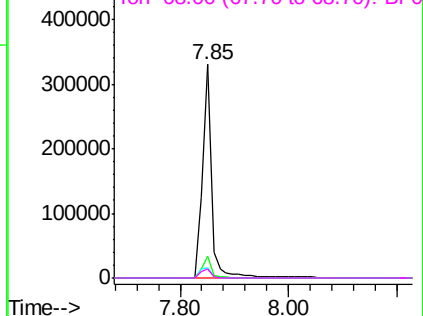


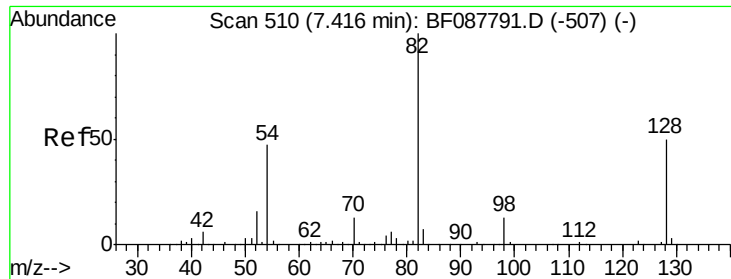

#23
 Nitrobenzene-d5
 Concen: 4.61 ng
 RT: 7.14 min Scan# 486
 Delta R.T. -0.03 min
 Lab File: BF088404.D
 Acq: 26 Jun 2016 6:31




Instrument :
 BNA_F
 ClientSampleId :
 PM-STA-1402(0-4)DL


Tot Ion: 82 Resp: 30220
 Ion Ratio Lower Upper
 82 100
 128 47.3 35.9 53.9
 54 45.1 40.9 61.3

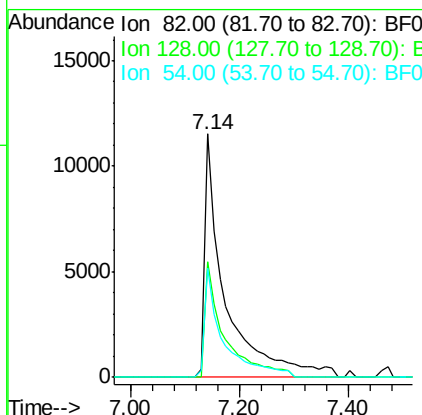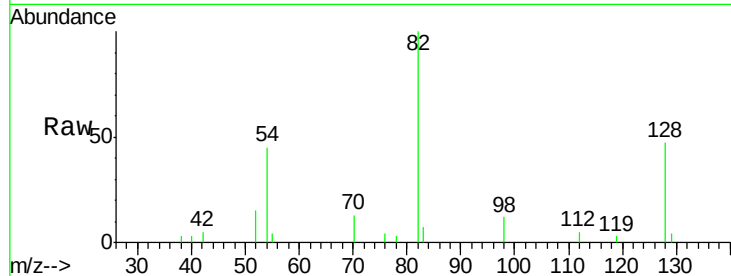

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.59 min Scan# 700
 Delta R.T. -0.06 min
 Lab File: BF088404.D
 Acq: 26 Jun 2016 6:31

Tgt Ion:164 Resp: 159936
 Ion Ratio Lower Upper
 164 100
 162 104.6 85.4 128.2
 160 46.5 39.5 59.3

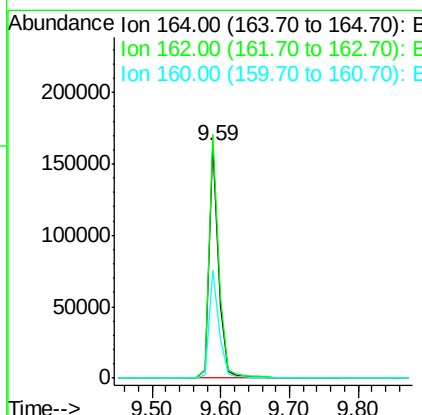







#41
 2,4,6-Tribromophenol
 Concen: 4.83 ng
 RT: 10.39 min Scan# 770
 Delta R.T. -0.05 min
 Lab File: BF088404.D
 Acq: 26 Jun 2016 6:31

Instrument :
 BNA_F
 ClientSampleId :
 PM-STA-1402(0-4)DL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.3	0.0	0.0#
141	55.2	0.0	0.0#

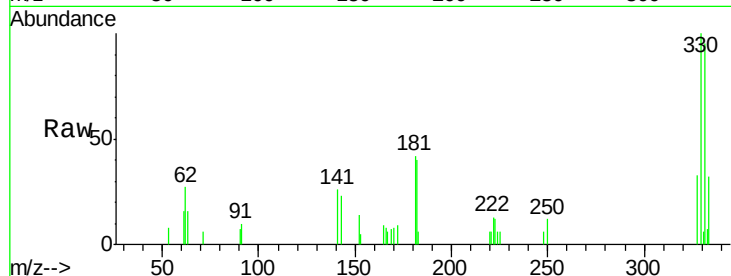


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


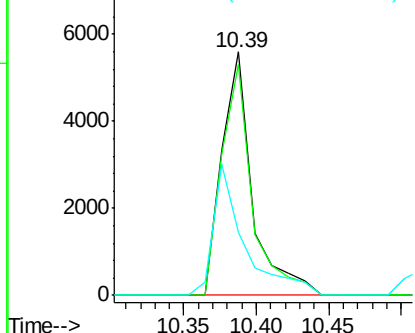



#44
 2-Fluorobiphenyl
 Concen: 1.47 ng
 RT: 8.92 min Scan# 642
 Delta R.T. -0.05 min
 Lab File: BF088404.D
 Acq: 26 Jun 2016 6:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.1	28.6	43.0
170	22.5	19.2	28.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

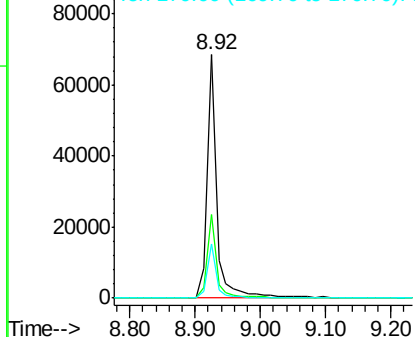

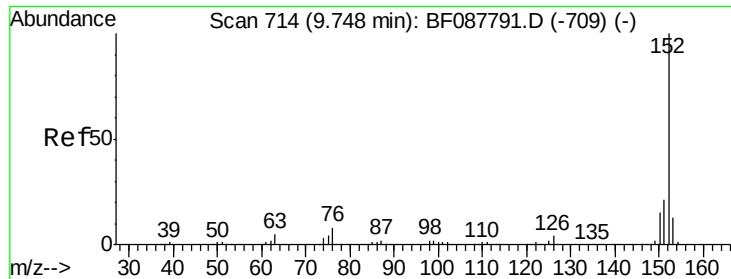

#48

Acenaphthylene

Concen: 5.34 ng

RT: 9.45 min Scan# 688

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion:152 Resp: 87855

Ion Ratio Lower Upper

152 100

151 19.7 16.2 24.4




153 13.4 11.0 16.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

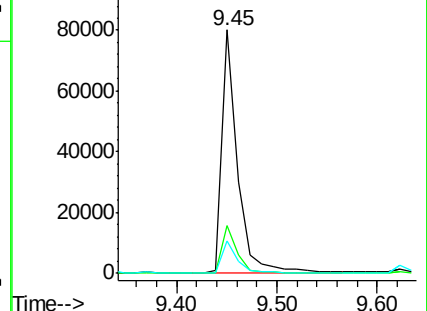

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.06 min Scan# 829

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31


Tgt Ion:188 Resp: 261007

Ion Ratio Lower Upper

188 100

94 12.2 9.0 13.6



80 13.5 10.0 15.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

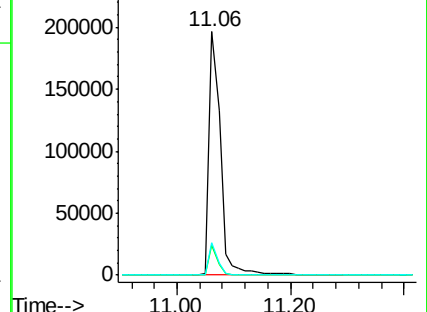



#70

Phenanthrene

Concen: 5.52 ng

RT: 11.08 min Scan# 831

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion:178 Resp: 75564

Ion Ratio Lower Upper

178 100

176 19.3 15.8 23.6




179 15.8 13.0 19.4



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

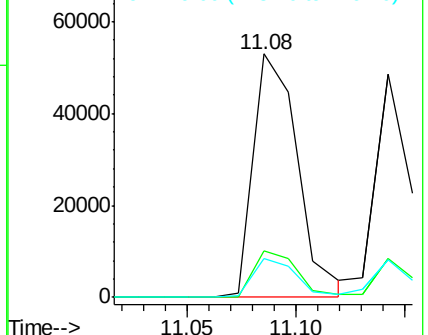

#71

Anthracene

Concen: 4.83 ng

RT: 11.14 min Scan# 836

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31


Tgt Ion:178 Resp: 66769

Ion Ratio Lower Upper

178 100

176 17.5 15.6 23.4



179 16.6 12.8 19.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



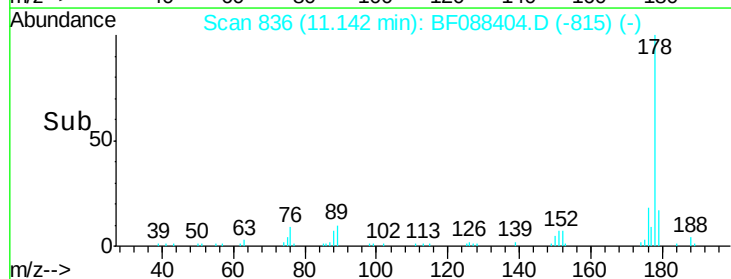
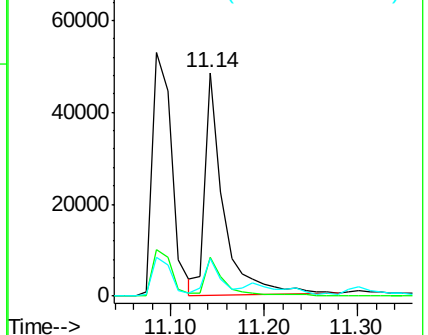


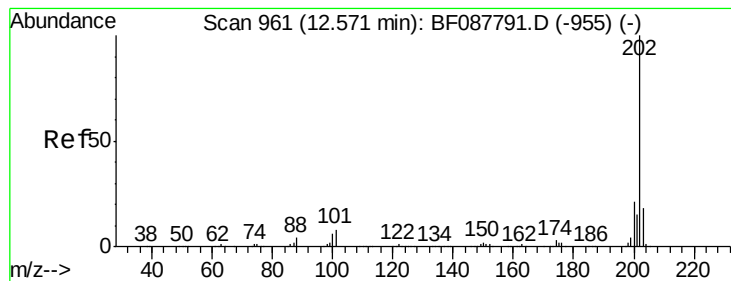

#74
Fluoranthene
Concen: 20.57 ng
RT: 12.27 min Scan# 935
Delta R.T. -0.05 min
Lab File: BF088404.D
Acq: 26 Jun 2016 6:31




Instrument :
BNA_F
ClientSampleId :
PM-STA-1402(0-4)DL


Tot Ion	Ratio	Lower	Upper
202	100		
101	10.2	0.0	33.1
203	17.2	0.0	38.1

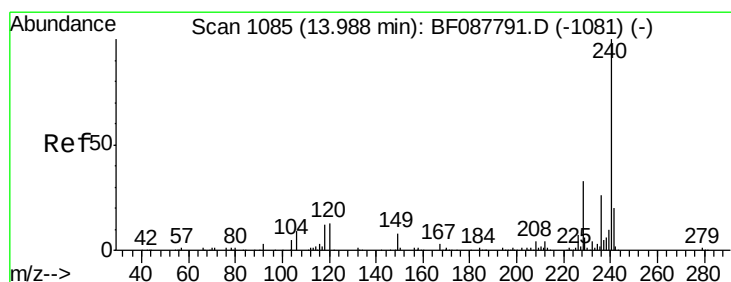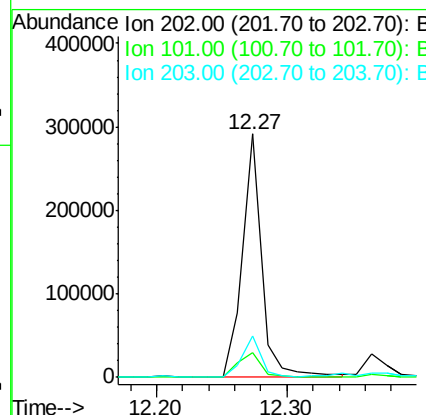

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.69 min Scan# 1059
Delta R.T. -0.06 min
Lab File: BF088404.D
Acq: 26 Jun 2016 6:31

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.5	6.8	10.2#
236	25.4	20.2	30.2

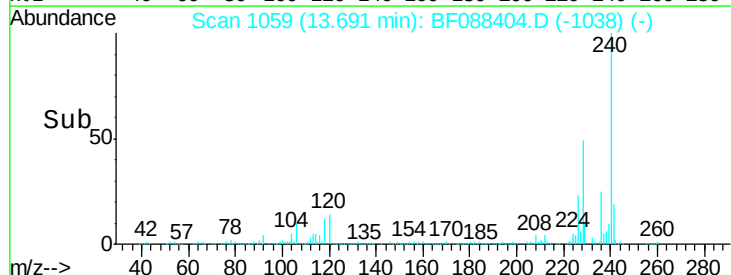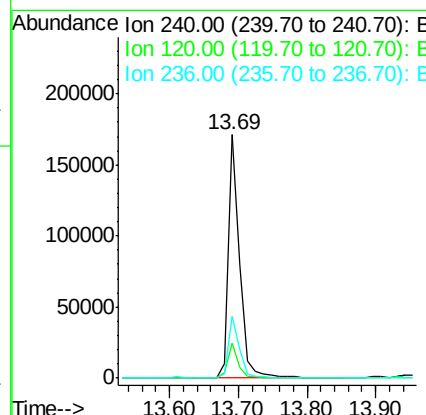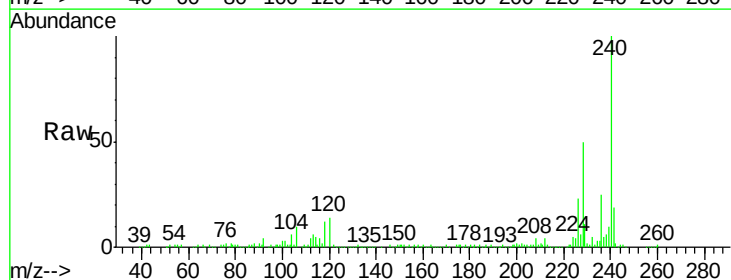

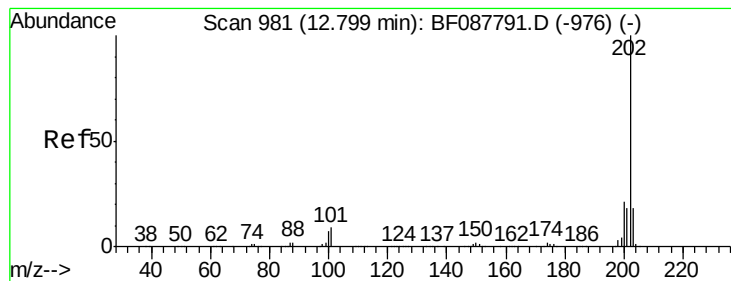

#77

Pvrene

Concen: 18.63 ng

RT: 12.50 min Scan# 955

Delta R.T. -0.05 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion:202 Resp: 275365

Ion Ratio Lower Upper

202 100

200 20.7 17.4 26.2




203 17.5 14.5 21.7



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

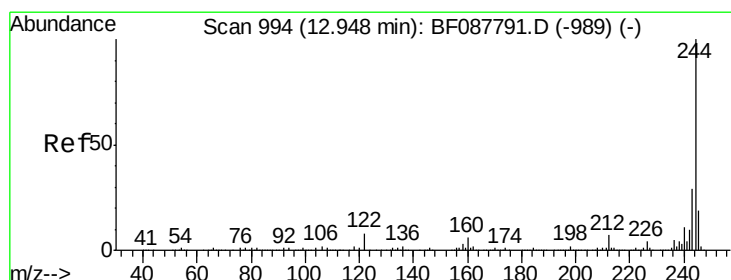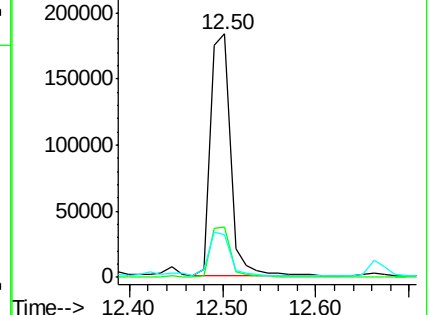

#78

Terphenyl-d14

Concen: 5.22 ng

RT: 12.64 min Scan# 967

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31


Tgt Ion:244 Resp: 45733

Ion Ratio Lower Upper

244 100

212 8.0 6.0 9.0



122 19.4 11.2 16.8#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

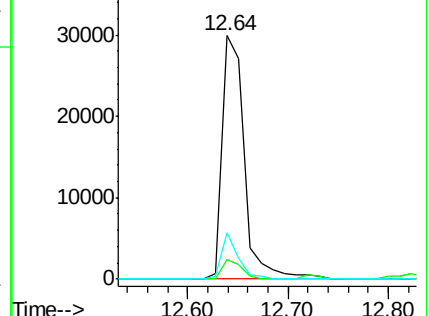

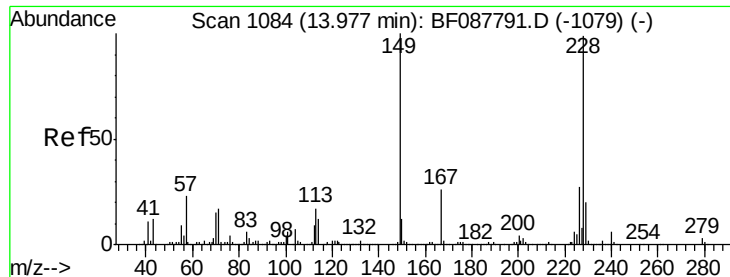

#80

Benzo(a)anthracene

Concen: 16.57 ng

RT: 13.68 min Scan# 1058

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion:228 Resp: 188092

Ion Ratio Lower Upper

228 100

226 31.5 22.3 33.5




229 23.1 16.0 24.0

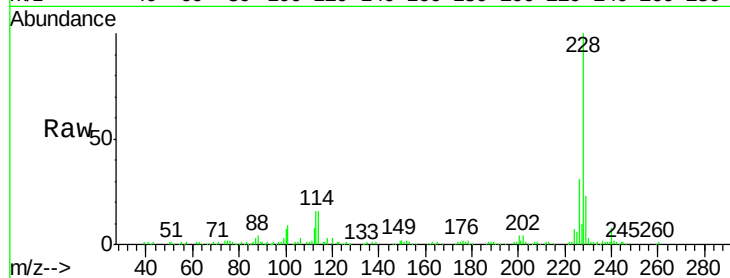

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

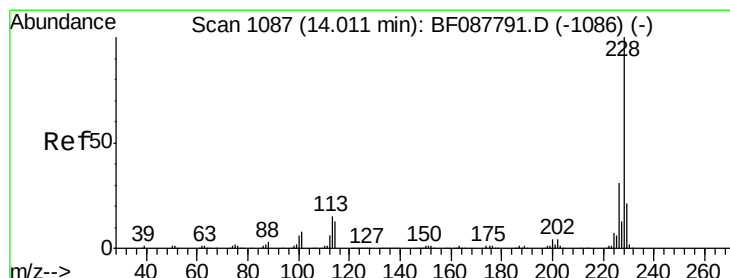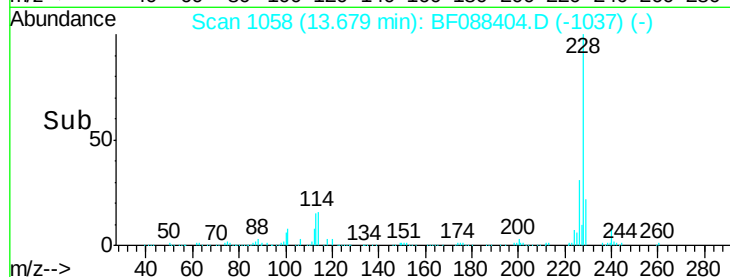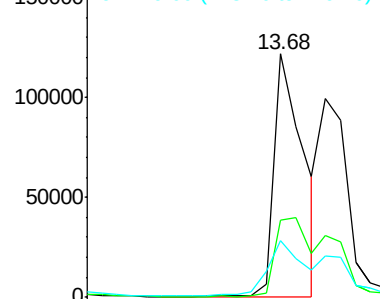

#82

Chrysene

Concen: 14.40 ng m

RT: 13.71 min Scan# 1061

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31


Tgt Ion:228 Resp: 153743

Ion Ratio Lower Upper

228 100

226 31.1 25.4 38.2



229 21.0 16.3 24.5

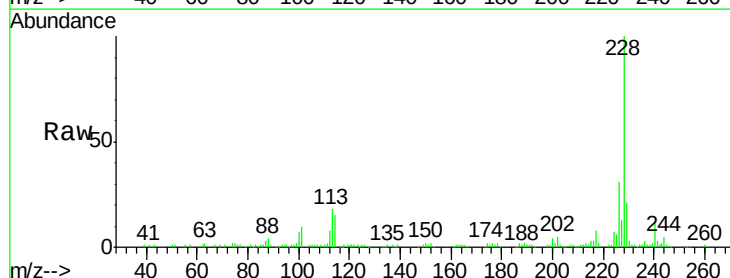


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



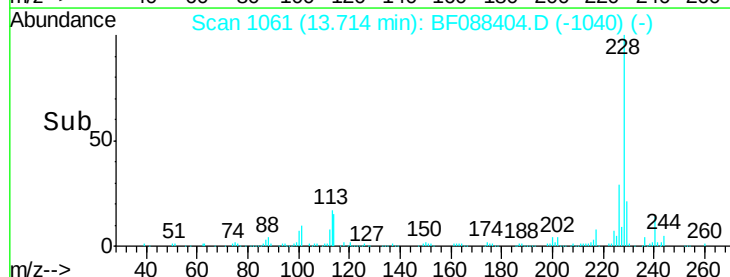
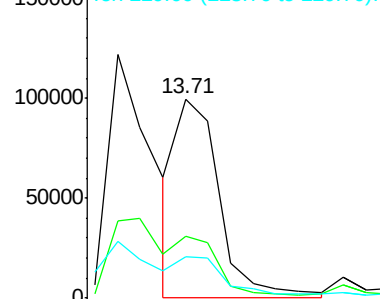


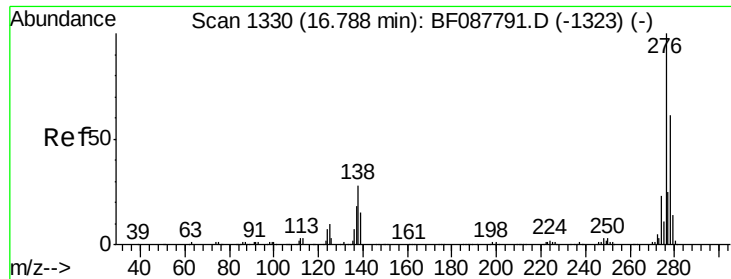

#85
 Indeno(1,2,3-cd)pyrene
 Concen: 8.91 ng
 RT: 16.29 min Scan# 1286
 Delta R.T. -0.08 min
 Lab File: BF088404.D
 Acq: 26 Jun 2016 6:31




Instrument :
 BNA_F
 ClientSampleId :
 PM-STA-1402(0-4)DL


Tot Ion	Ratio	Lower	Upper
276	100		
138	27.0	0.0	0.0#
277	23.1	0.0	0.0#

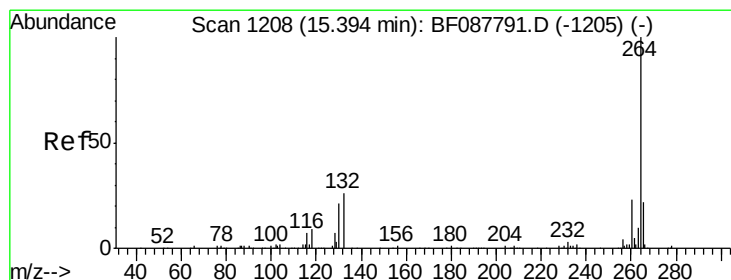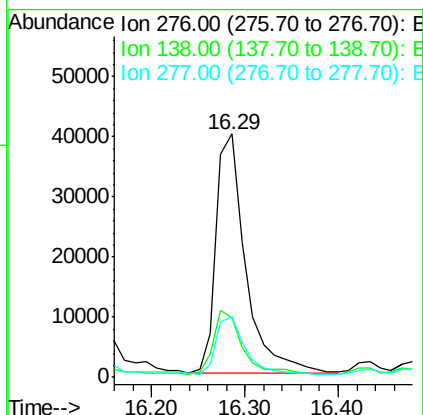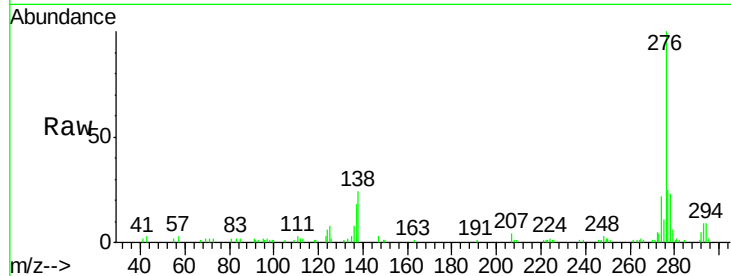

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.05 min Scan# 1178
 Delta R.T. -0.06 min
 Lab File: BF088404.D
 Acq: 26 Jun 2016 6:31

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.2	28.8
265	21.9	16.9	25.3

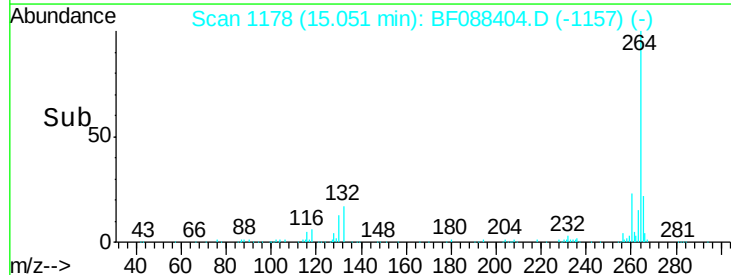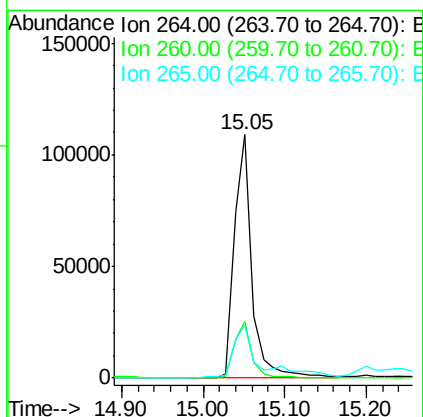



#87

Benzo(b)fluoranthene

Concen: 19.86 ng m

RT: 14.69 min Scan# 1146

Delta R.T. -0.06 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL





Tot Ion:252 Resp: 226685

Ion Ratio Lower Upper

252 100

253 22.6 17.4 26.2

125 14.7 7.1 10.7#

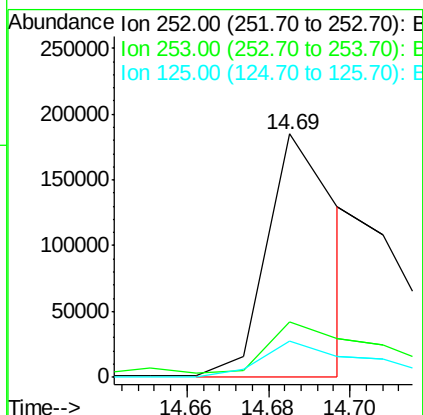

#88

Benzo(k)fluoranthene

Concen: 13.72 ng m

RT: 14.70 min Scan# 1147

Delta R.T. -0.07 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31




Tgt Ion:252 Resp: 118183


Ion Ratio Lower Upper

252 100

253 22.9 18.0 27.0

125 12.6 11.2 16.8

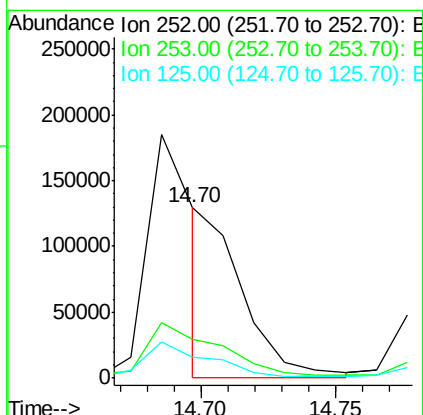


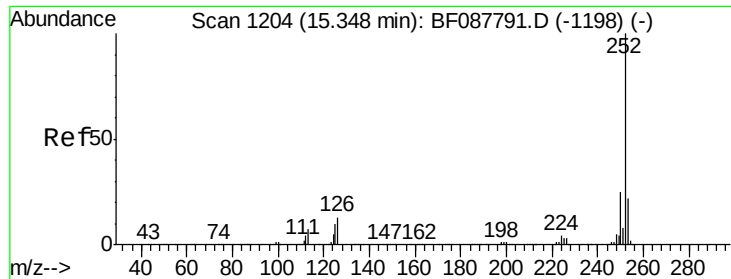




#89
Benzo(a)pyrene
Concen: 14.37 ng
RT: 14.99 min Scan# 1173
Delta R.T. -0.06 min
Lab File: BF088404.D
Acq: 26 Jun 2016 6:31

Instrument :
BNA_F
ClientSampleId :
PM-STA-1402(0-4)DL

Tot Ion:252 Resp: 132706
Ion Ratio Lower Upper
252 100
253 24.1 17.9 26.9
125 14.8 12.5 18.7

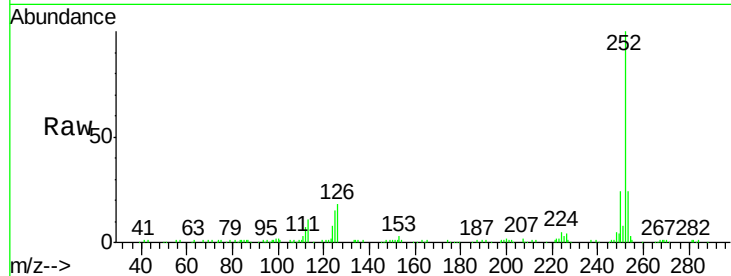


Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E


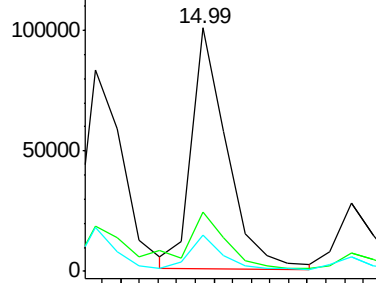



#90
Dibenzo(a,h)anthracene
Concen: 2.62 ng m
RT: 16.29 min Scan# 1286
Delta R.T. -0.08 min
Lab File: BF088404.D
Acq: 26 Jun 2016 6:31

Tgt Ion:278 Resp: 22476
Ion Ratio Lower Upper
278 100
139 0.0 15.7 23.5#
279 27.8 19.4 29.2



Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

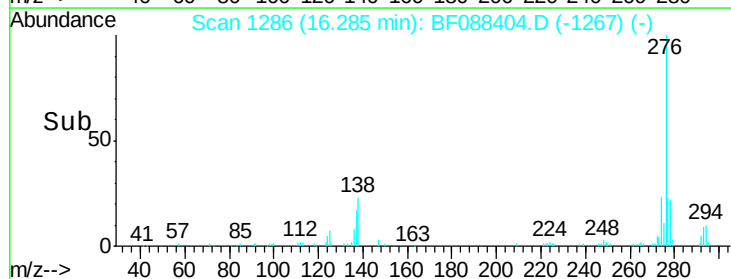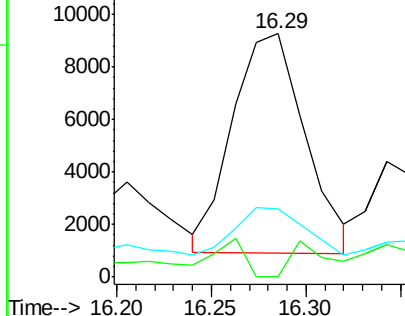

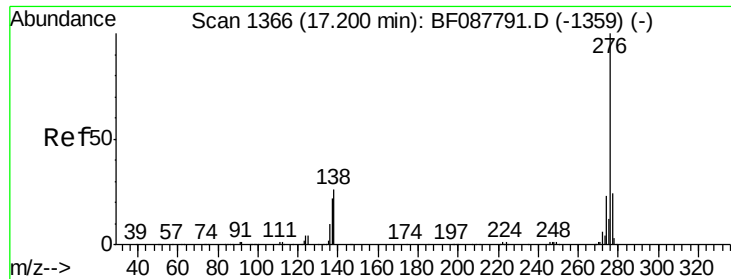

#91

Benzo(a,h,i)perylene

Concen: 7.98 ng

RT: 16.65 min Scan# 1318

Delta R.T. -0.09 min

Lab File: BF088404.D

Acq: 26 Jun 2016 6:31

Instrument :

BNA_F

ClientSampleId :

PM-STA-1402(0-4)DL


Tot Ion: 276 Resp: 70396

Ion Ratio Lower Upper

276 100

277 24.6 18.9 28.3

138 26.6 21.4 32.2



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

