


Data Path : Z:\HPCHEM1\BNA F\Data\BF062516\
 Data File : BF088392.D
 Acq On : 26 Jun 2016 00:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 19:14:18 2016

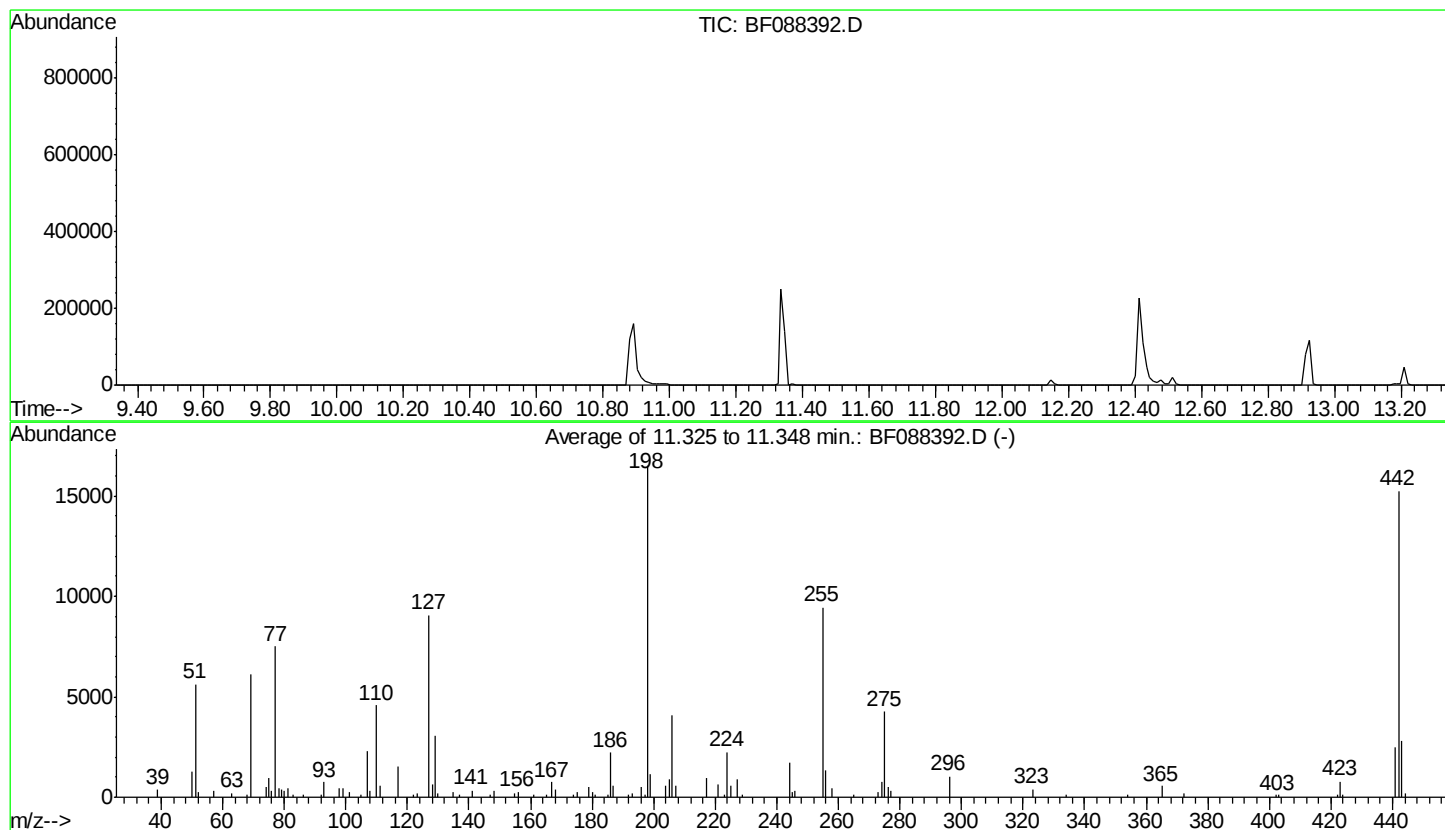

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	5620	PASS
68	69	0.00	2	1.8	109	PASS
69	198	0.00	100	37.1	6127	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.9	9063	PASS
197	198	0.00	2	0.6	102	PASS
198	198	100	100	100.0	16512	PASS
199	198	5	9	6.8	1131	PASS
275	198	10	60	25.8	4266	PASS
365	198	1	100	3.3	545	PASS
441	442	0.01	24	16.4	2502	PASS
442	198	50	100	92.4	15258	PASS
443	442	15	24	18.6	2836	PASS