

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062518\
 Data File : BF106768.D
 Acq On : 25 Jun 2018 13:43
 Operator : JU/SJ
 Sample : J3627-29
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 26KV-CC-15

Quant Time: Jun 25 15:04:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 22 11:34:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	47769	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	186263	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	97231	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	186322	20.00	ng	0.00
75) Chrysene-d12	14.16	240	138631	20.00	ng	0.00
86) Perylene-d12	15.72	264	144768	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	230235	81.61	ng	0.00
7) Phenol-d6	6.60	99	306121	86.89	ng	0.00
23) Nitrobenzene-d5	7.52	82	197514	58.93	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	72367	64.22	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	405300	67.52	ng	-0.01
78) Terphenyl-d14	13.08	244	425802	74.40	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.71	163	45739	6.272	ng	Qvalue # 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062518\
Data File : BF106768.D
Acq On : 25 Jun 2018 13:43
Operator : JU/SJ
Sample : J3627-29
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26KV-CC-15

Quant Time: Jun 25 15:04:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 22 11:34:03 2018
Response via : Initial Calibration

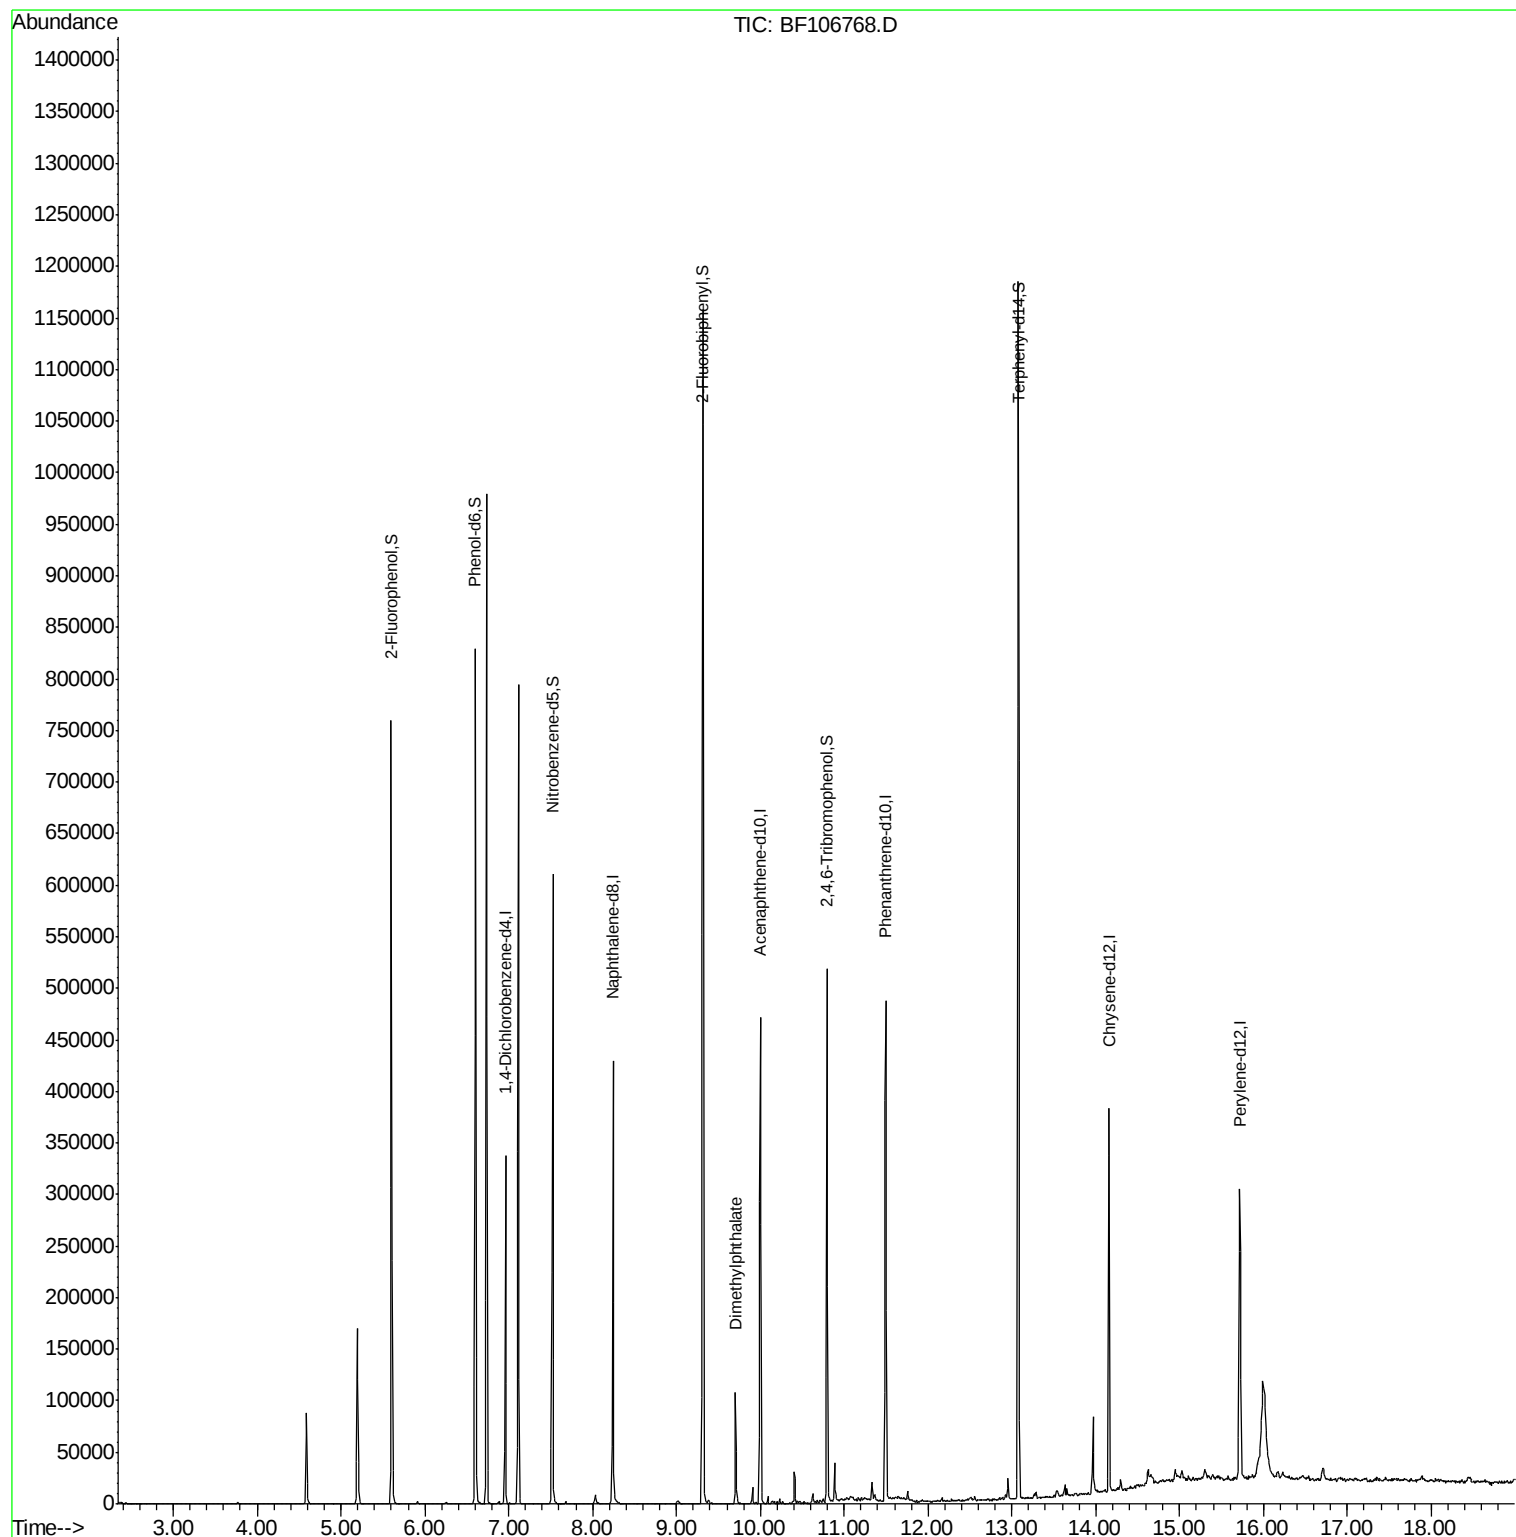




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 786
Delta R.T. 0.00 min
Lab File: BF106768.D
Acq: 25 Jun 2018 13:43

Instrument :
BNA_F
ClientSampleId :
26KV-CC-15

Tot Ion:152 Resp: 47769
Ion Ratio Lower Upper
152 100
150 159.7 124.6 186.8
115 59.6 50.1 75.1

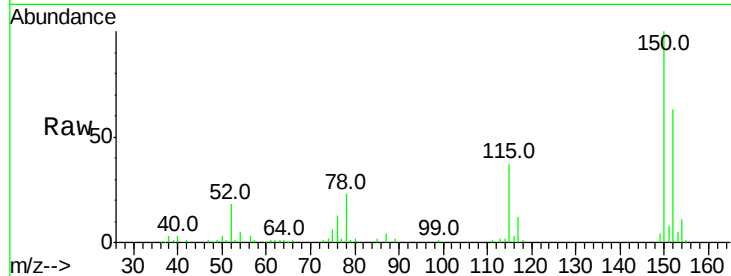


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

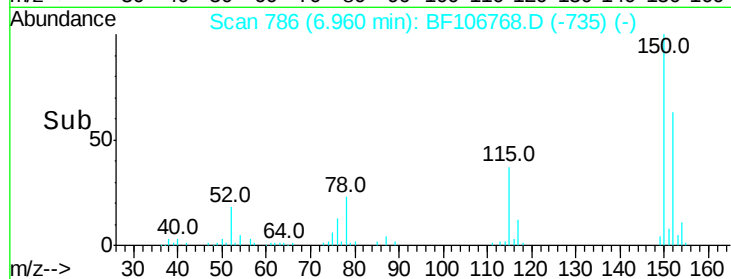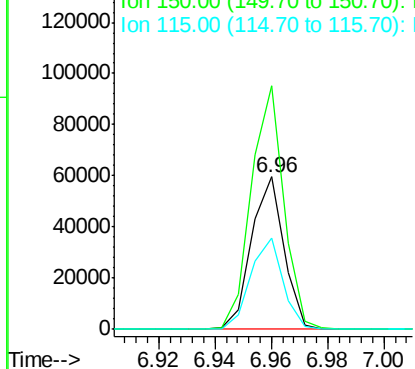



#5

2-Fluorophenol
Concen: 81.614 ng
RT: 5.61 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF106768.D
Acq: 25 Jun 2018 13:43

Tgt Ion:112 Resp: 230235
Ion Ratio Lower Upper
112 100
64 55.6 47.9 71.9
63 27.1 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

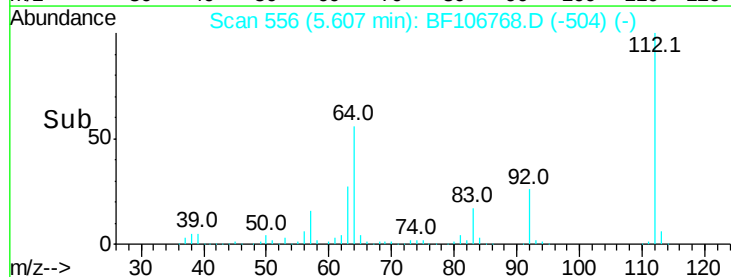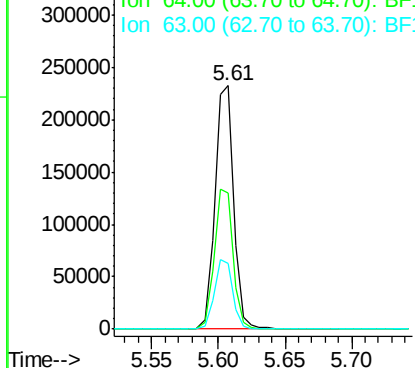



#7

Phenol-d6

Concen: 86.894 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43

Instrument :

BNA_F

ClientSampleId :

26KV-CC-15


Tot Ion: 99 Resp: 306121

Ion Ratio Lower Upper

99 100

42 16.2 14.5 21.7




71 34.1 25.4 38.0

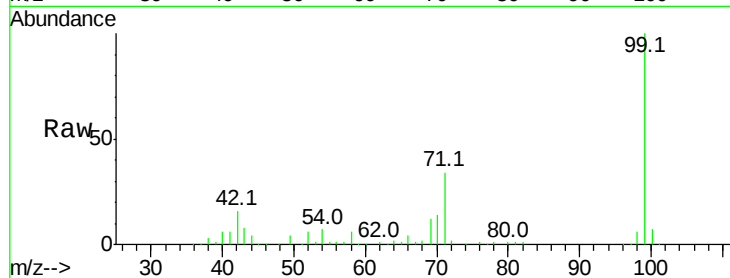

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

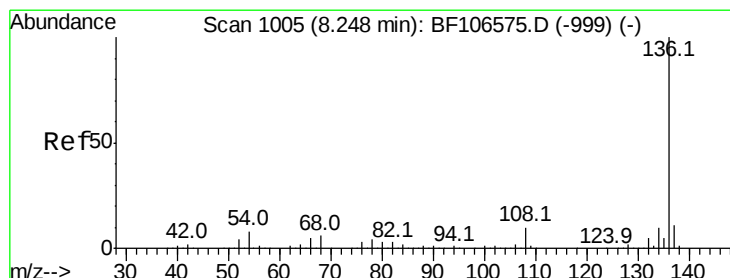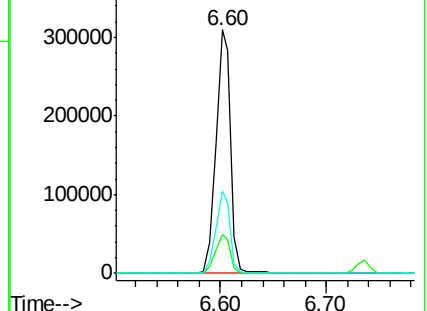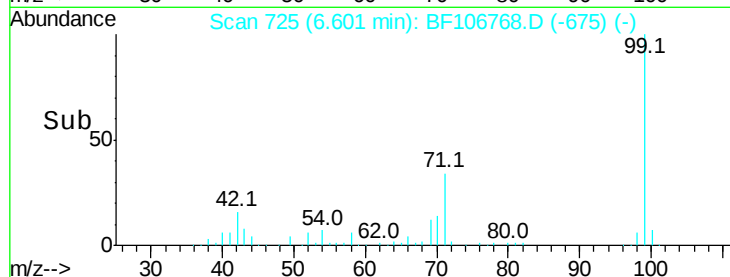

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1004

Delta R.T. -0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43

Tgt Ion: 136 Resp: 186263


Ion Ratio Lower Upper

136 100

137 10.7 8.9 13.3

54 7.6 6.6 9.8

68 6.0 5.0 7.4


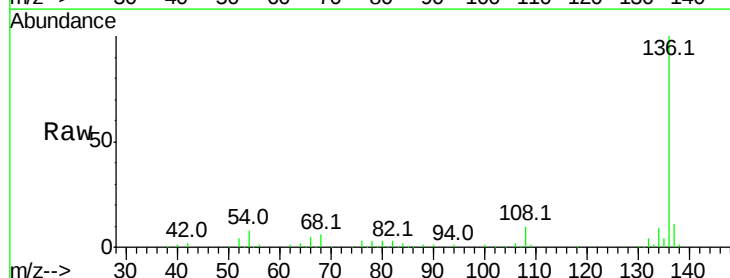



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

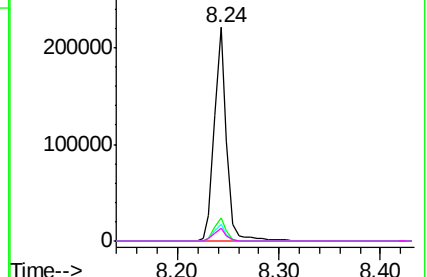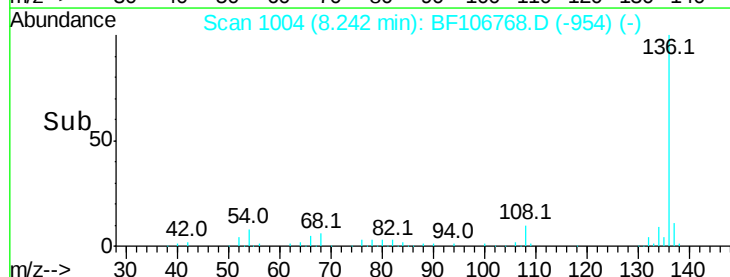

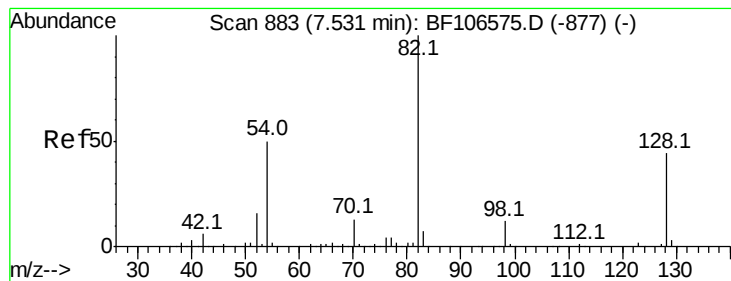

#23

Nitrobenzene-d5

Concen: 58.930 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43

Instrument :

BNA_F

ClientSampleId :

26KV-CC-15


Tot Ion: 82 Resp: 197514

Ion Ratio Lower Upper




82 100

128 46.2 36.1 54.1

54 47.2 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

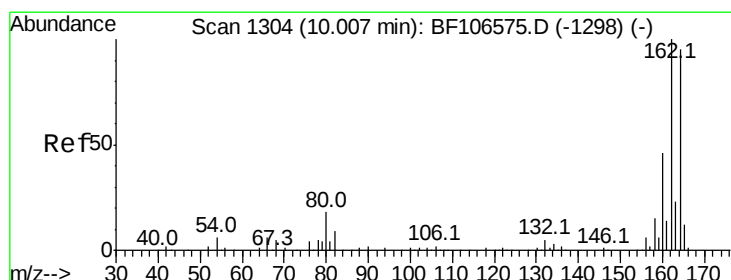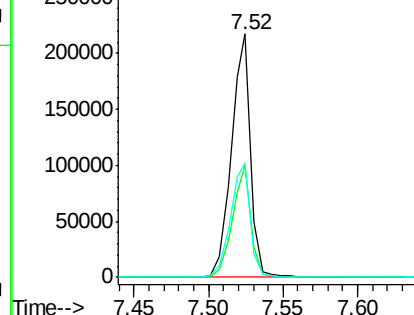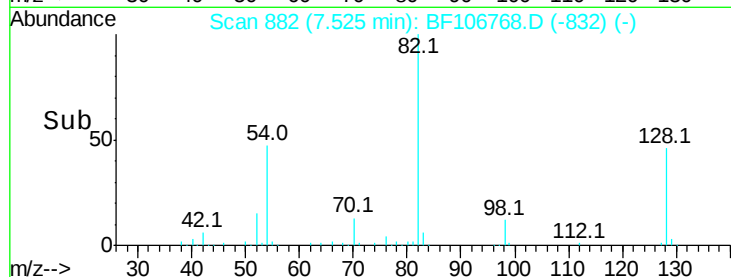

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43


Tgt Ion: 164 Resp: 97231

Ion Ratio Lower Upper



164 100

162 96.8 86.1 129.1

160 45.1 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

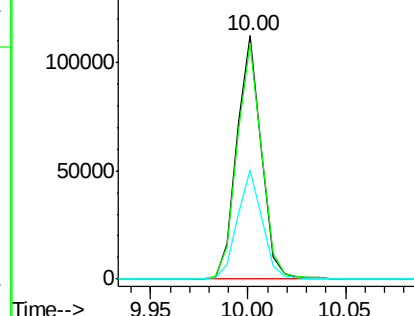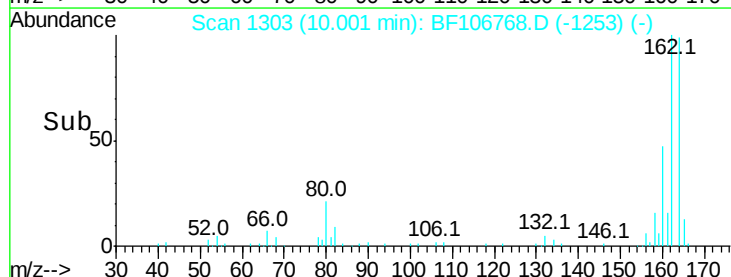






#41
 2,4,6-Tribromophenol
 Concen: 64.216 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF106768.D
 Acq: 25 Jun 2018 13:43

Instrument :
 BNA_F
 ClientSampleId :
 26KV-CC-15

Tot Ion:330 Resp: 72367
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.0 115.6
 141 23.8 29.9 44.9#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

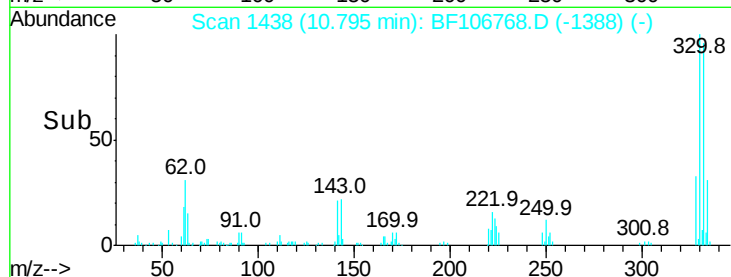
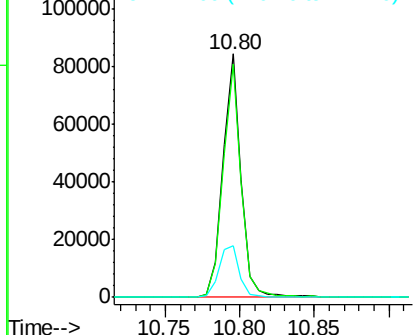


#44
 2-Fluorobiphenyl
 Concen: 67.523 ng
 RT: 9.31 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF106768.D
 Acq: 25 Jun 2018 13:43

Tgt Ion:172 Resp: 405300
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.7 44.5
 170 24.1 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

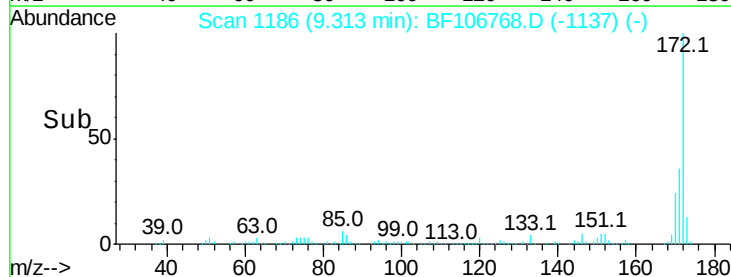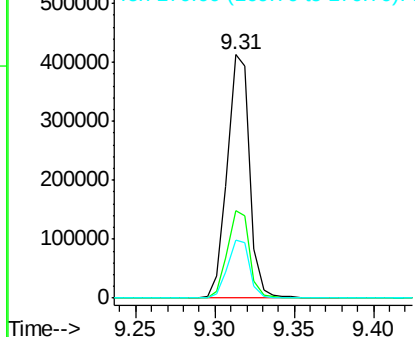



#49

Dimethylphthalate

Concen: 6.272 ng

RT: 9.71 min Scan# 1253

Delta R.T. -0.02 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43

Instrument :

BNA_F

ClientSampleId :

26KV-CC-15


Tot Ion:163 Resp: 45739

Ion Ratio Lower Upper

163 100

194 4.3 2.7 4.1#




164 10.5 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

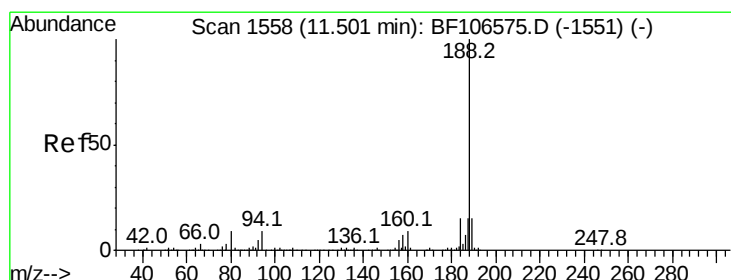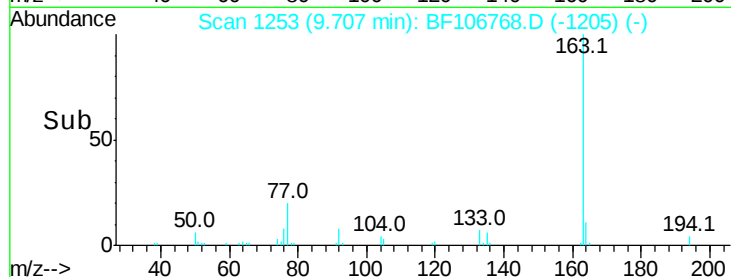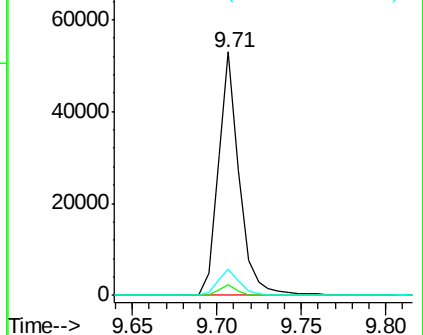

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43


Tgt Ion:188 Resp: 186322

Ion Ratio Lower Upper

188 100

94 8.1 8.5 12.7#



80 8.1 9.2 13.8#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

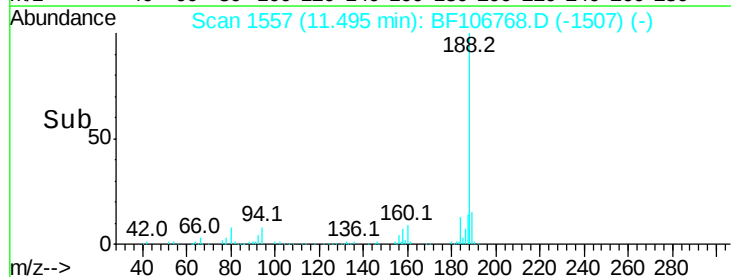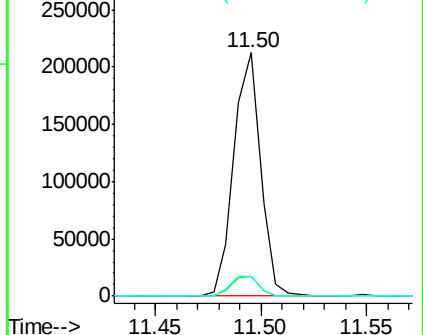



#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2010

Delta R.T. 0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43

Instrument :

BNA_F

ClientSampleId :

26KV-CC-15


Tot Ion:240 Resp: 138631

Ion Ratio Lower Upper

240 100

120 8.3 9.5 14.3#



236 25.8 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

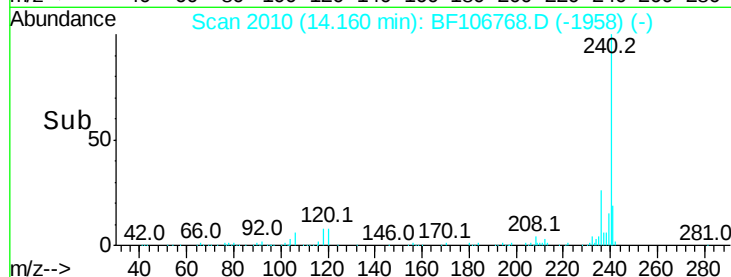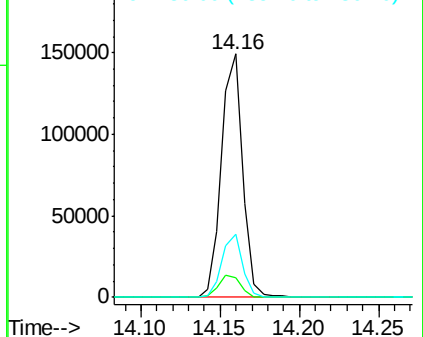

#78

Terphenyl-d14

Concen: 74.400 ng

RT: 13.08 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BF106768.D

Acq: 25 Jun 2018 13:43


Tgt Ion:244 Resp: 425802

Ion Ratio Lower Upper

244 100

212 6.4 5.4 8.0



122 9.0 11.0 16.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

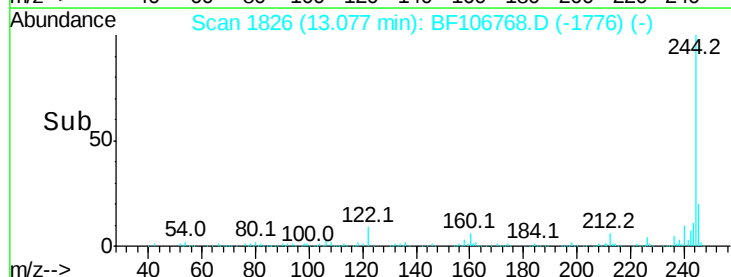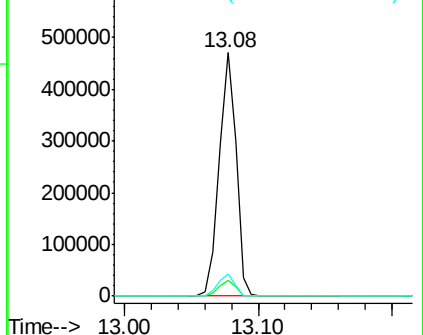




#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.72 min Scan# 2275
 Delta R.T. 0.03 min
 Lab File: BF106768.D
 Acq: 25 Jun 2018 13:43

Instrument :
 BNA_F
 ClientSampleId :
 26KV-CC-15

Tot Ion:	264	Resp:	144768
Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.2	28.8
265	22.0	17.5	26.3



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

