

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062518\
 Data File : BF106808.D
 Acq On : 26 Jun 2018 8:10
 Operator : JU/SJ
 Sample : J3689-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062118-DBRI-E-U-S

Quant Time: Jun 26 09:04:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 25 18:50:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	42932	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	150273	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	65055	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	123458	20.00	ng	0.00
75) Chrysene-d12	14.14	240	117423	20.00	ng	-0.02
86) Perylene-d12	15.68	264	78457	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	98358	38.79	ng	0.00
7) Phenol-d6	6.60	99	75084	23.71	ng	-0.02
23) Nitrobenzene-d5	7.52	82	224027	82.85	ng	-0.01
41) 2,4,6-Tribromophenol	10.79	330	62314	82.64	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	412485	112.01	ng	0.00
78) Terphenyl-d14	13.08	244	454663	93.79	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062518\
Data File : BF106808.D
Acq On : 26 Jun 2018 8:10
Operator : JU/SJ
Sample : J3689-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062118-DBRI-E-U-S

Quant Time: Jun 26 09:04:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 25 18:50:17 2018
Response via : Initial Calibration

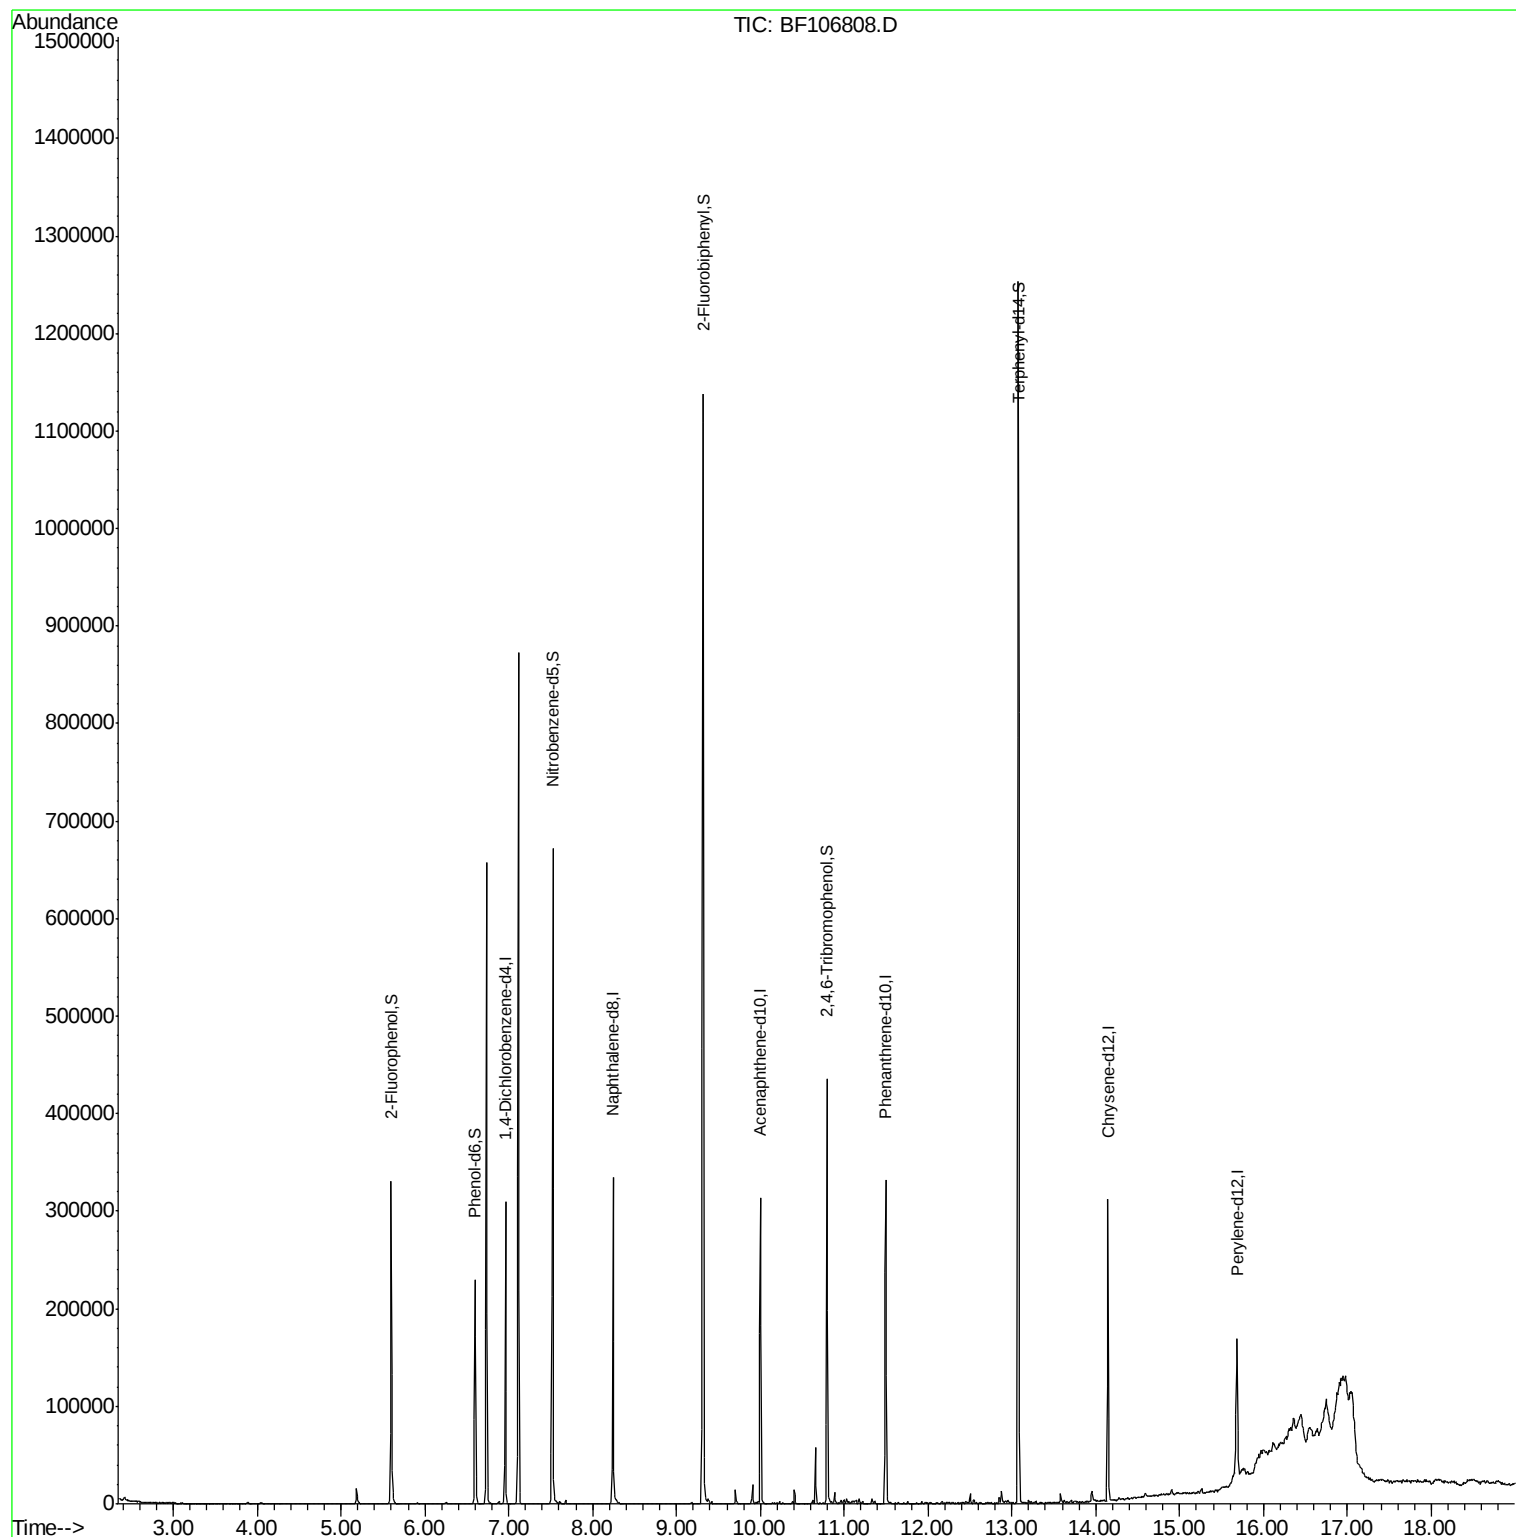




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 786
Delta R.T. -0.00 min
Lab File: BF106808.D
Acq: 26 Jun 2018 8:10

Instrument :
BNA_F
ClientSampleId :
062118-DBRI-E-U-S

Tot Ion:152 Resp: 42932
Ion Ratio Lower Upper
152 100
150 158.0 124.6 186.8
115 59.8 50.1 75.1

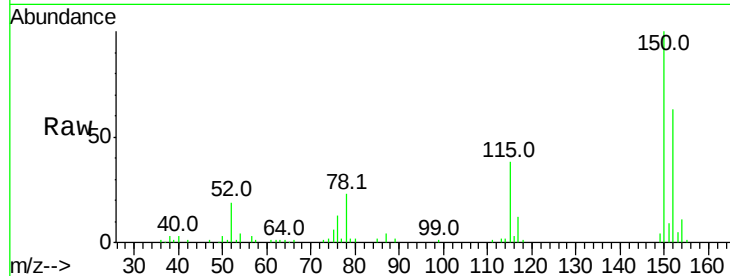


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

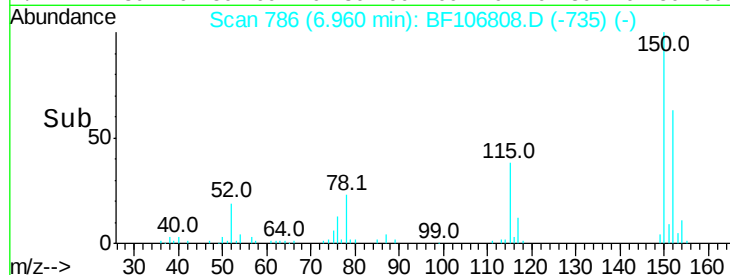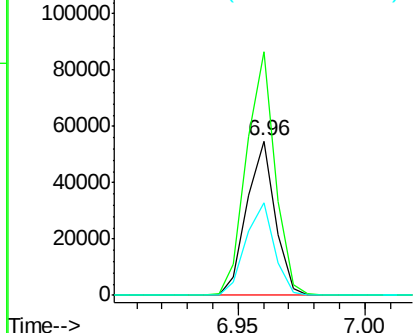



#5

2-Fluorophenol
Concen: 38.794 ng
RT: 5.60 min Scan# 555
Delta R.T. -0.00 min
Lab File: BF106808.D
Acq: 26 Jun 2018 8:10

Tgt Ion:112 Resp: 98358
Ion Ratio Lower Upper
112 100
64 56.0 47.9 71.9
63 27.3 23.7 35.5

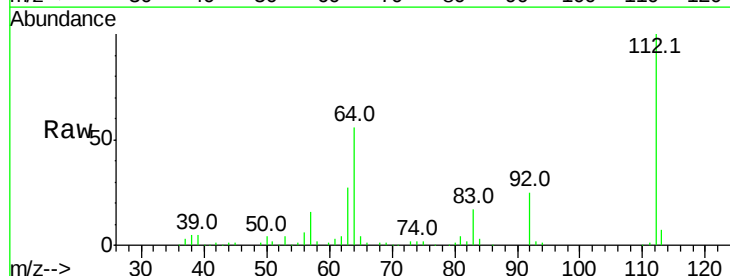

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

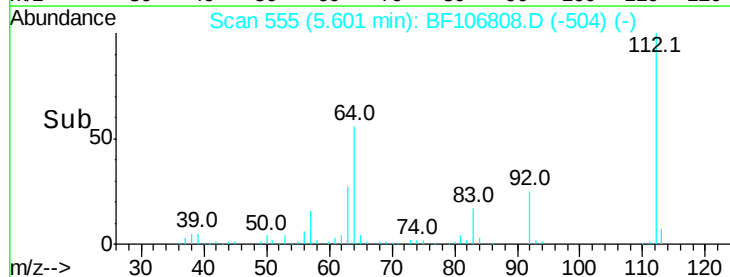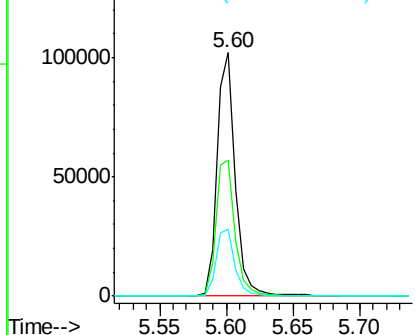



#7

Phenol-d6

Concen: 23.714 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF106808.D

Acq: 26 Jun 2018 8:10

Instrument :

BNA_F

ClientSampleId :

062118-DBRI-E-U-S


Tot Ion: 99 Resp: 75084

Ion Ratio Lower Upper



99 100

42 16.5 14.5 21.7

71 32.7 25.4 38.0

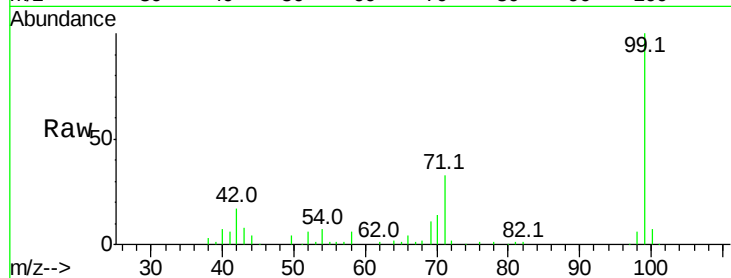

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

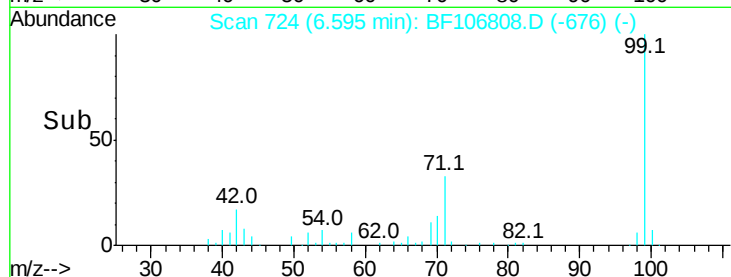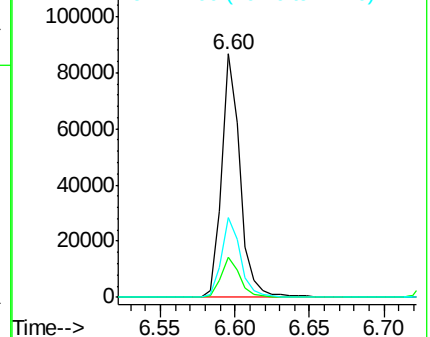

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1004

Delta R.T. -0.01 min

Lab File: BF106808.D

Acq: 26 Jun 2018 8:10

Tgt Ion: 136 Resp: 150273


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3

54 8.0 6.6 9.8

68 6.3 5.0 7.4

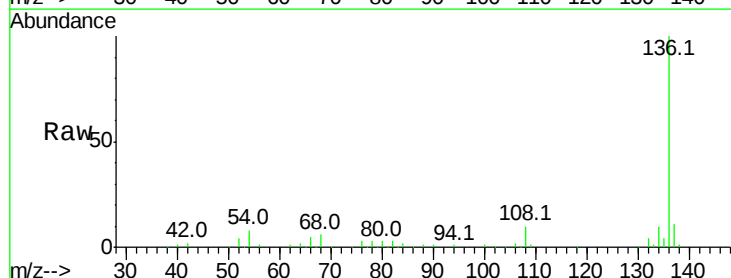

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

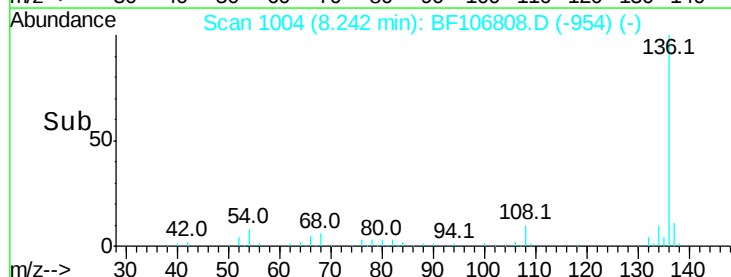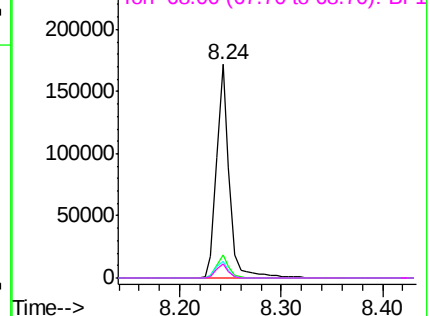






#23
Nitrobenzene-d5
Concen: 82.849 ng
RT: 7.52 min Scan# 882
Delta R.T. -0.01 min
Lab File: BF106808.D
Acq: 26 Jun 2018 8:10

Instrument :
BNA_F
ClientSampleId :
062118-DBRI-E-U-S

Tot Ion	82	Resp	224027
Ion Ratio	Lower	Upper	
82	100		
128	44.9	36.1	54.1
54	48.2	41.4	62.2

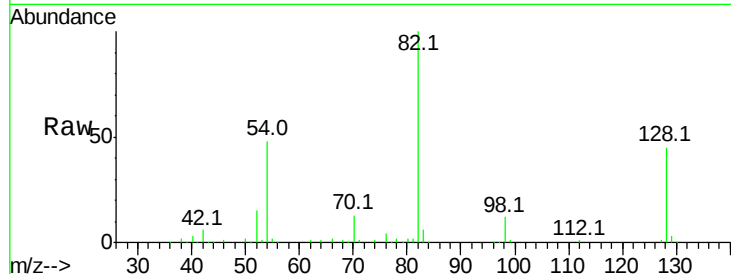


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

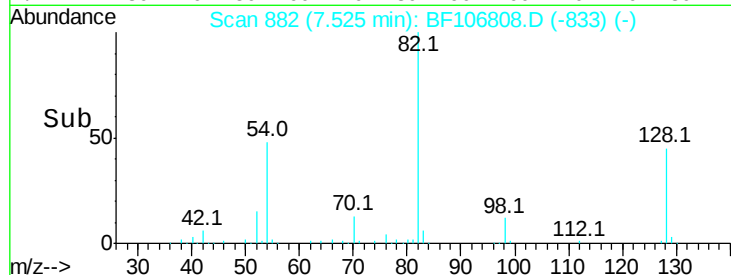
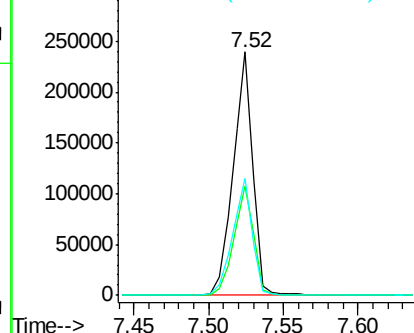


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.00 min Scan# 1303
Delta R.T. -0.01 min
Lab File: BF106808.D
Acq: 26 Jun 2018 8:10

Tgt Ion	164	Resp	65055
Ion Ratio	Lower	Upper	
164	100		
162	99.0	86.1	129.1
160	43.2	38.3	57.5

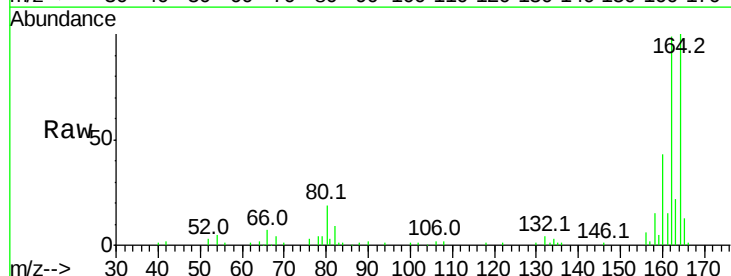

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

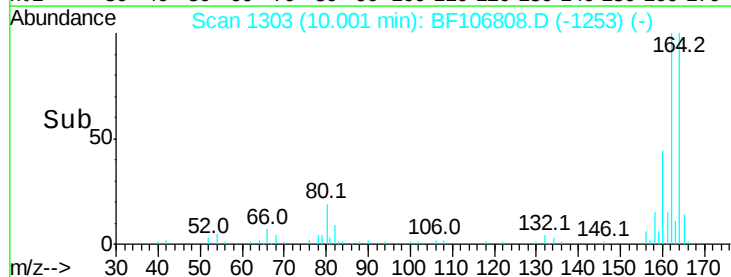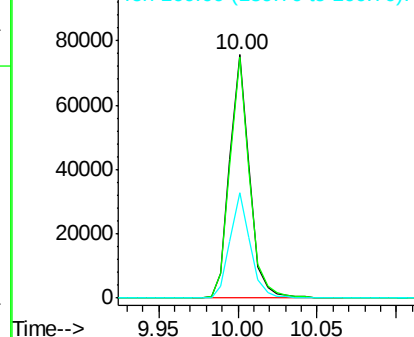






#41
 2,4,6-Tribromophenol
 Concen: 82.644 ng
 RT: 10.79 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF106808.D
 Acq: 26 Jun 2018 8:10

Instrument :
 BNA_F
 ClientSampleId :
 062118-DBRI-E-U-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	23.7	29.9	44.9#

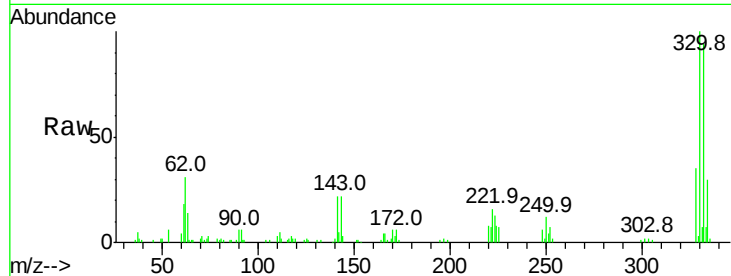


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

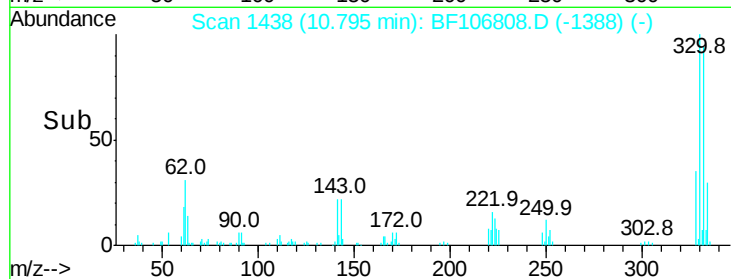
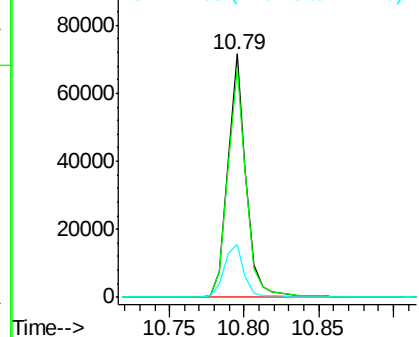


#44
 2-Fluorobiphenyl
 Concen: 112.009 ng
 RT: 9.32 min Scan# 1187
 Delta R.T. -0.01 min
 Lab File: BF106808.D
 Acq: 26 Jun 2018 8:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.7	44.5
170	24.0	19.6	29.4

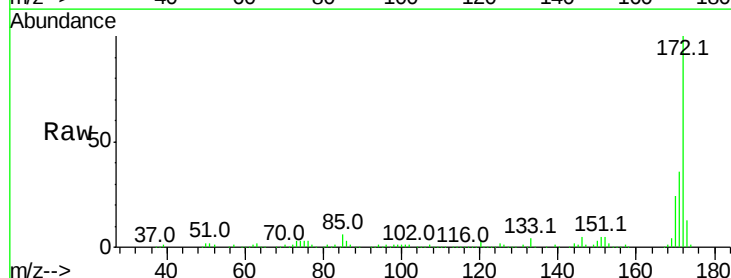

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

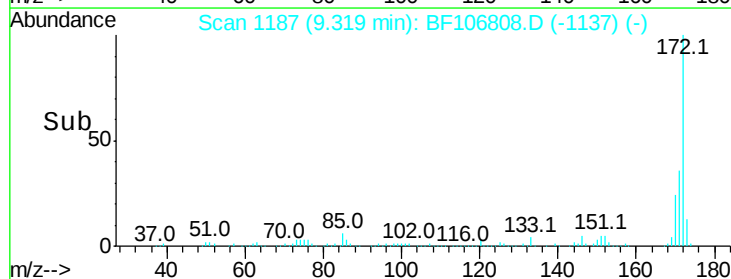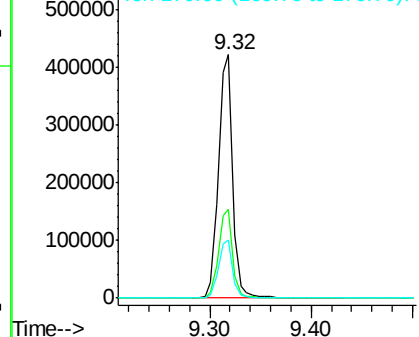



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.49 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106808.D

Acq: 26 Jun 2018 8:10

Instrument :

BNA_F

ClientSampleId :

062118-DBRI-E-U-S


Tot Ion:188 Resp: 123458

Ion Ratio Lower Upper

188 100

94 8.4 8.5 12.7#


80 8.8 9.2 13.8#

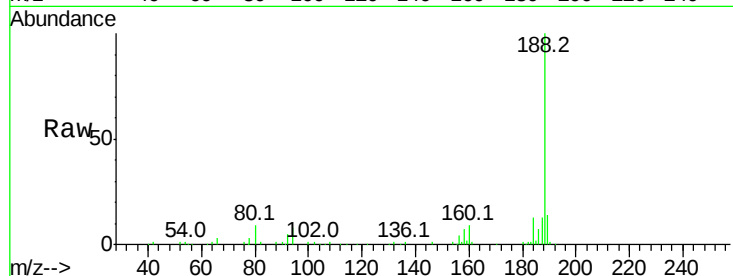



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

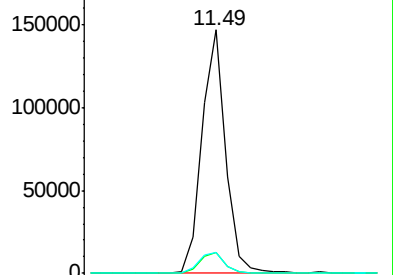

Time-->

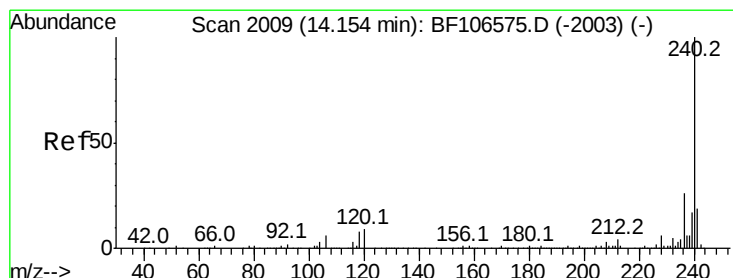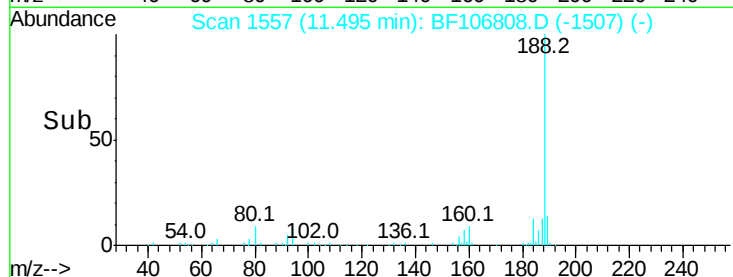

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.14 min Scan# 2007

Delta R.T. -0.02 min

Lab File: BF106808.D

Acq: 26 Jun 2018 8:10


Tgt Ion:240 Resp: 117423

Ion Ratio Lower Upper

240 100

120 10.1 9.5 14.3


236 25.7 20.7 31.1

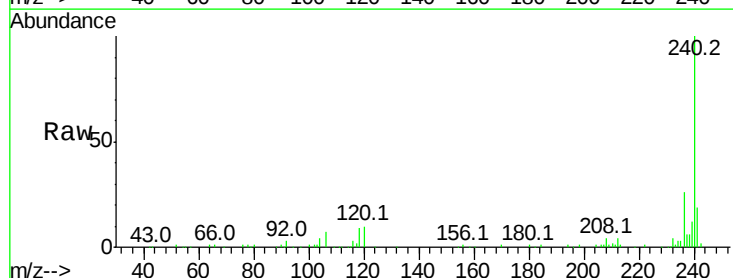


Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

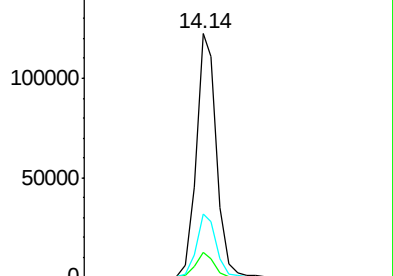

Time-->

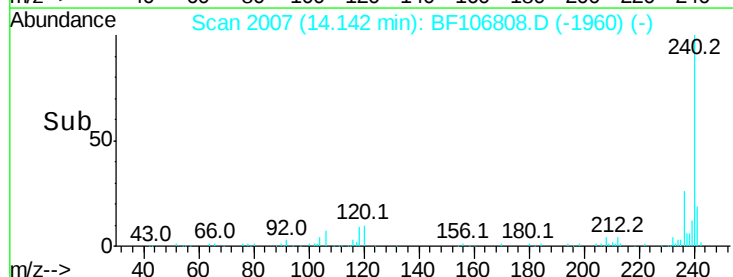

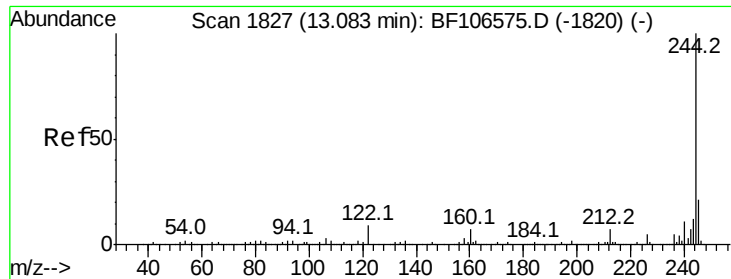

#78

Terphenyl-d14

Concen: 93.792 ng

RT: 13.08 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BF106808.D

Acq: 26 Jun 2018 8:10

Instrument :

BNA_F

ClientSampleId :

062118-DBRI-E-U-S


Tot Ion:244 Resp: 454663

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 8.9 11.0 16.4#

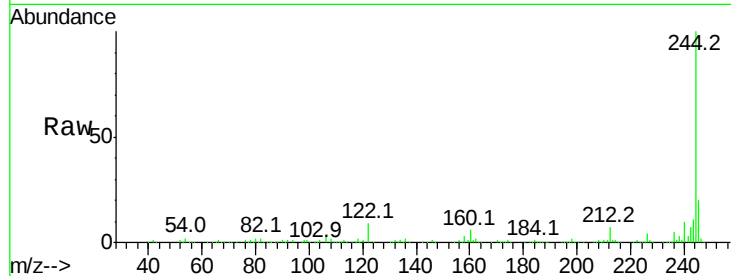

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

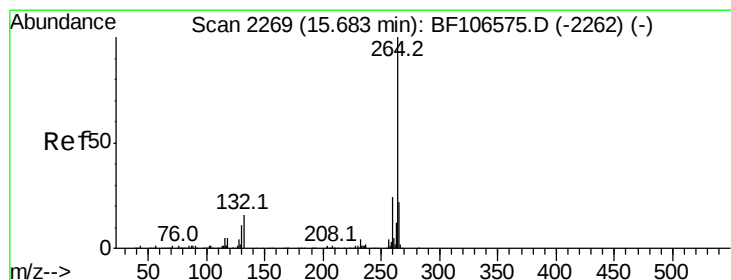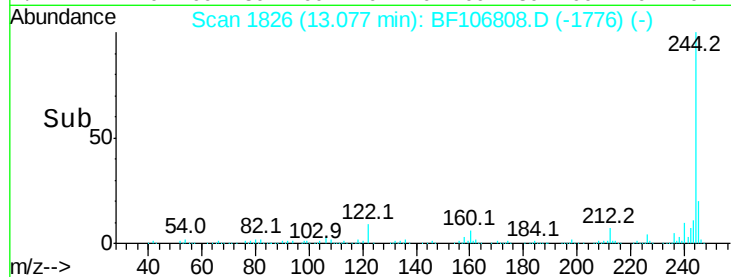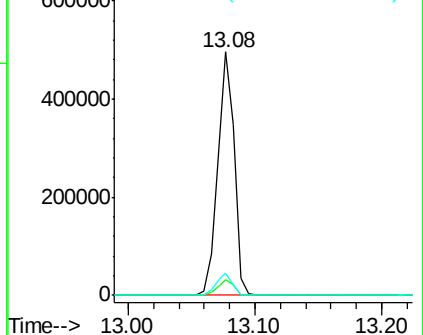

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.68 min Scan# 2269

Delta R.T. -0.04 min

Lab File: BF106808.D

Acq: 26 Jun 2018 8:10


Tgt Ion:264 Resp: 78457

Ion Ratio Lower Upper

264 100

260 22.7 19.2 28.8

265 20.9 17.5 26.3

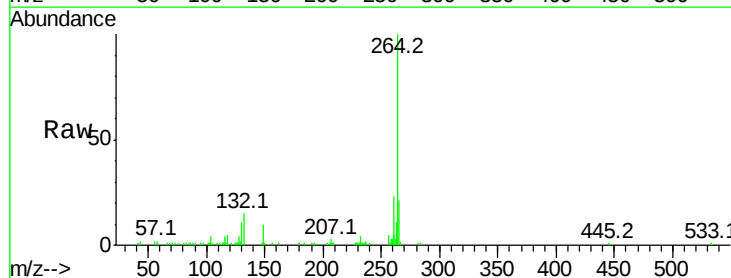

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

