
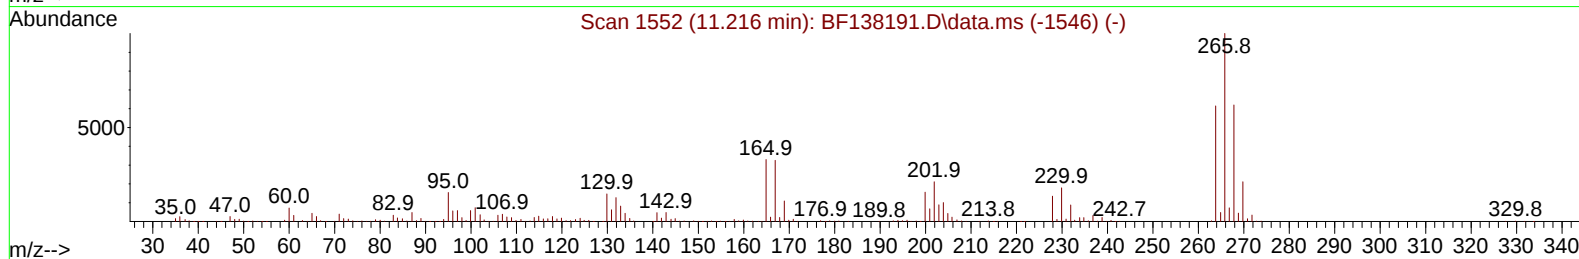
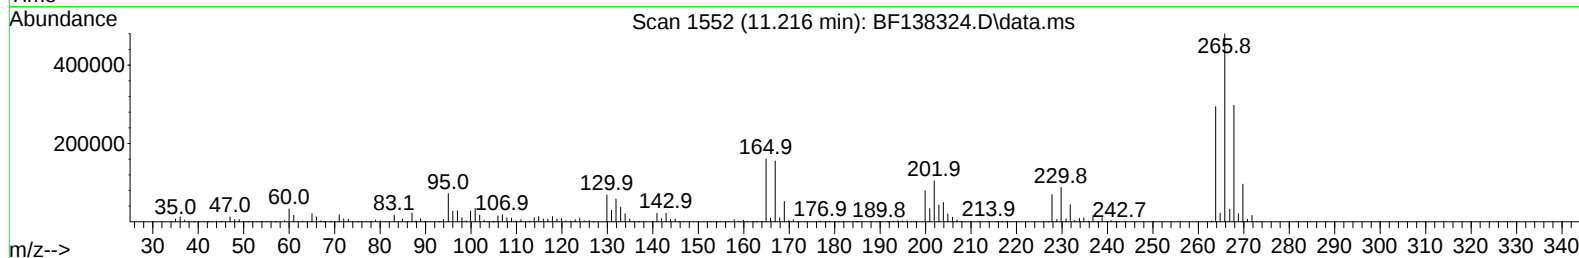


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062524\
Data File : BF138324.D
Acq On : 25 Jun 2024 09:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 11:41:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

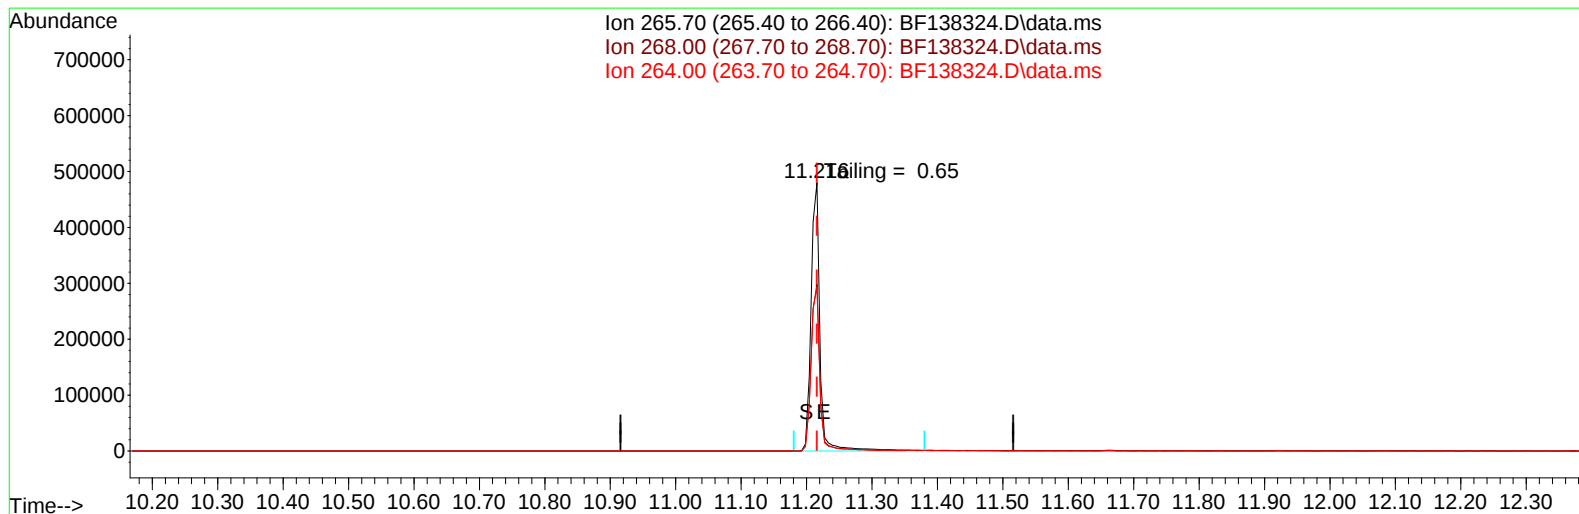

TIC: BF138324.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 121996.96 ng

response 455648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.01
264.00	61.50	61.18
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062524\  
Data File : BF138324.D  
Acq On    : 25 Jun 2024  09:48  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 25 11:41:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

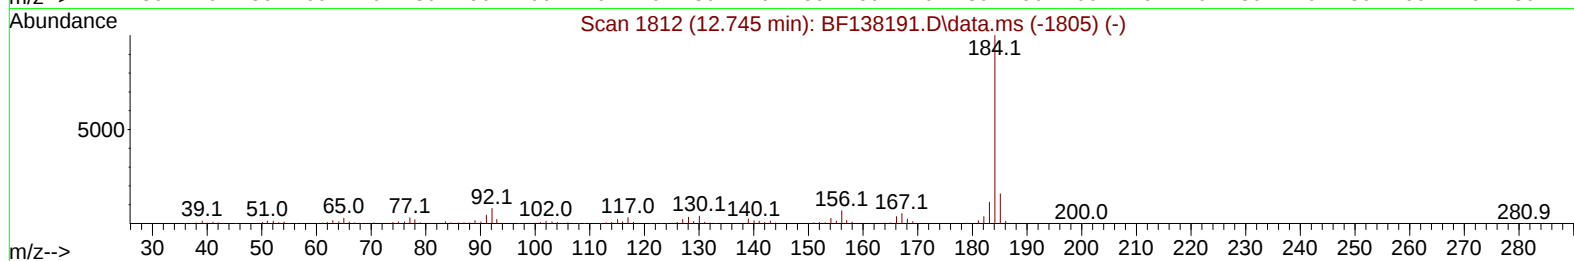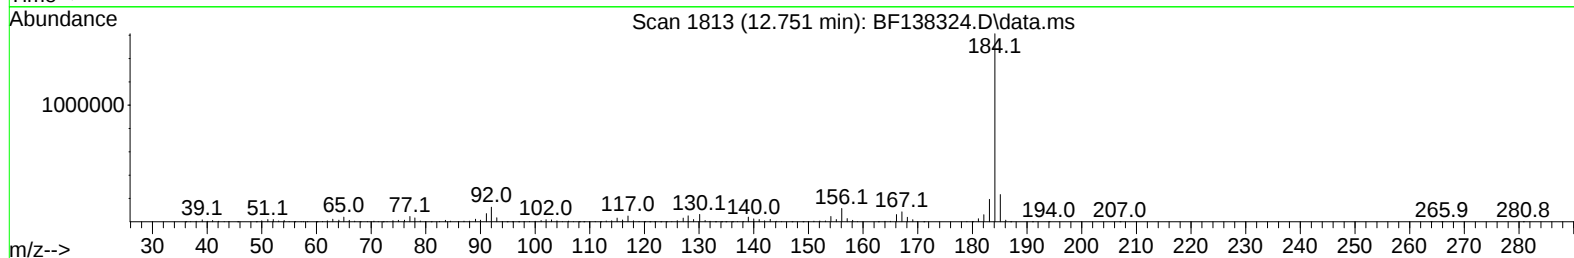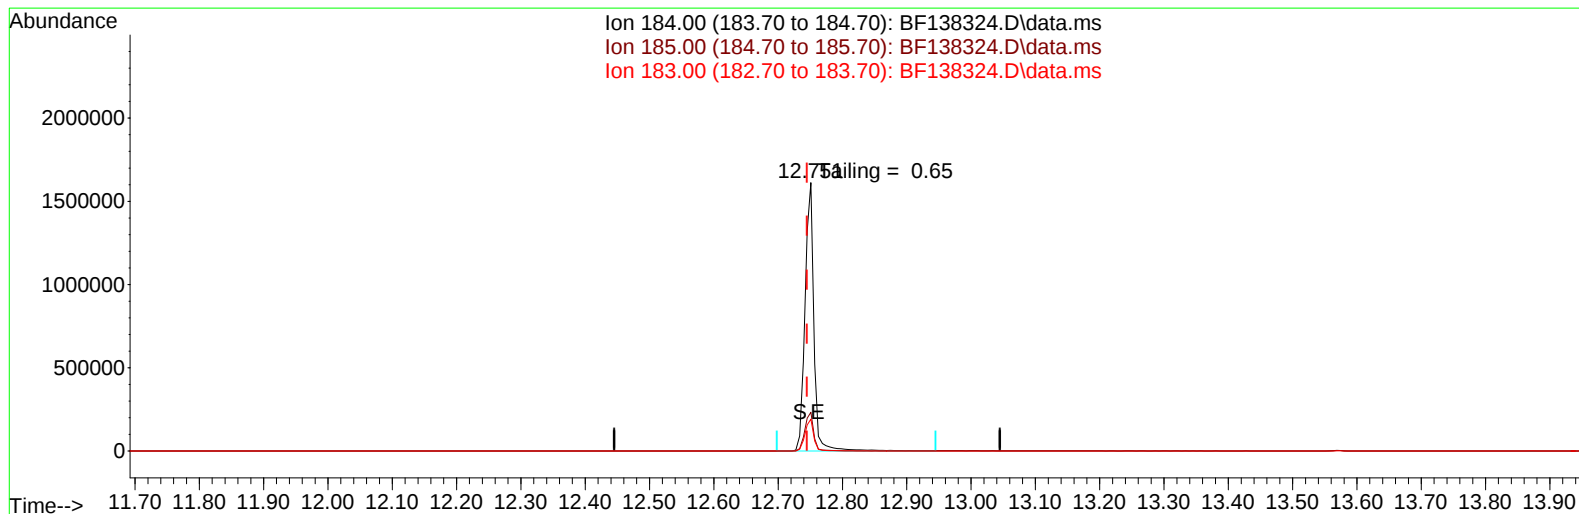

TIC: BF138324.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 1167444.36 ng

response **1566405**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.80	14.45
--------	-------	-------

183.00	11.30	11.89
--------	-------	-------

0.00 0.00 0.00