


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062524\
Data File : BF138324.D
Acq On : 25 Jun 2024 09:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

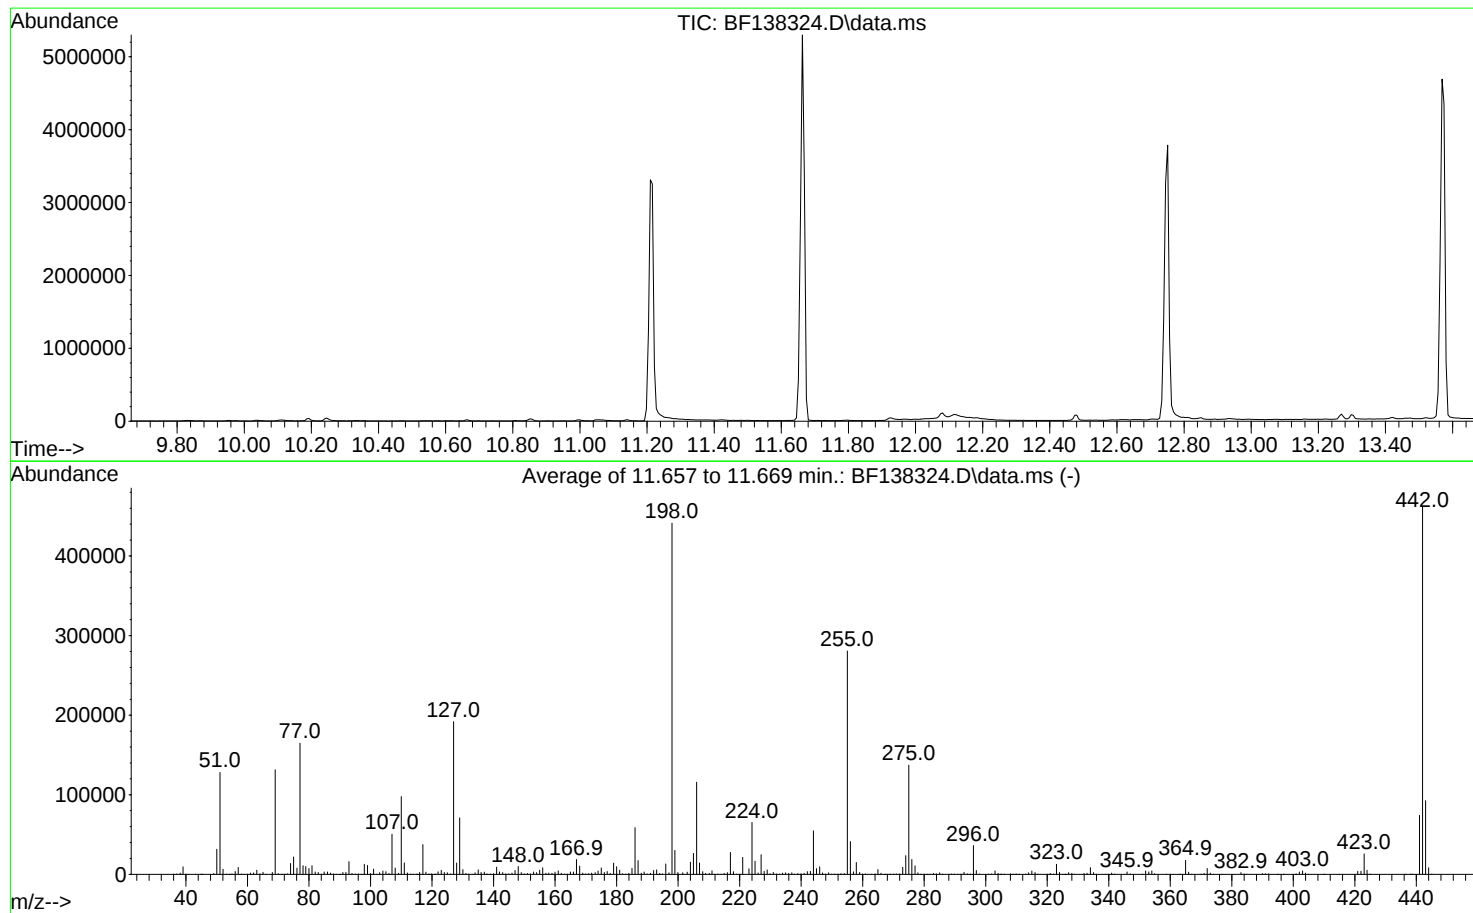




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	128081	PASS
68	69	0.00	2	1.8	2369	PASS
69	198	0.00	100	29.8	131485	PASS
70	69	0.00	2	0.7	918	PASS
127	198	10	80	43.5	191872	PASS
197	198	0.00	2	0.4	1971	PASS
198	198	100	100	100.0	441365	PASS
199	198	5	9	6.8	30091	PASS
275	198	10	60	31.1	137251	PASS
365	198	1	100	4.0	17699	PASS
441	198	0.01	100	16.8	74136	PASS
442	442	50	100	100.0	462208	PASS
443	442	15	24	20.1	92691	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062524\
Data File : BF138324.D
Acq On : 25 Jun 2024 09:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 11:41:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

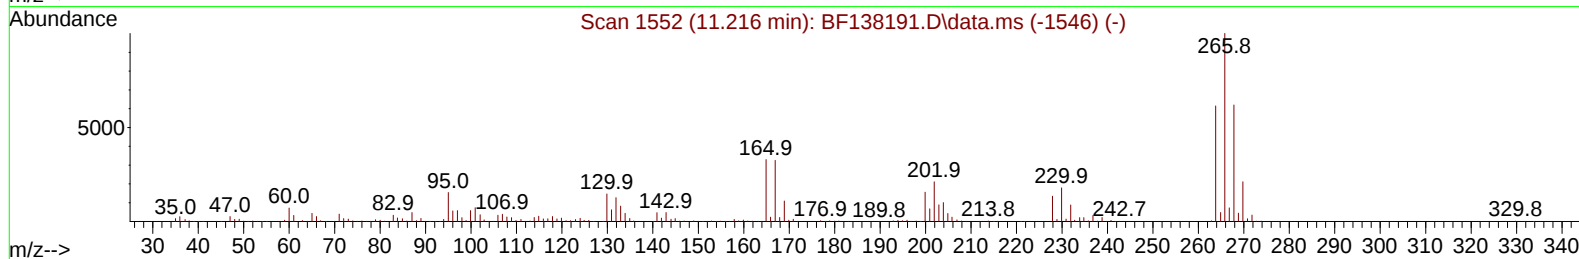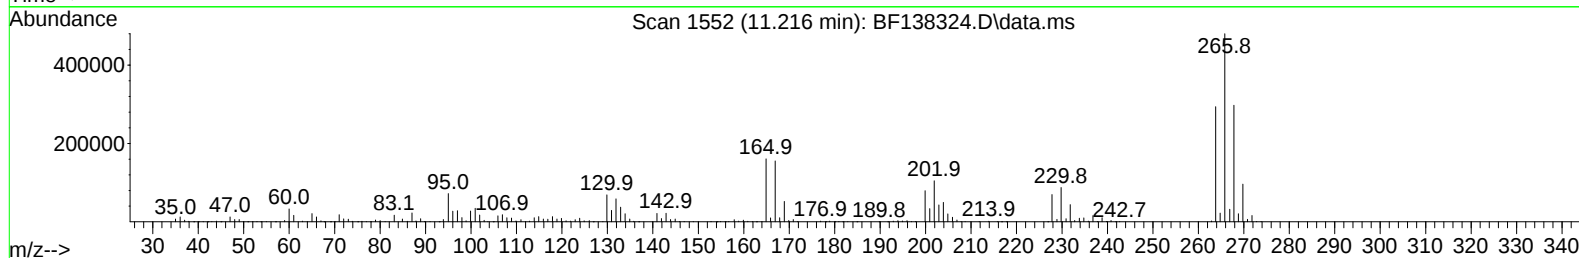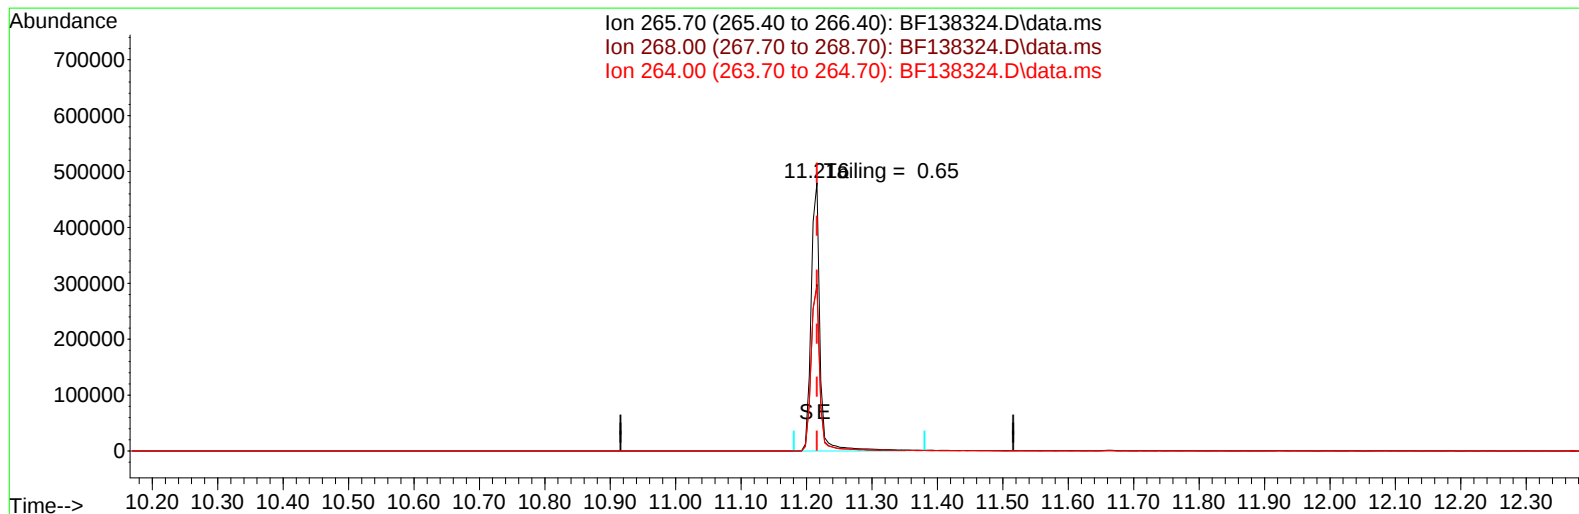

TIC: BF138324.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 121996.96 ng

response 455648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.01
264.00	61.50	61.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/25/2024	BNA_F	<u>BF138324.D</u>
Compound Name	Response	Retention Time
DDT	901338	13.574
DDD	21737	13.269
DDE	3458	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25195	926533	2.72

Instrument :
BNA_F
ClientSampleId :
DFTPP