
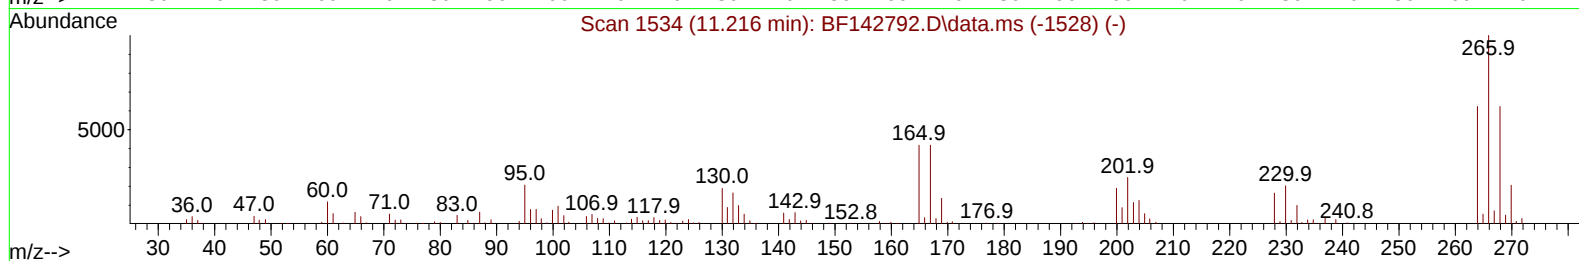
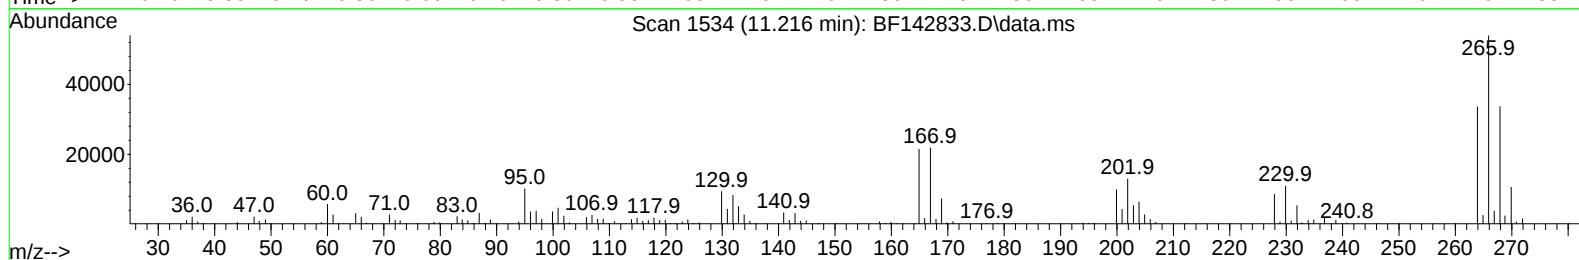


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062525\
Data File : BF142833.D
Acq On : 25 Jun 2025 12:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 13:51:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

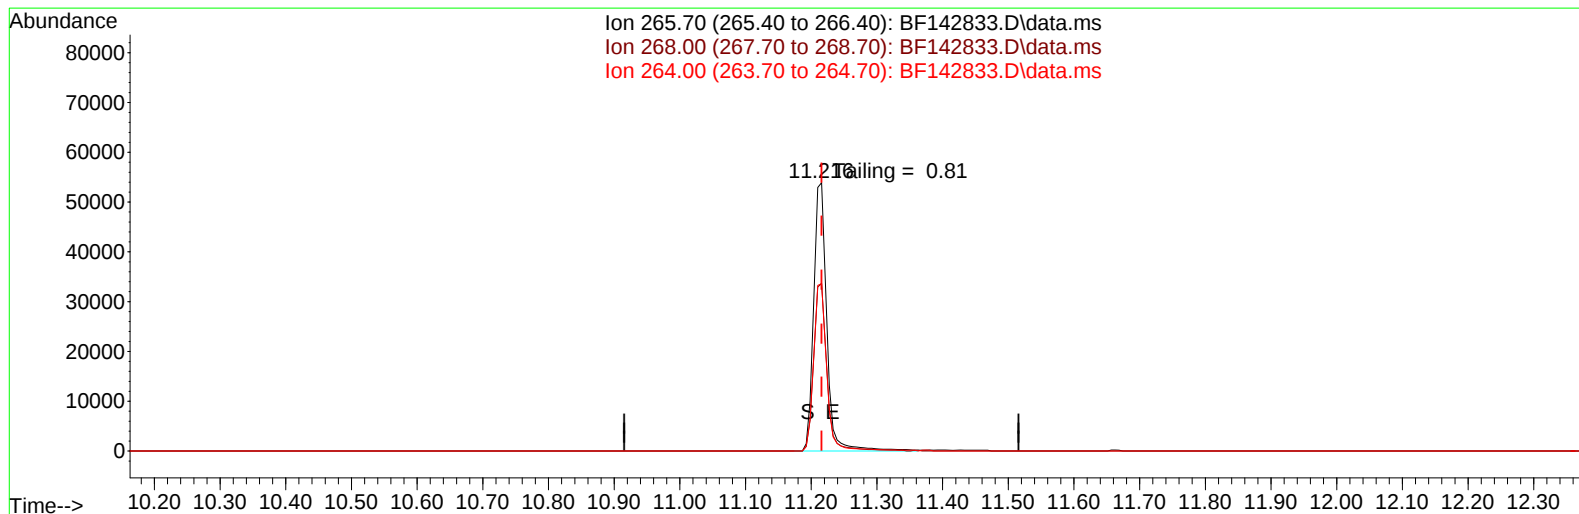

TIC: BF142833.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.000) 32756.87 ng

response 75756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.42
264.00	62.40	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062525\
Data File : BF142833.D
Acq On : 25 Jun 2025 12:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 13:51:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

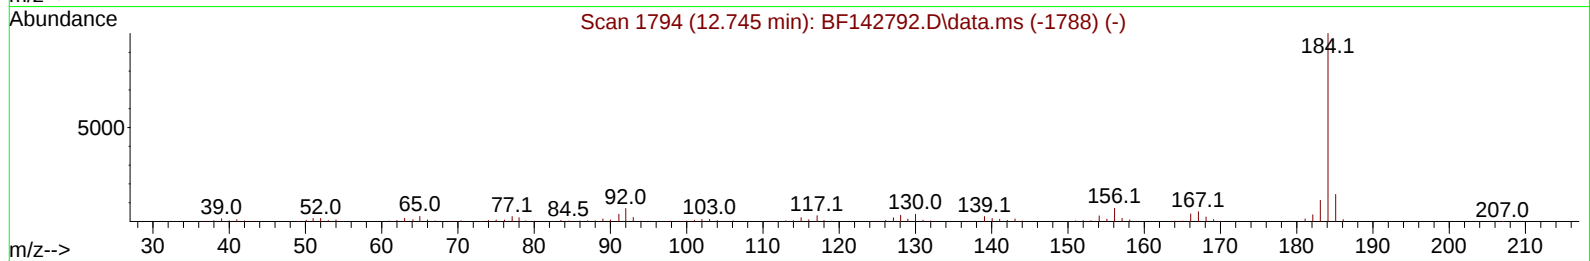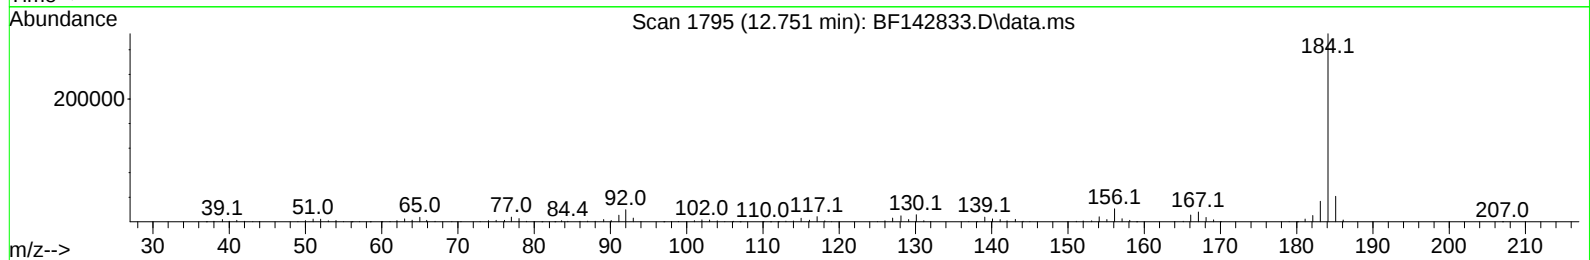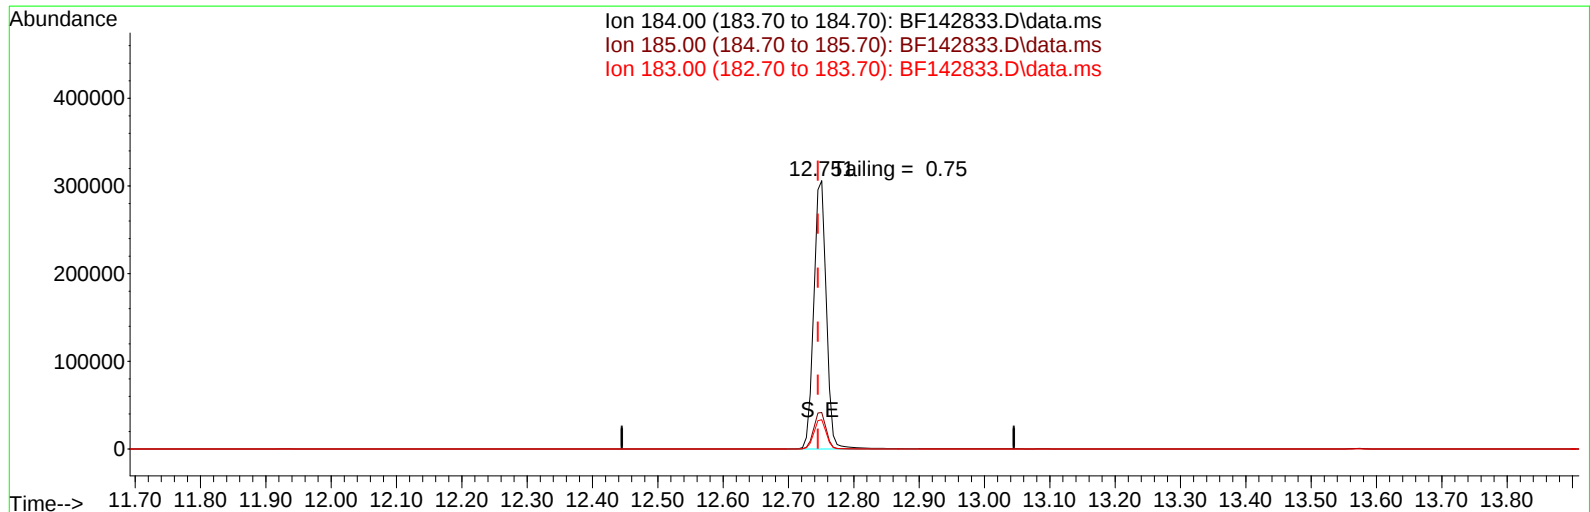

TIC: BF142833.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 410200

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.59
183.00	11.20	10.93
0.00	0.00	0.00