
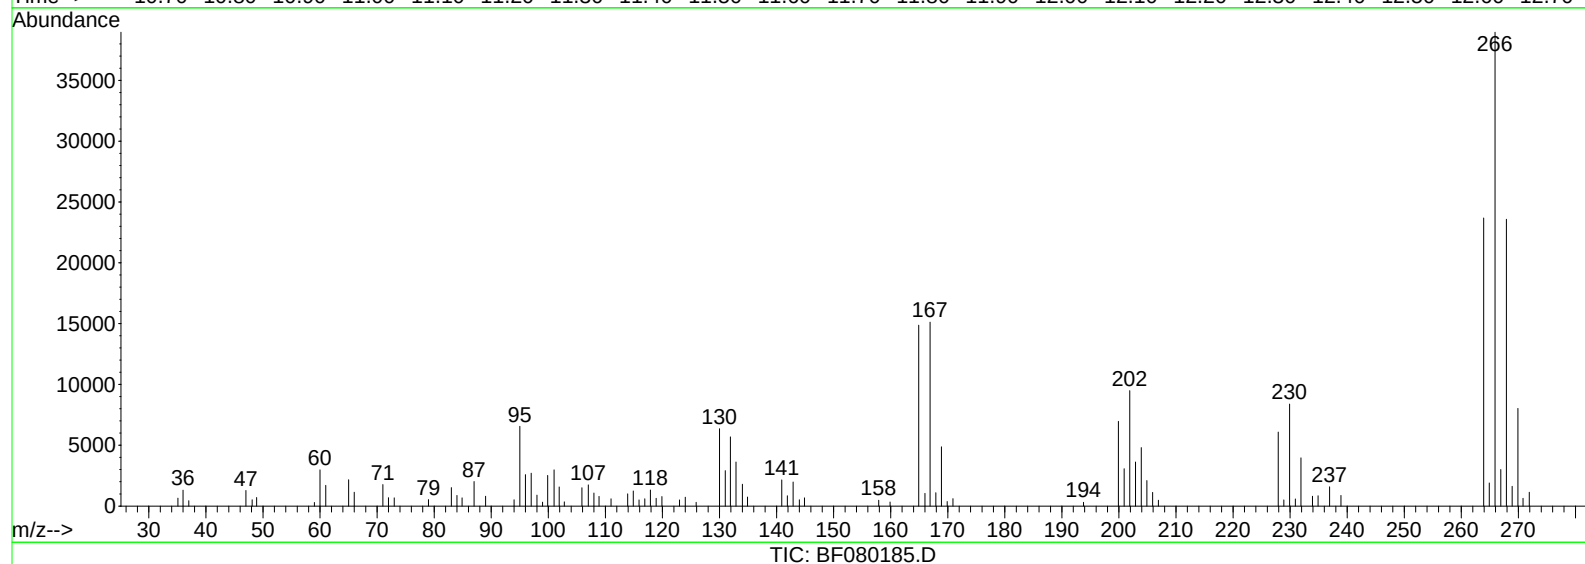


Data Path : Z:\HPCHEM1\BNA F\Data\BF062615\
Data File : BF080185.D
Acq On : 26 Jun 2015 9:03
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 05:35:27 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

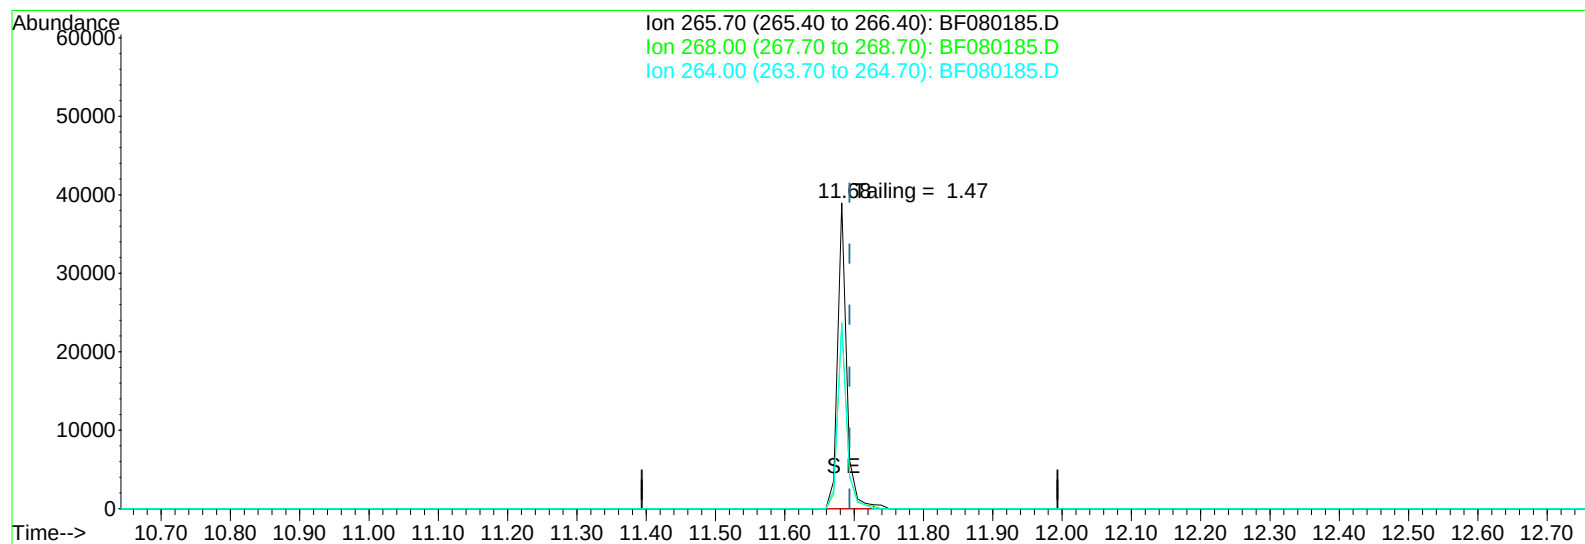

(69) Pentachlorophenol (C)



11.682min (-0.011) 0.00ng

response 35361

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	60.53
264.00	62.70	60.80
0.00	0.00	0.00

```
Data Path   : Z:\HPCHEM1\BNA F\Data\BF062615\  
Data File  : BF080185.D  
Acq On     : 26 Jun 2015    9:03  
Operator   : TP/IZ  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1    Sample Multiplier: 1
```

Quant Time: Jun 27 05:35:27 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

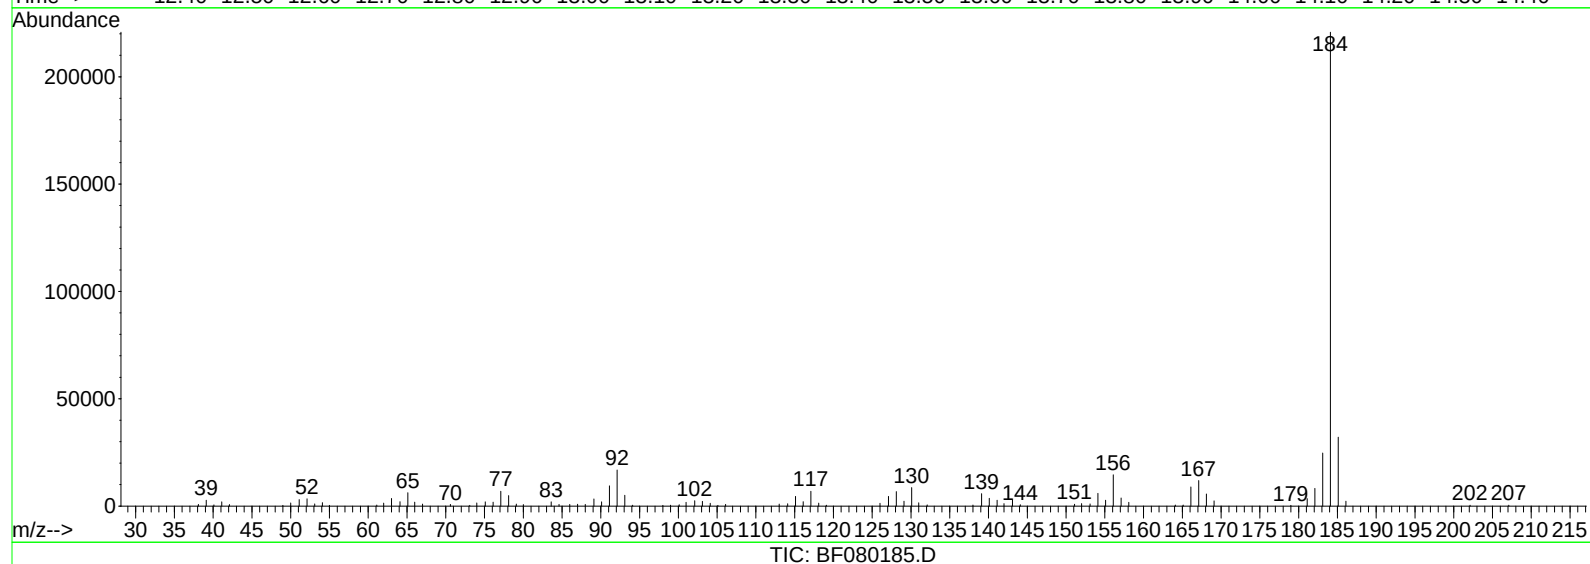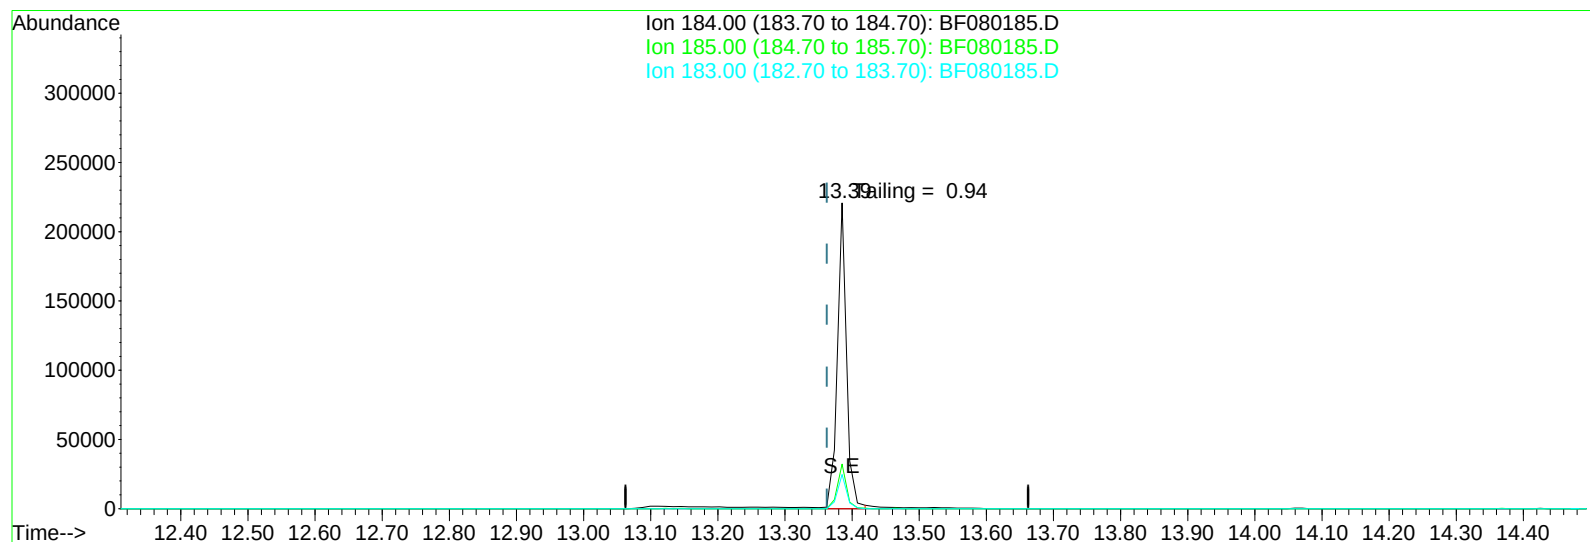

(76) Benzidine

13.385min (+0.023) 3494.41ng

response 208344

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.55
183.00	9.50	11.18
0.00	0.00	0.00